

# **BRS**

## **BioResorbable Scaffold**

# **BRS**

## **BioResorbable Scaffold**

# Revolution in PCI

## ADVANCEMENTS IN THE TREATMENT OF HEART DISEASE

1977

BALLOON ANGIOPLASTY



1988



BARE METAL STENT

2001

DRUG ELUTING STENT




TODAY


DISSOLVING STENT  
— ABBOTT'S ABSORB™

# *Disappear !*

## *Human Imaging at 5 Year*

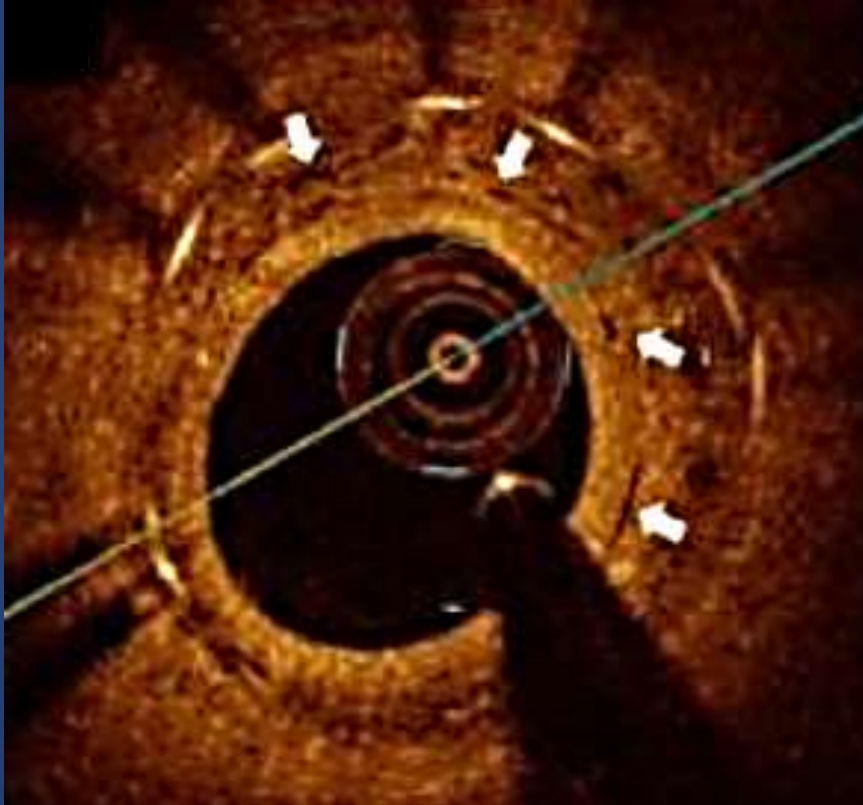


Metallic DES

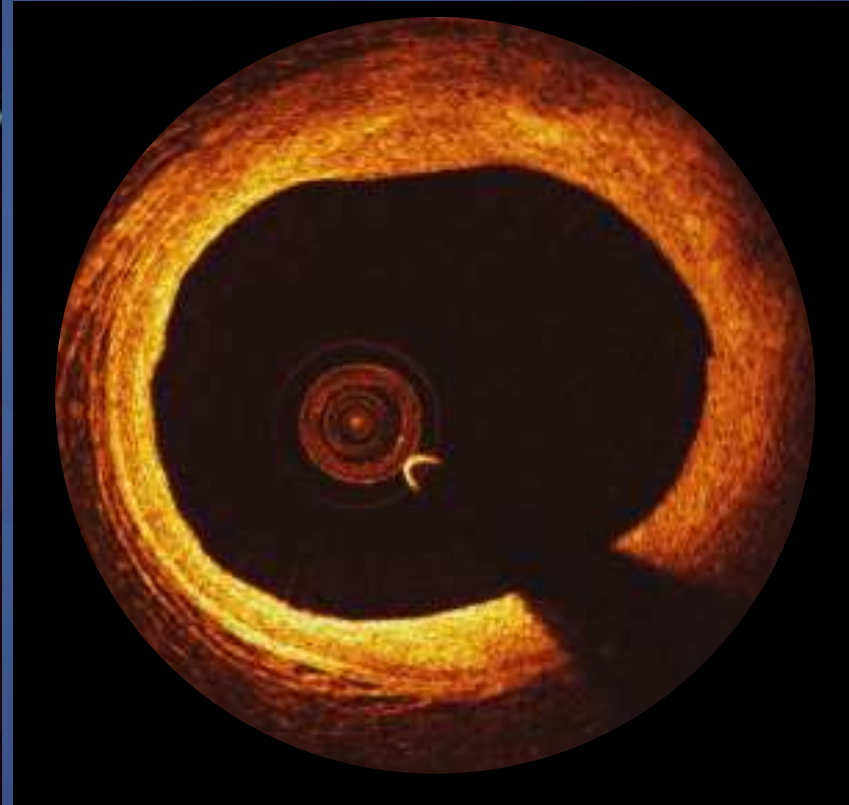


BVS



# *Plaque Stabilization and Lumen Enlargement*

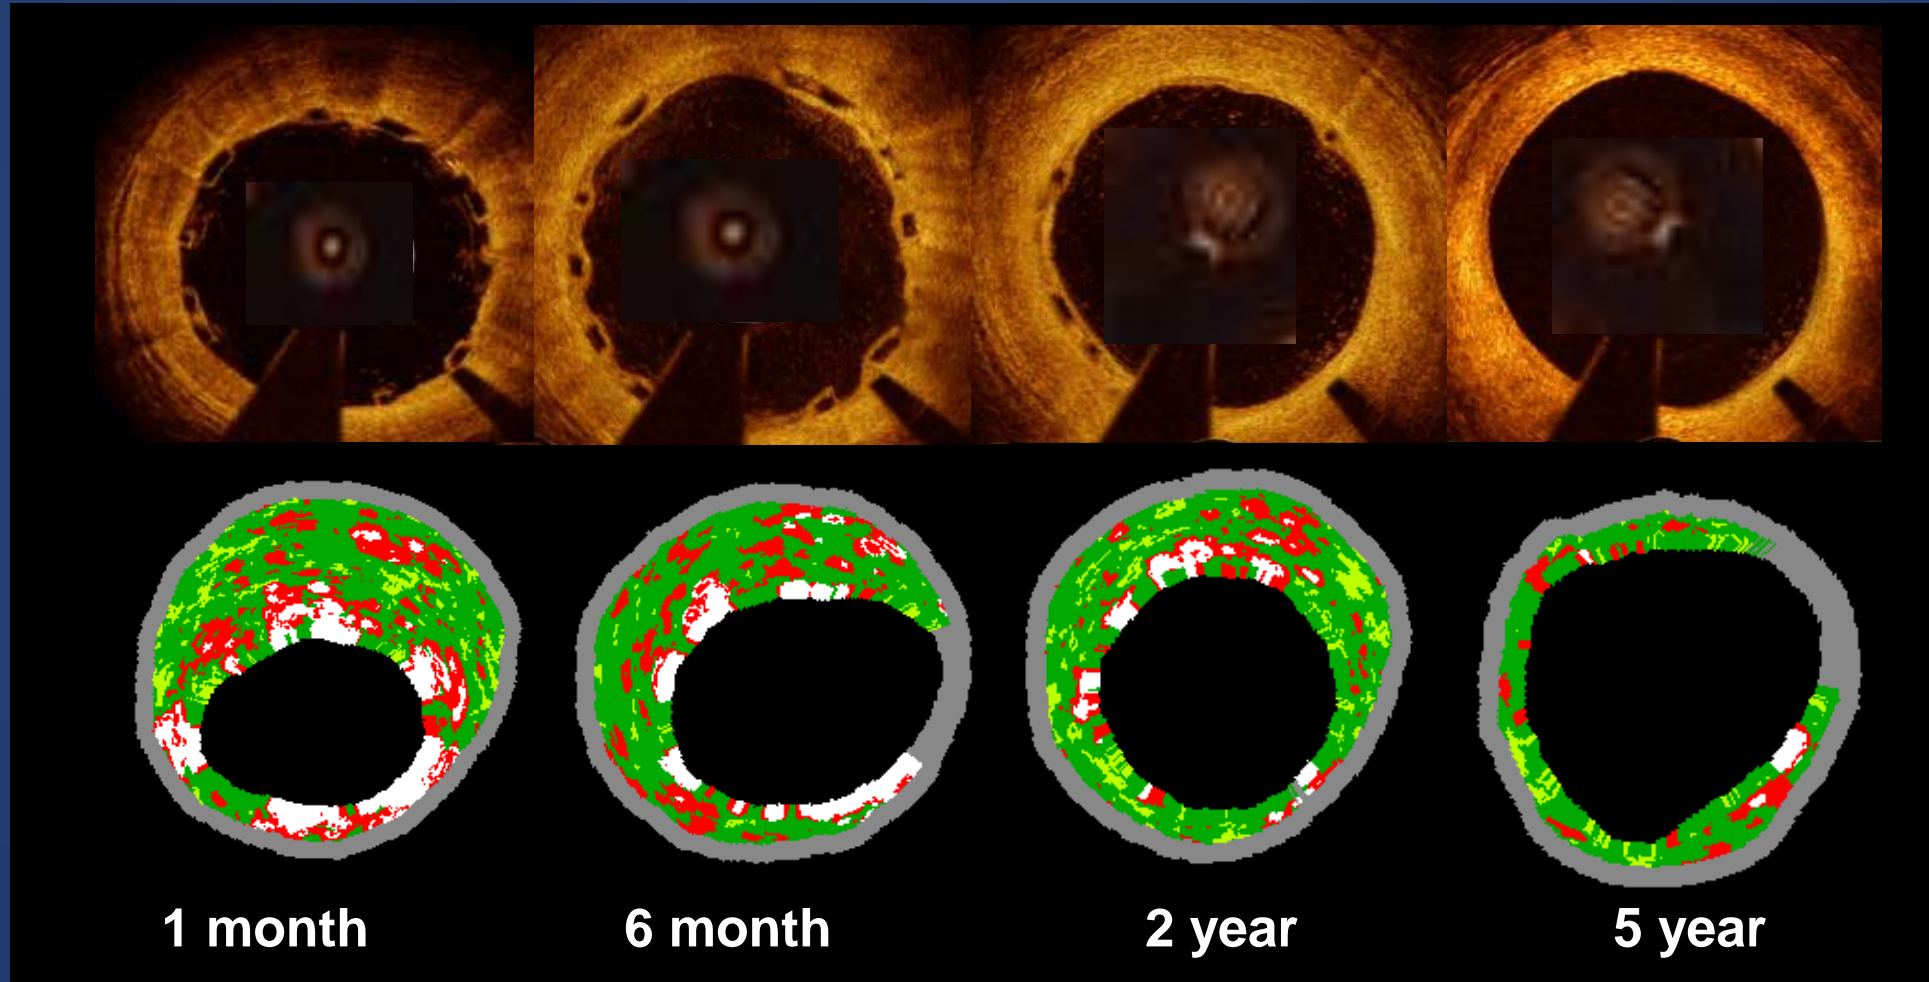

# BRS Design Considerations

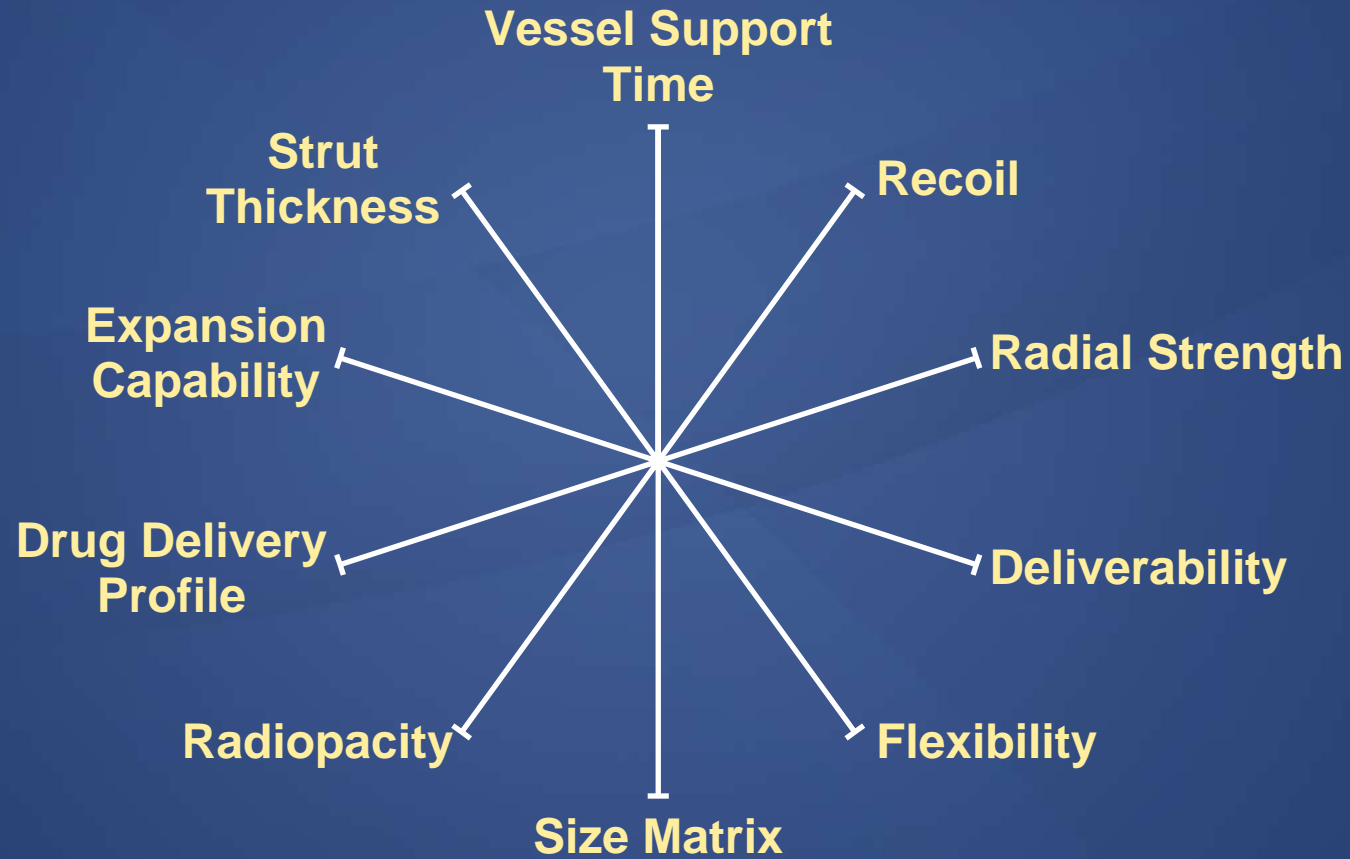

# Design and Structure of Clinically Tested BRS

Scaffold (manufacturer)	Strut material	Coating material	Eluted drug	Radial support	Resorption (months)
Metallic					
AMS-1 (Biotronik)	Mg alloy	None	None	Weeks	<4
DREAMS-1 (Biotronik)	Mg alloy with some rare metals	PLGA	Paclitaxel	3–6 months	9
DREAMS-2 (Biotronik)	Mg alloy with some rare metals	PLLA	Sirolimus	3–6 months	9
Polymeric					
Igaki-Tamai (Kyoto Medical)	PLLA	None	None	6 months	24–36
BVS 1.0 (Abbott Vascular)	PLLA	PDLLA	Everolimus	Weeks	18–24
BVS 1.1 (Abbott Vascular)	PLLA	PDLLA	Everolimus	6 months	24–48
DESolve (Elixir)	PLLA	None	Myolimus	N/A	12–24
REVA (Reva Medical)	PTD-PC	None	None	3–6 months	24
ReZolve (Reva Medical)	PTD-PC	None	Sirolimus	4–6 months	4–6
ReZolve2 (Reva Medical)		None	Sirolimus		
ART 18AZ (ART)	PDLLA	None	None	3–6 months	3–6
Fortitude (Amaranth)	PLLA	None	None	3–6 months	3–6
IDEAL BTI (Xenogenics)	Poly lactide and salicylates	SA/AA	Sirolimus	3 months	6–9

# Design of BRSs in Clinical or Preclinical use

Company / Device	Design of the bioresorbable device	Strut thickness, ( $\mu$ m)	Polymer / Drug	Absorption time	Late loss, (mm)
Kyoto Medical / Igaki-Tamai		170	PLLA	2 years (y)	0.48 (6m)
Biotronik / DREAMS		125	Mg alloy (AMS-4) / sirolimus	4 to 6 months (m)	0.68 (6m)*
Abbott / ABSORB BVS		150	PLLA / everolimus	2y	0.19 (6m)
Reva Medical / ReSolve		200	Tyrosine poly carbonate with iodine / sirolimus abluminal	2y	1.81 (6m)
- / BTI		200	Salicylic acid into polymer (PLA or adipic acid) / sirolimus	6m	NA
Elixir / DESolve		150	PLLA / novolimus	1 to 2y	NA



# BRS System


## Bioresorbable Scaffold

- Poly (L-lactide) (PLLA)
- Based on proven MULTI-LINK pattern
- Naturally resorbed, fully metabolized\*



## Bioresorbable Coating

- Poly (D,L-lactide) (PDLLA)
- Naturally resorbed, fully metabolized

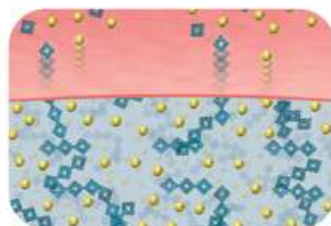

## Everolimus

- Similar dose density and release rate to XIENCE V





## XIENCE V Delivery System

- World-class deliverability



# Bioresorbable Polymer

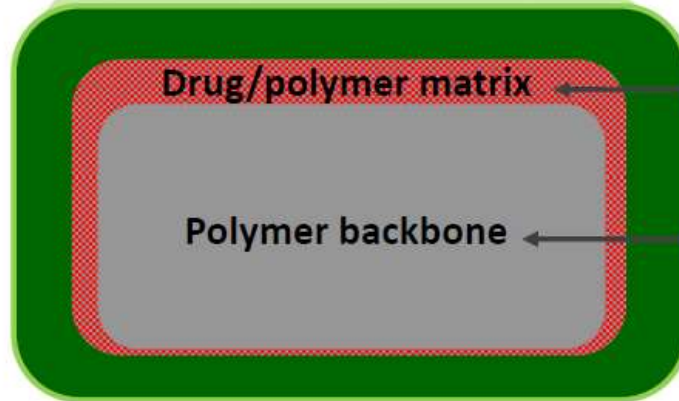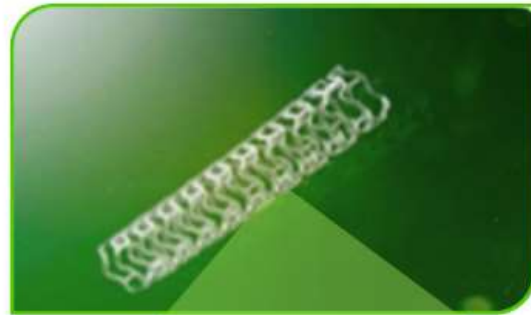

## Everolimus/PDLLA Matrix Coating


- Thin layer
- Amorphous (non-crystalline)
- 1:1 ratio of Everolimus/PDLLA matrix
- Conformal coating, 2-4  $\mu\text{m}$  thick
- Controlled drug release

## PLLA Scaffold


- Semi-crystalline
- Provides device structure
- Processed for required radial strength




# Poly-L-Lactic Acid (PLLA)

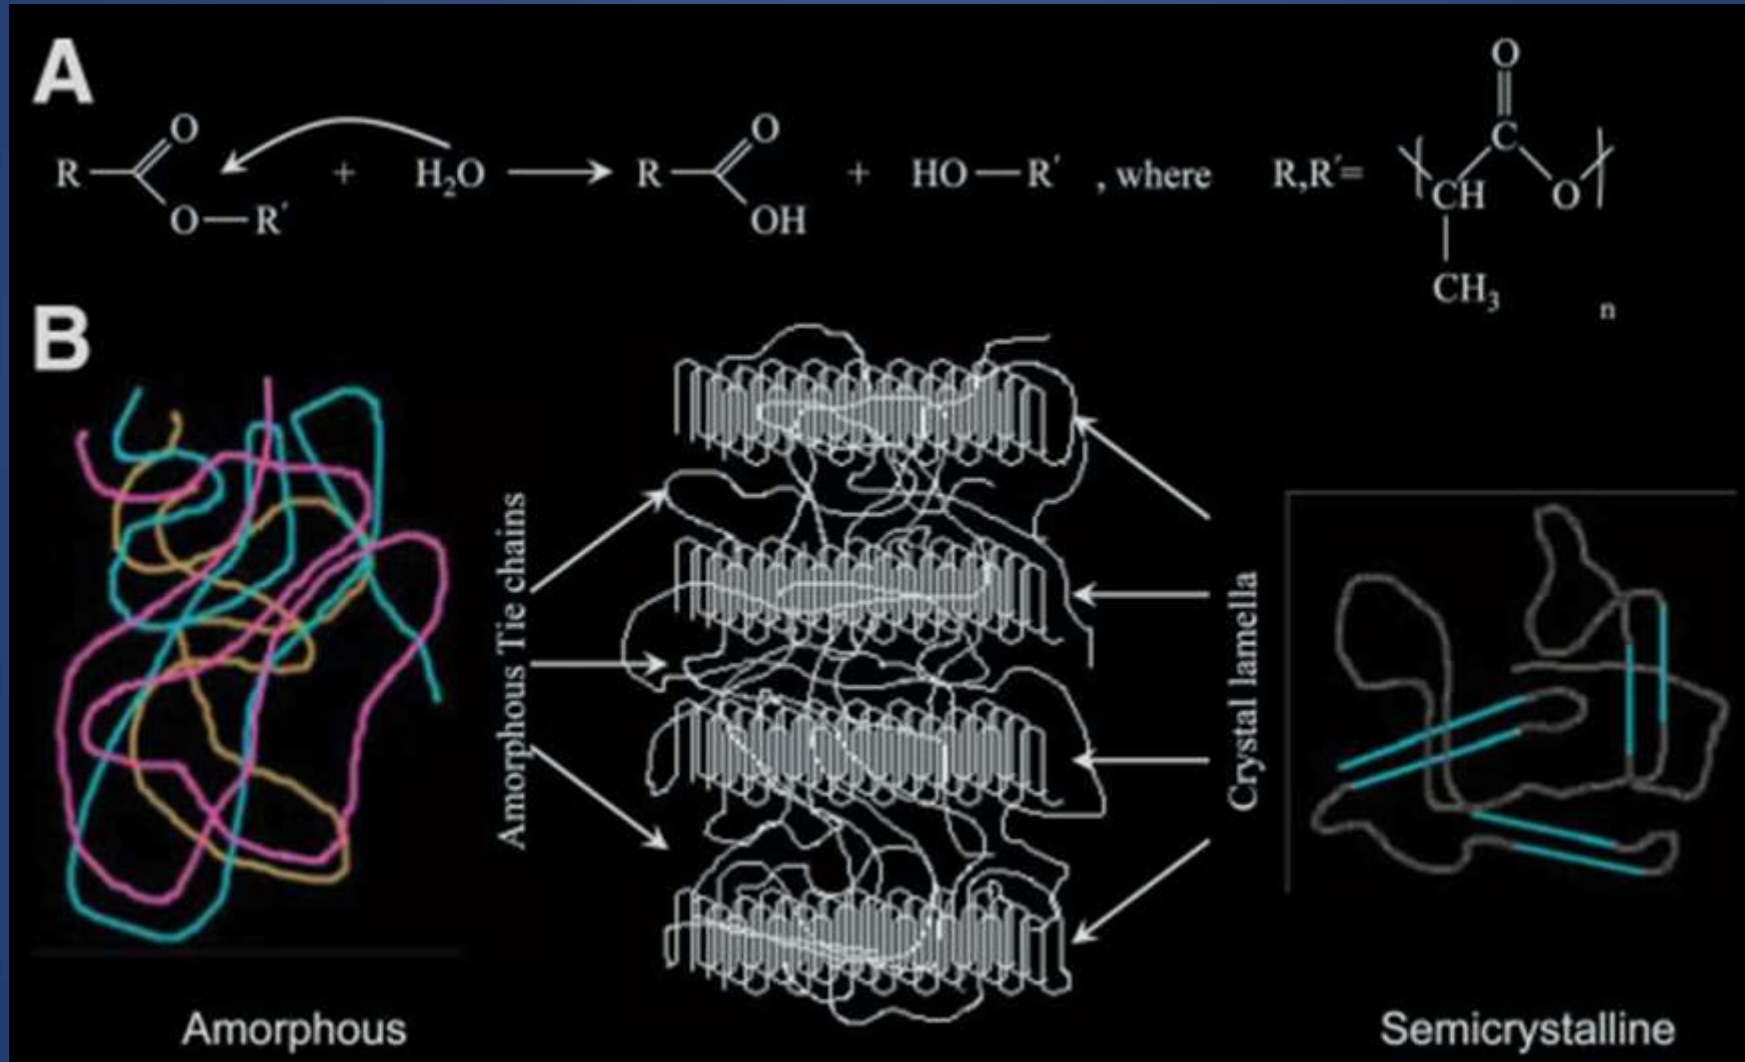

# Degradation of PLLA

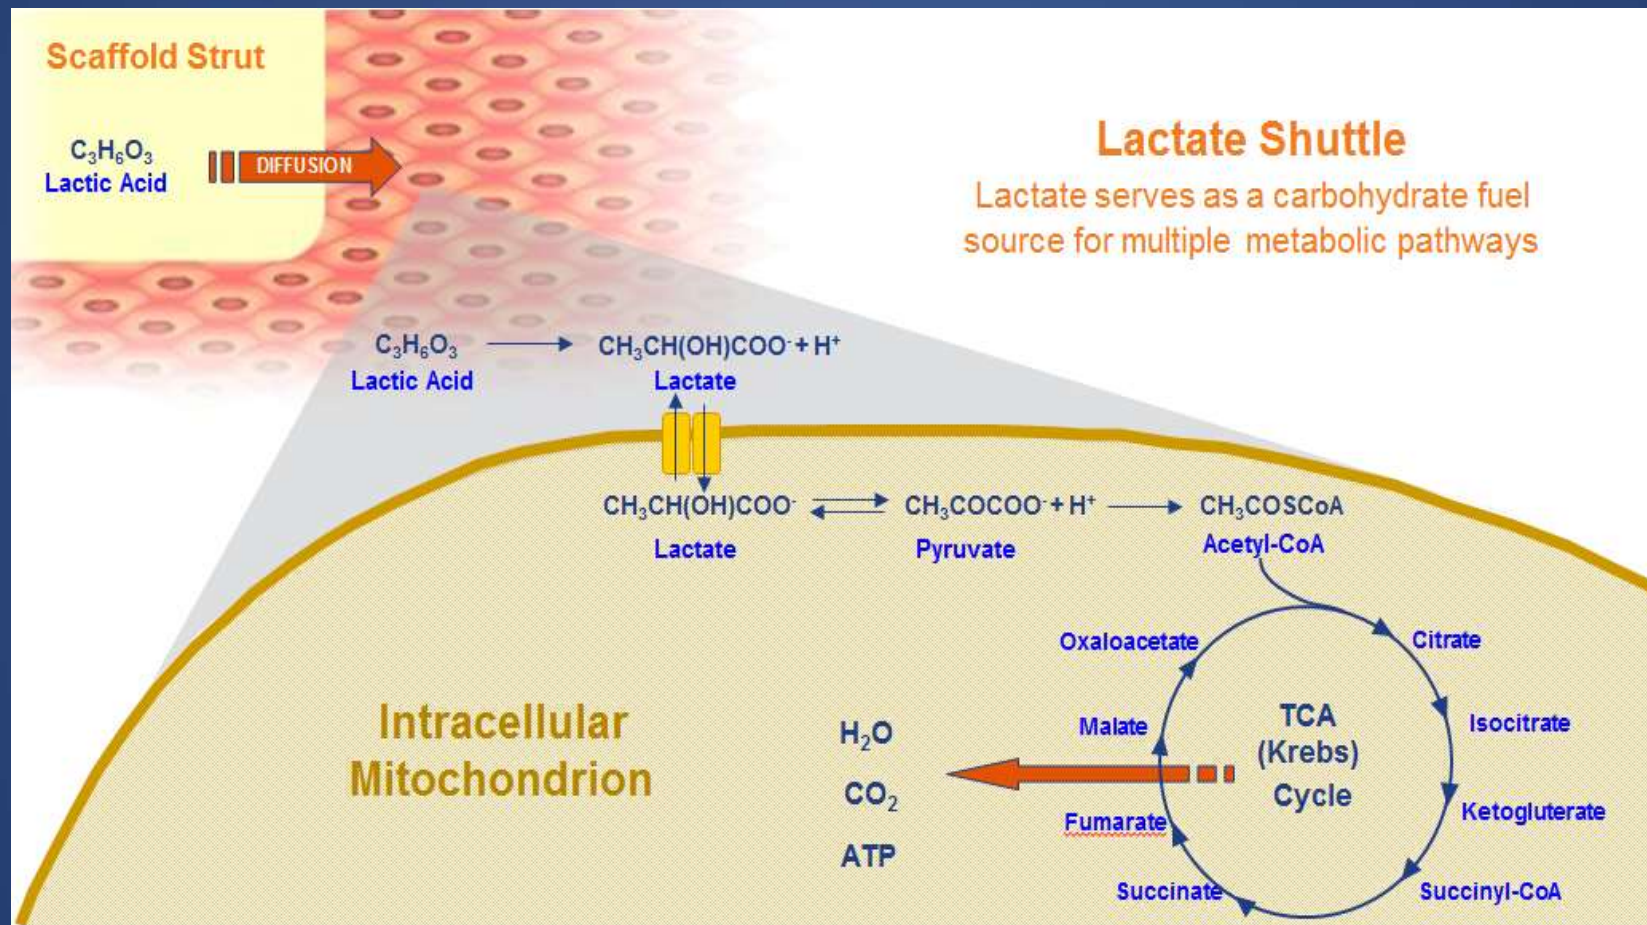


# Bioresorption of Metal scaffold

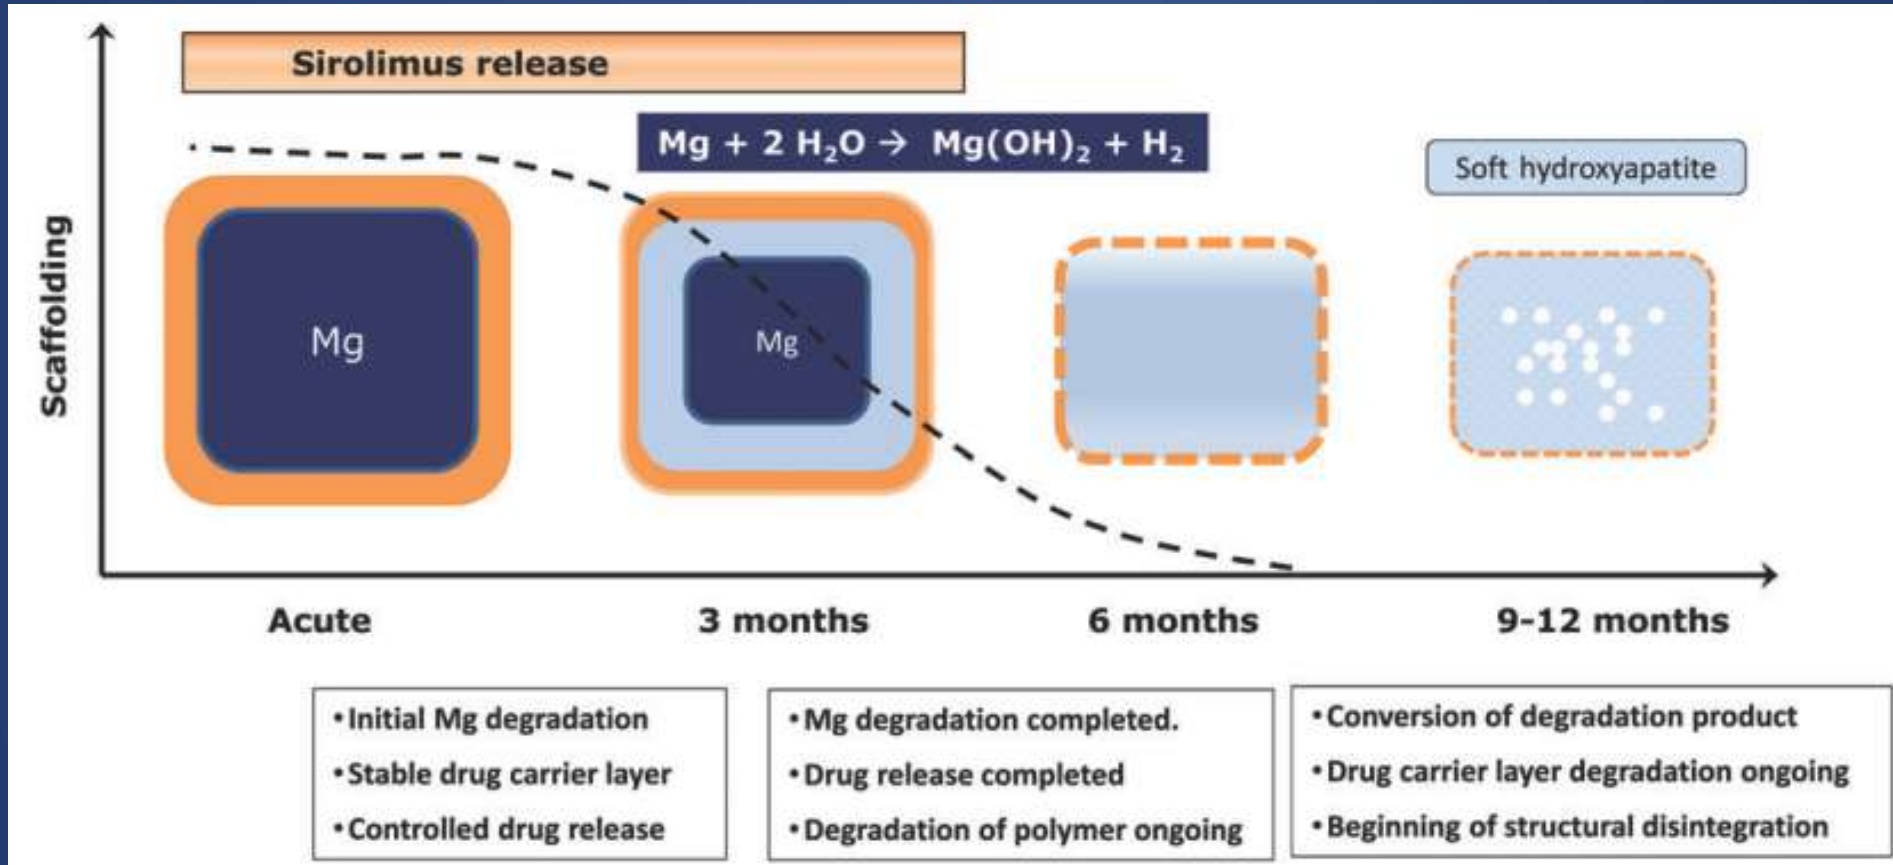




# Resorption: Vascular response

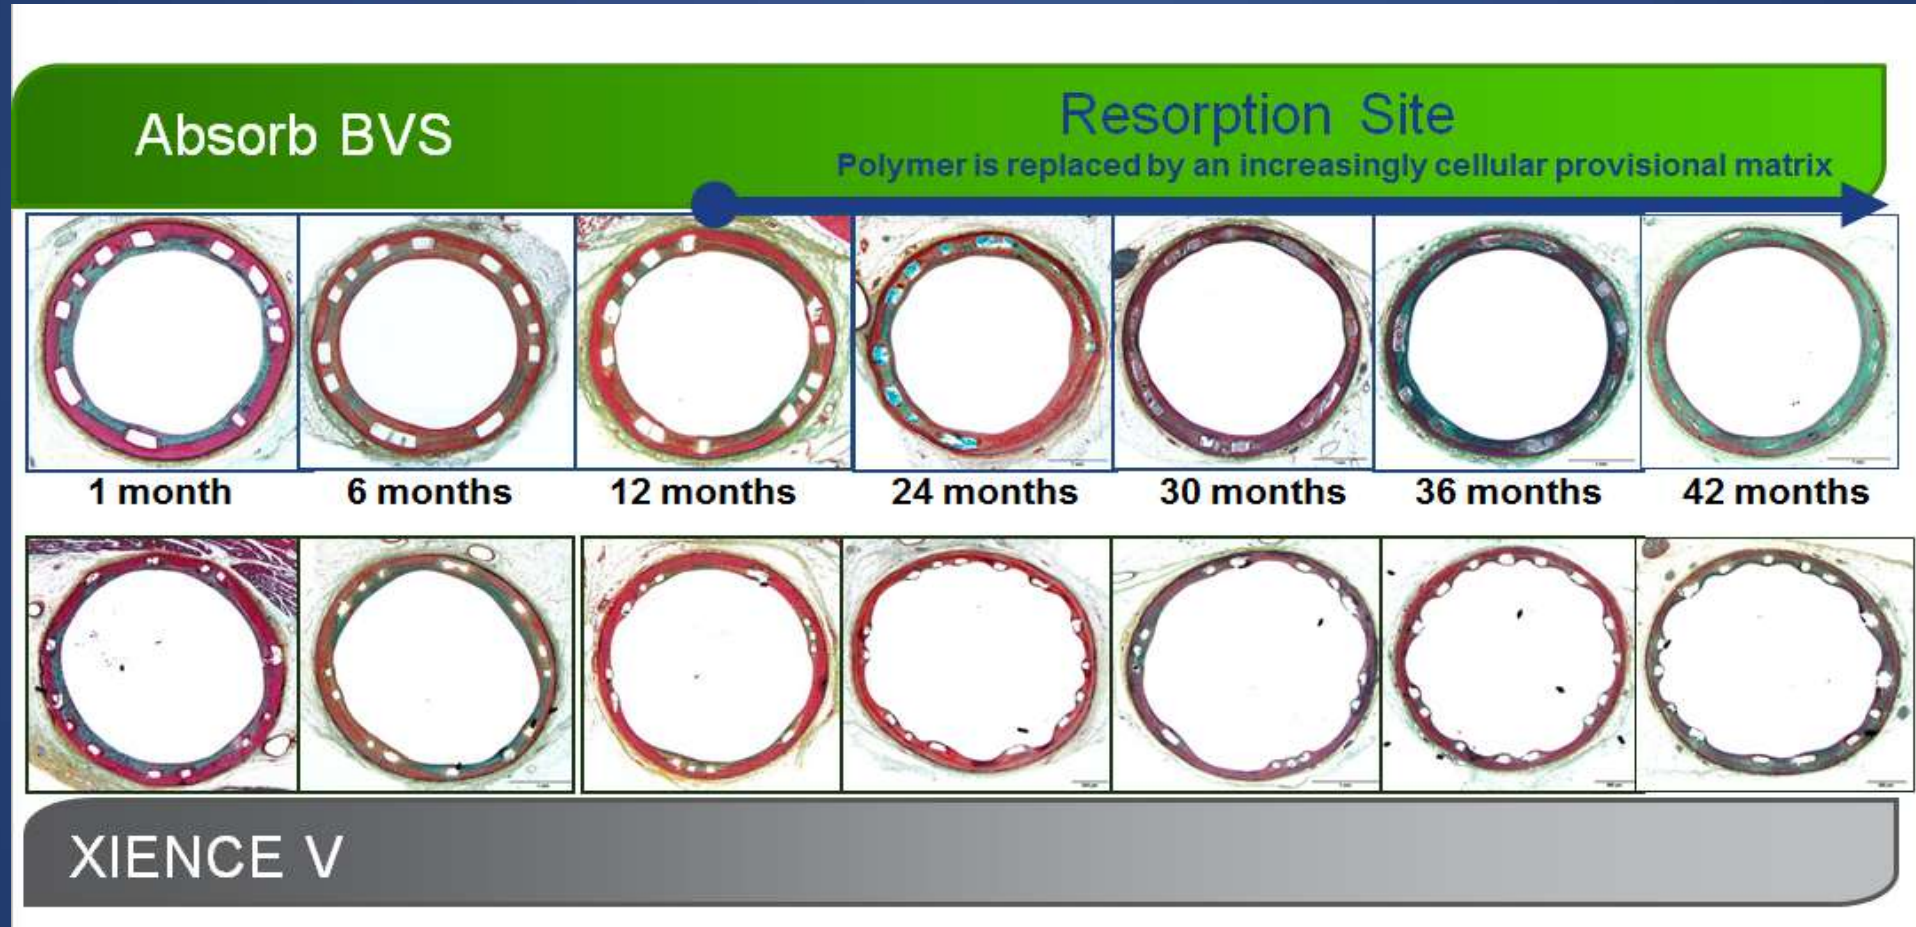


# Resorption: Vascular response

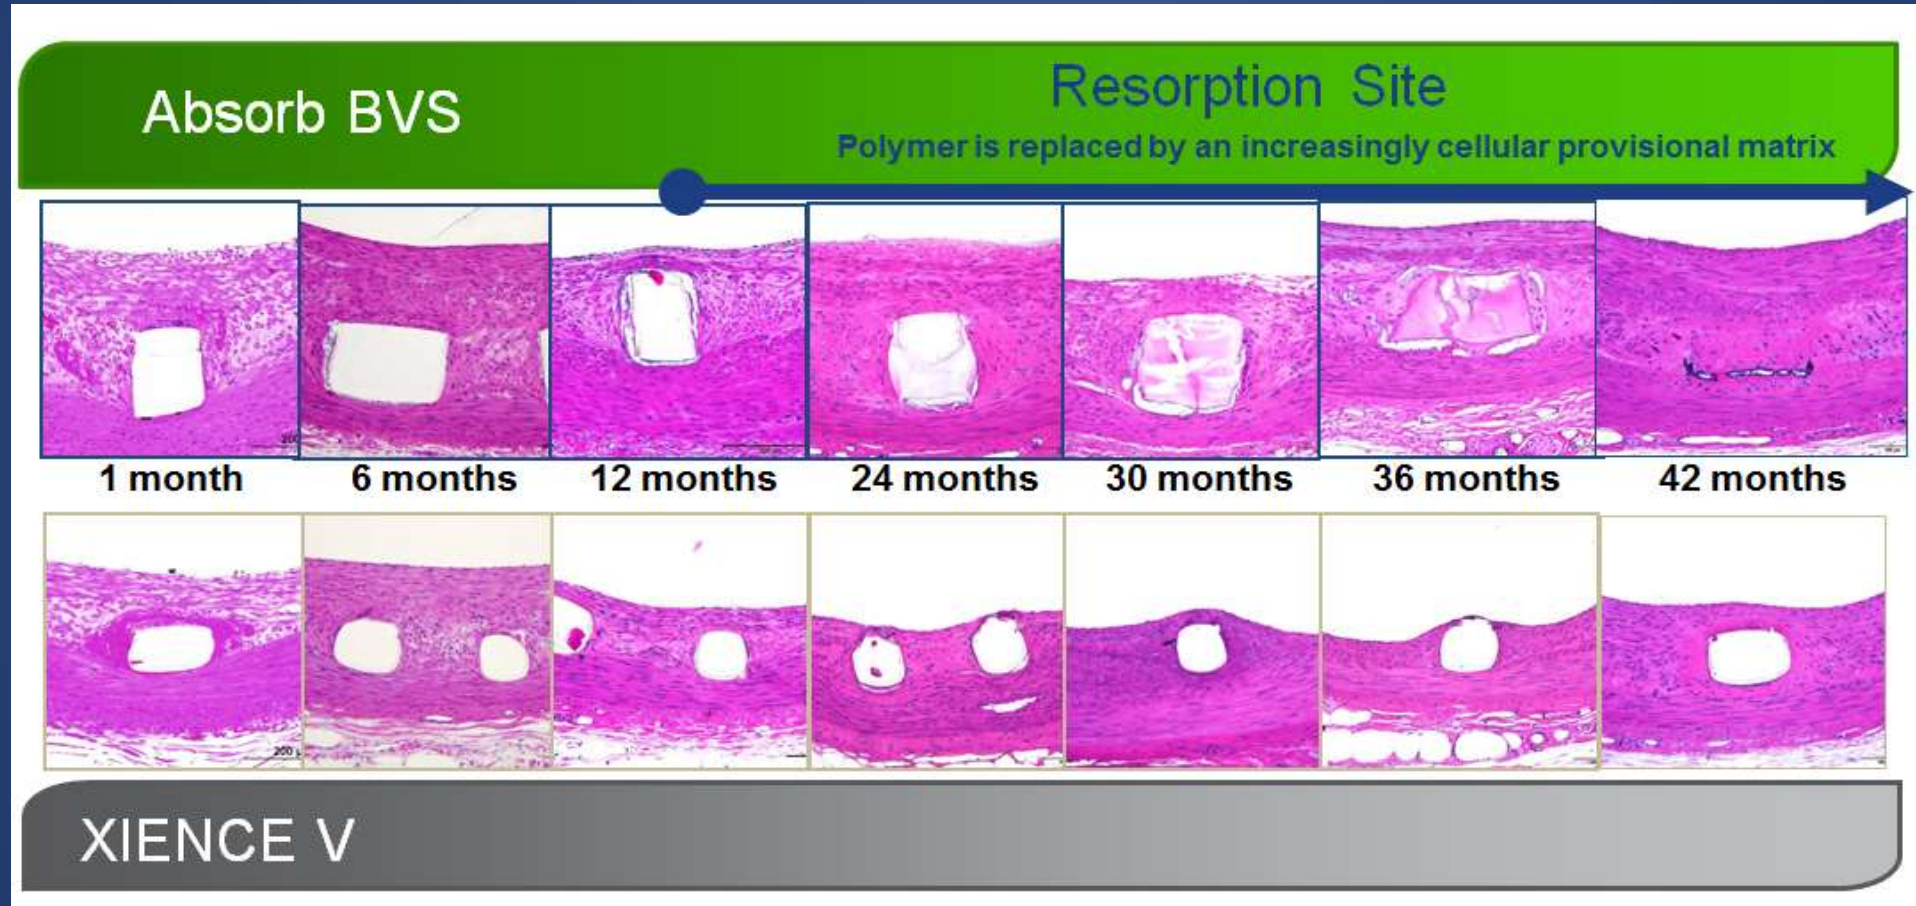





# Resorption: Vascular response

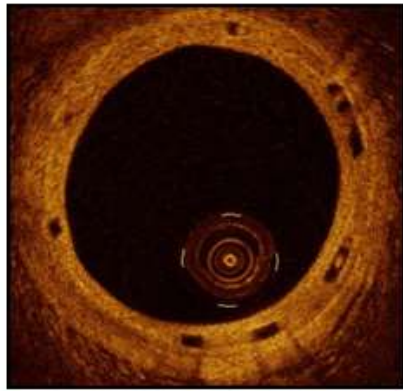


6 months

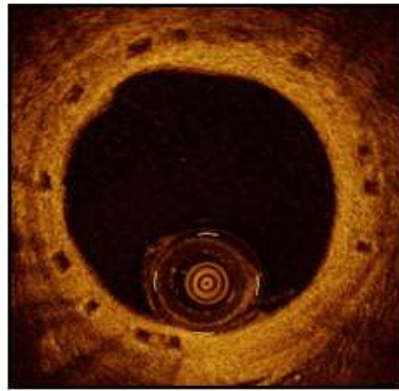




24 months

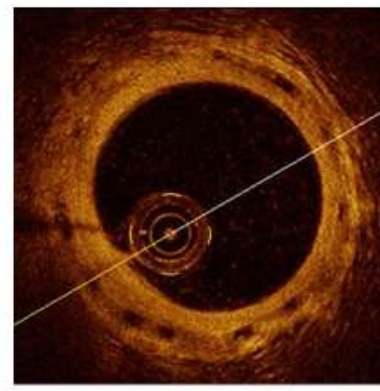

36 months

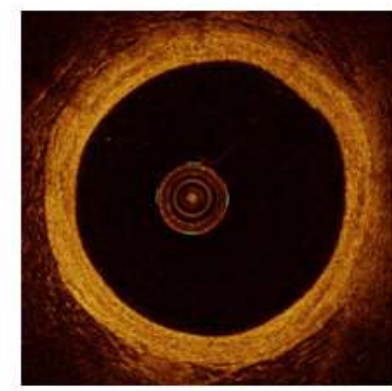

42 months

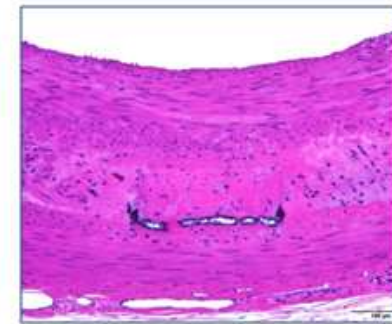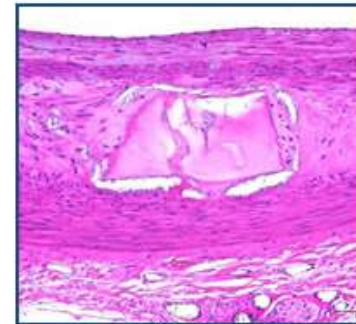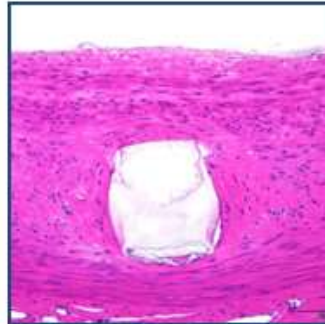





# Vessel Healing

The timing of scaffold degradation and resorption are critical for directing the vessel toward optimal healing, functionality and stability


Insufficient  
vessel support

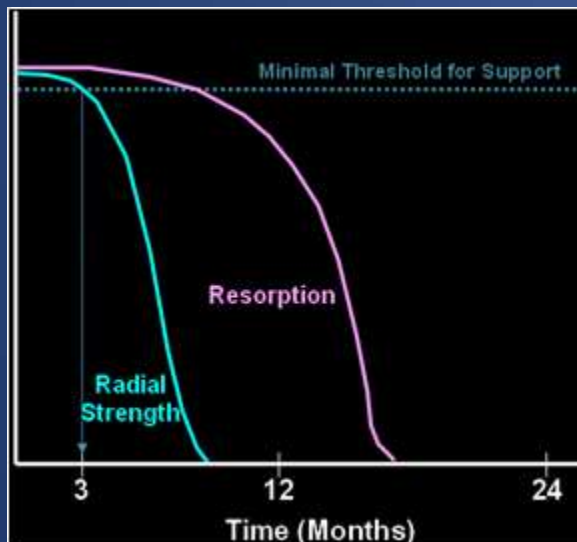

Resorbs too  
rapidly

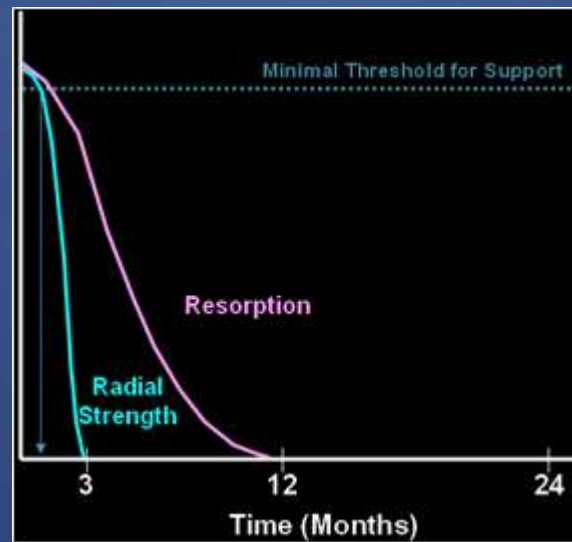


Ideal timing


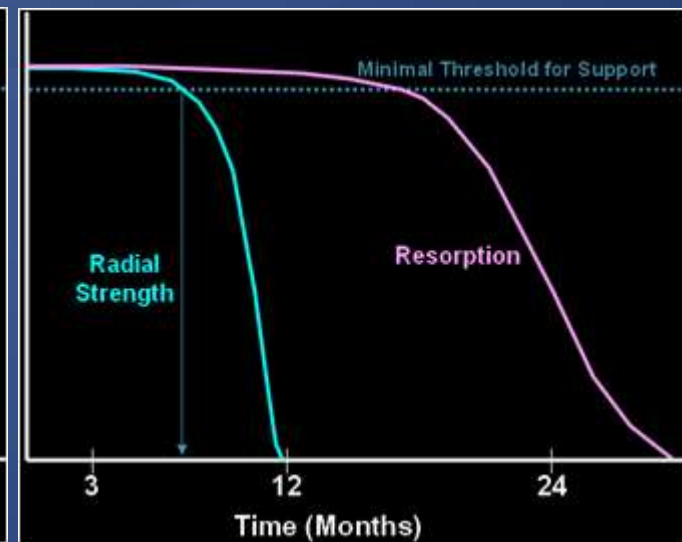


# Scaffold Marker Beads

- Two pairs of platinum marker – one pair at each end of the scaffold
- The marker on the scaffold lie near the inner edge of the balloon markers

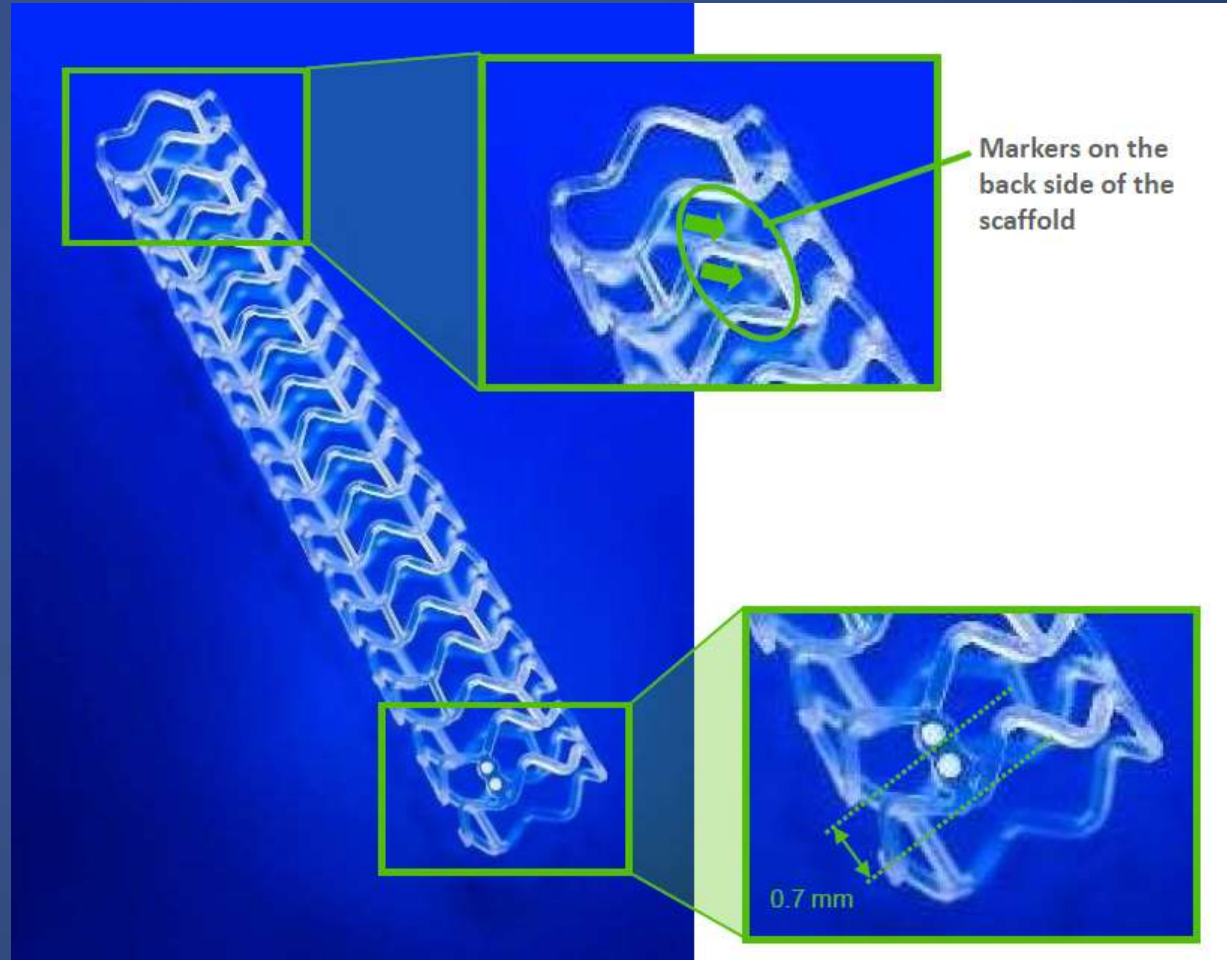


# Locating Scaffold Marker Beads

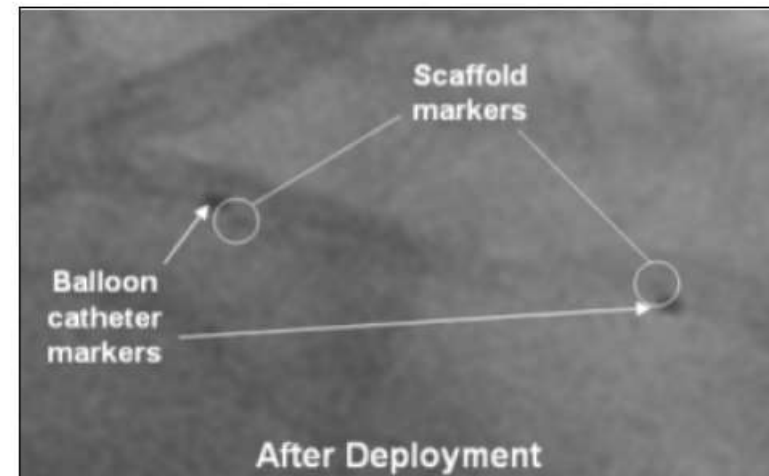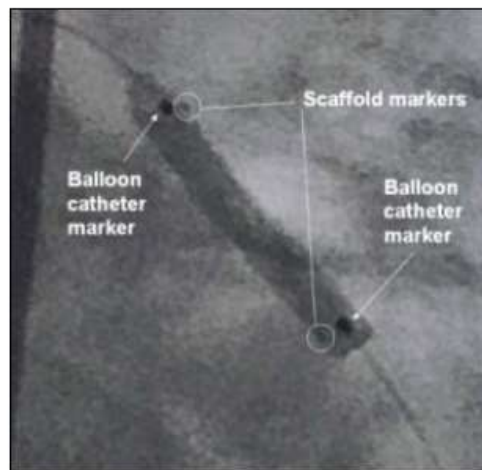

# How Much Radial Strength is Needed?

- Industry standards for stent radial from animal studies:
  - Maximal transluminal pressures of canine artery: 200 – 275 mmHg
  - Human arteries pressures around 100 mmHg
  - Stents withstand the difference between transluminal and intraluminal pressures: up to 175 mmHg
  - Adding a factor of safety the minimum acceptable collapse pressure for stents is **300** mmHg



# Radial Strength

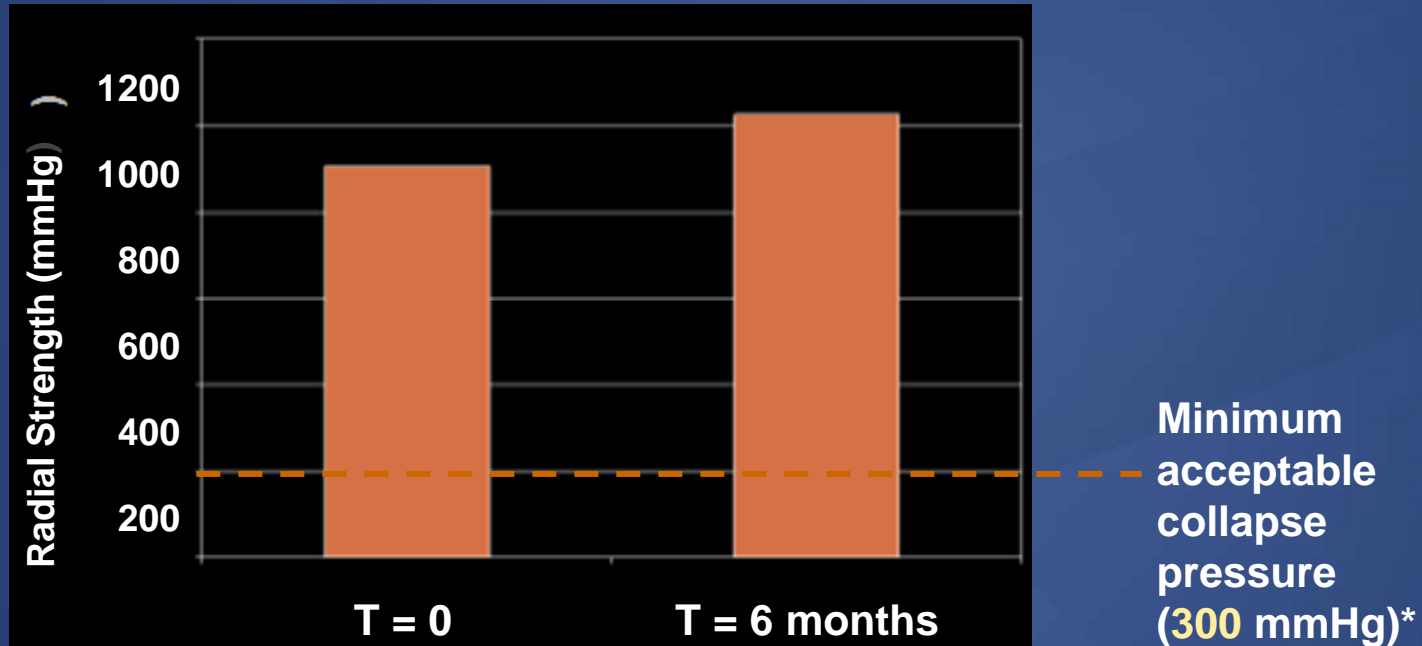

**BVS maintains adequate support for at least as long as is needed**

# What is the Minimum Duration of Radial Support?


Quantitative angiographic study in 342 consecutive patients

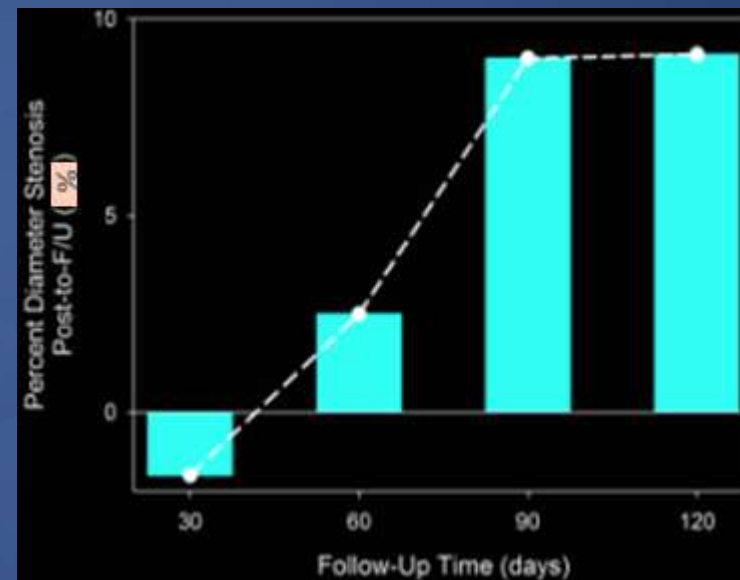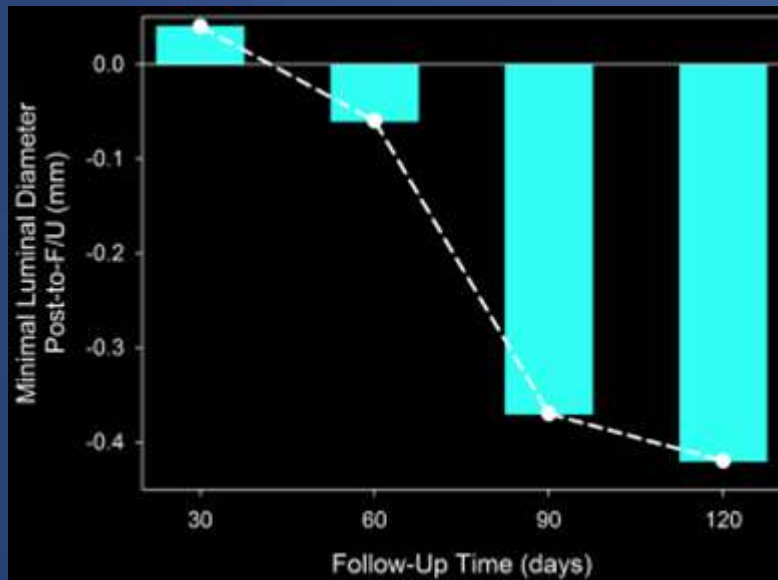

The lumen appears to stabilize **3 months** after PTCA



# What is the Minimum Duration of Radial Support?

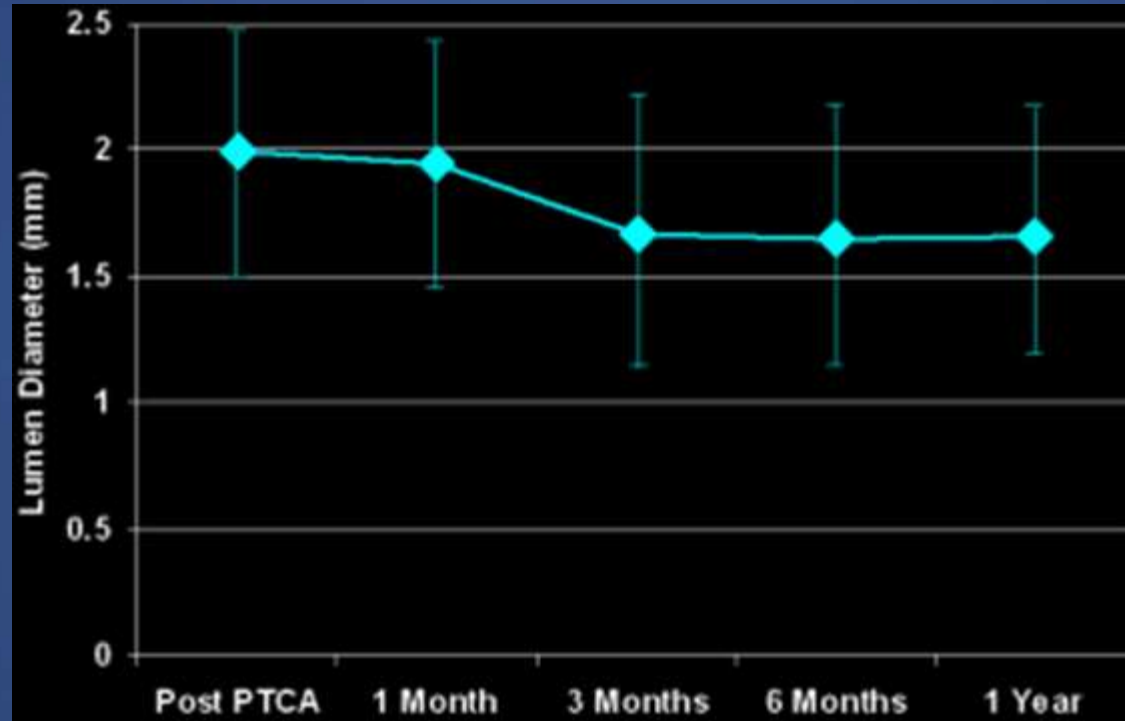

Changes in MLD following PTCA  
stabilize at 3 months

# Temperature Requirements

- Polymer based scaffold
- Polymers' performance is affected by temperature, as temperature affects the polymer material characteristics
- BVS needs to be maintained **between -20°C and 25°C at all**
  - Transported, received and stored in a temperature controlled environment

# Available Sizes of the Absorb BRS

		Lengths (mm)				
		8	12	18	23	28
Diameters (mm)	2.5	X	X	X	X	X
	3.0	X	X	X	X	X
	3.5		X	X	X	X

# ***Leaving Nothing Behind !***

- Initial scaffolding similar to metallic stents
- Restore vessel to natural state with normal function and healing response
  - Preservation of vascular geometry
  - Restoration of vascular physiology
  - Eliminate source of inflammation/irritation
  - Vessel free for future interventions
- Prevention of very late thrombotic events
- Passivation of vulnerable plaques

# Comparison of BRS with Other Angioplasty Technique/Devices

	POBA	BMS	DES	BRS
Acute occlusion	+	-	-	-
Acute recoil	+	-	-	-
Acute ST	+	+	+	+
Subacute ST	+/-	+	+	+
Late ST	-	+	+	+/- ?
Constrictive remodeling	-	+	+	+
Neointimal hyperplasia	-	++	+	+/-
Expansive remodeling	+	-	-	+
Late luminal enlargement	+	-	-	+
Vasomotion Restoration	+	-	-	+

# Limitations of BRS

- Thickness of strut
- Post-dilatation with a balloon diameter more than 0.5 mm bigger than the scaffold diameter
- Limited sizes and diameters currently available
- Slow and prolonged dilatations
- Lack of visibility on X-ray imaging




# **Technical Considerations of BRS Implantation**

# Unique characteristics of BRS

## Considering technical aspects

- The struts are **not visible under fluoroscopy or cine**. Only IVUS or OCT will allow visualization of struts.
- To provide sufficient radial strength, BVS has **thicker struts (156 $\mu$ m)** than contemporary metallic stents ( $\sim$ 80 $\mu$ m). This results in **larger crossing profile (1.4mm for Absorb)** and reduced deliverability or trackability.
- **Over-dilatation can result in strut disruption** and loss of radial strength.




# Scaffold mounted on the balloon

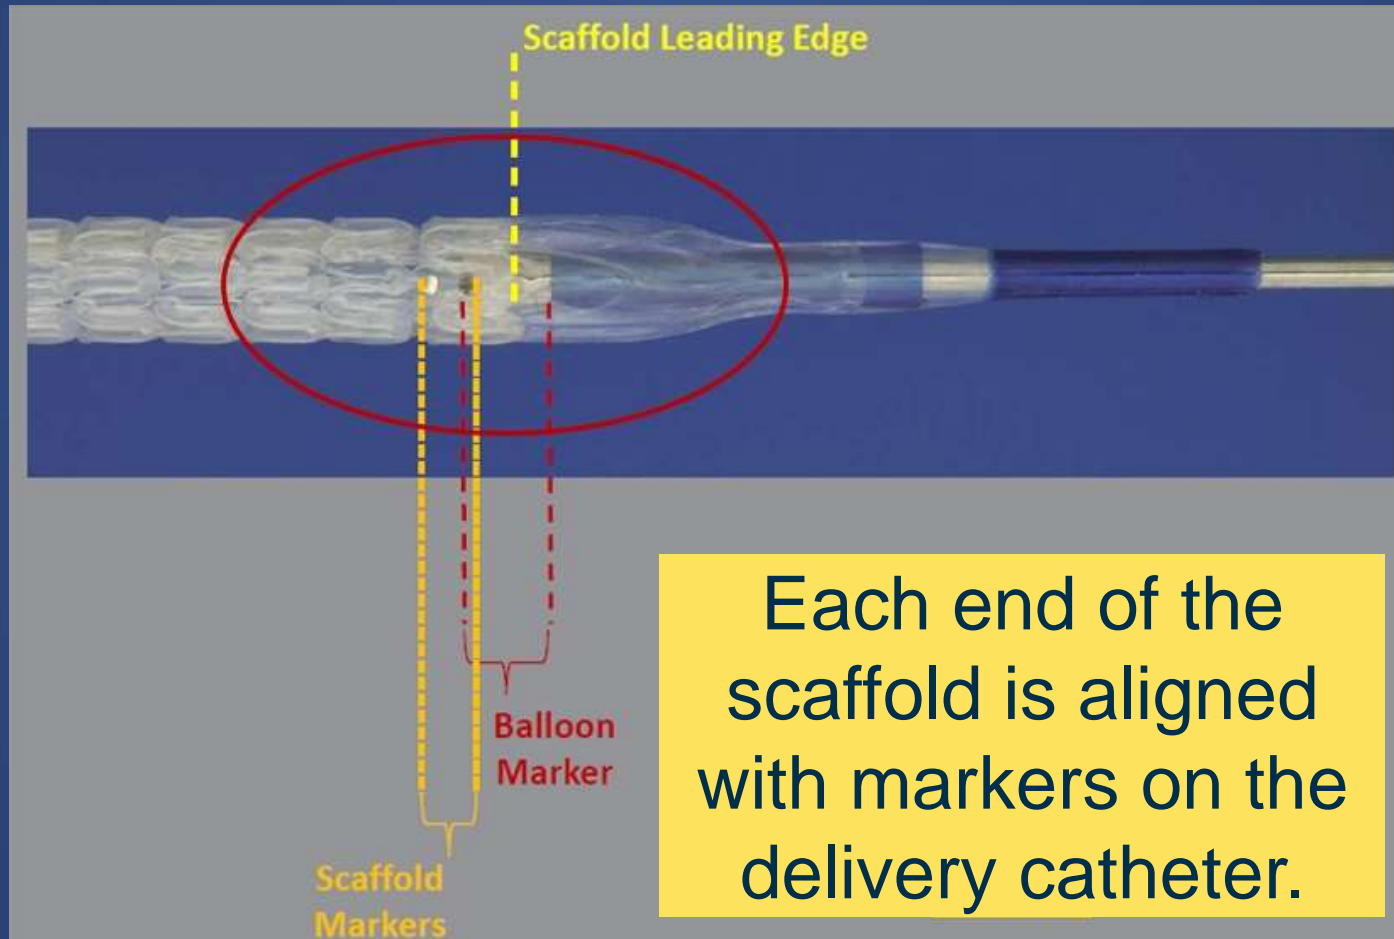

Use balloon markers to position scaffold


# Scaffold design

## Locating Scaffold Marker Beads

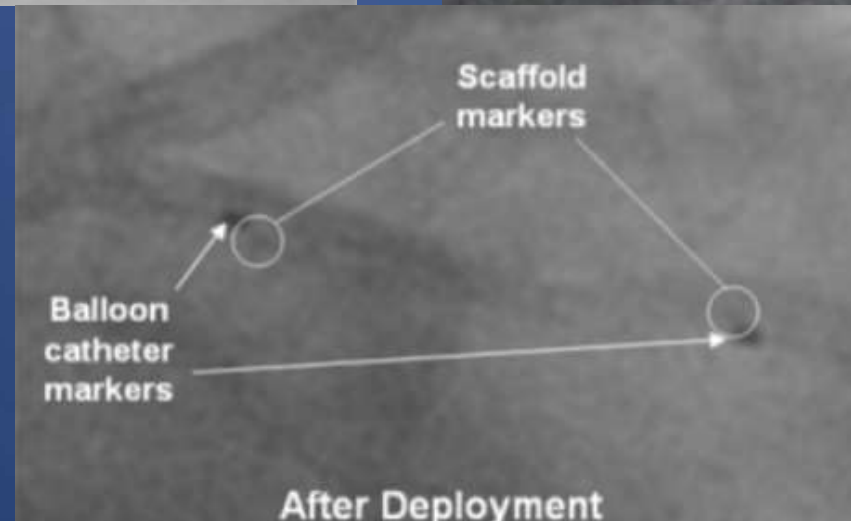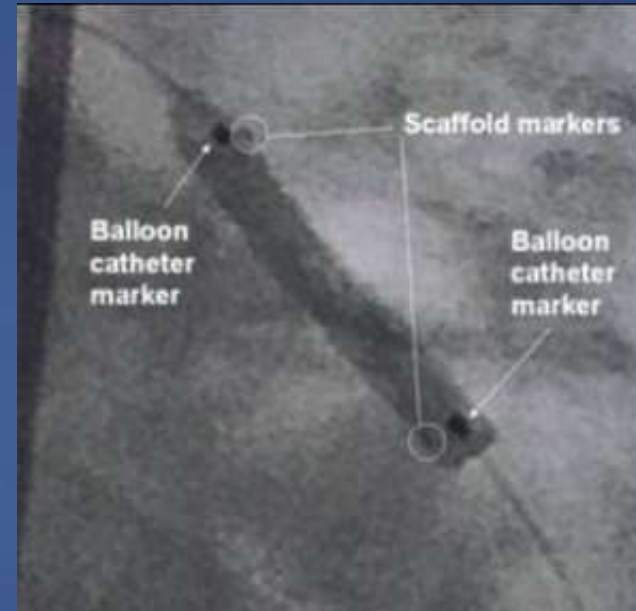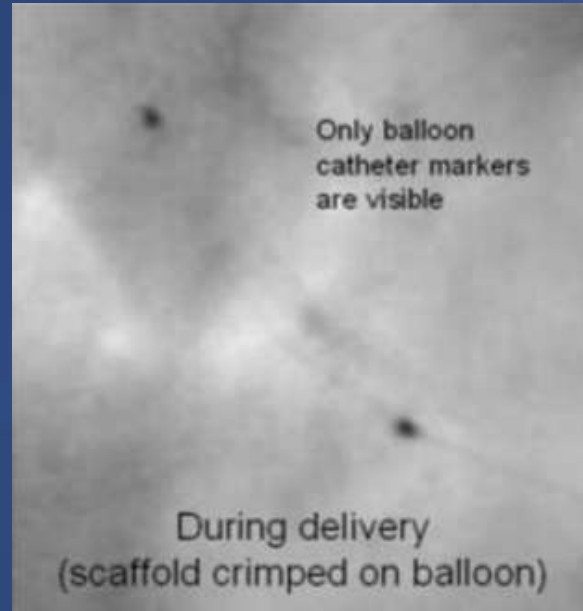


# Scaffold overlap

The distal balloon marker (BLUE) lines up with the proximal marker beads of the implanted scaffold

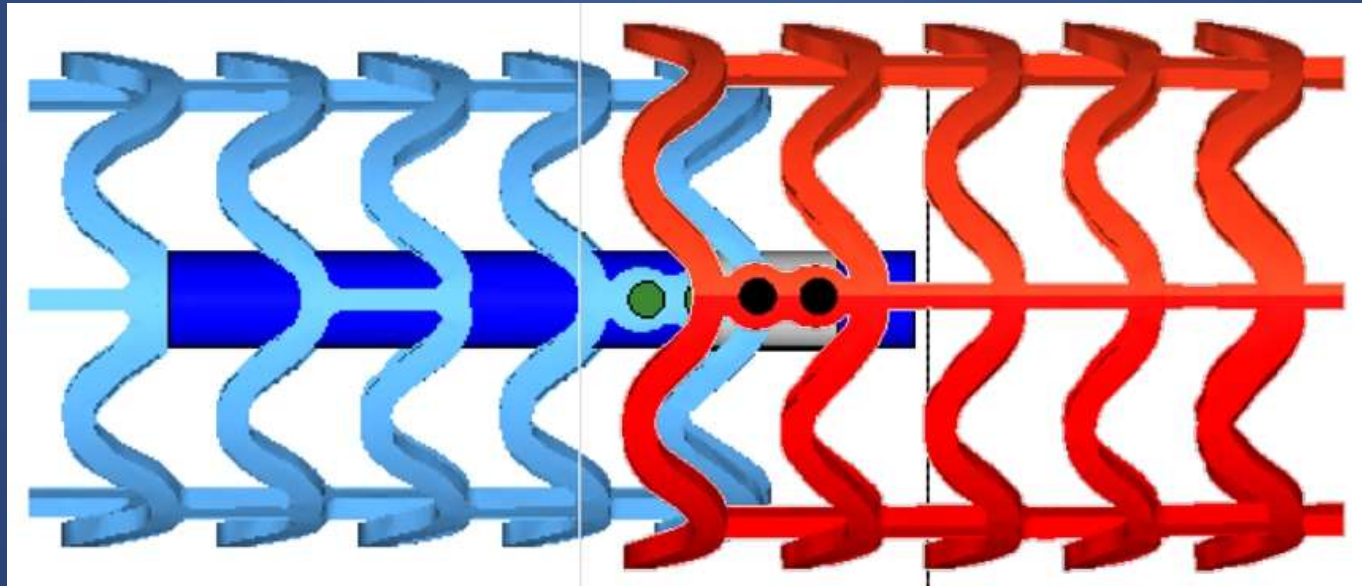

Balloon Marker under Scaffold Markers  
The result will be ~ 1mm of overlap

# Scaffold Overlap

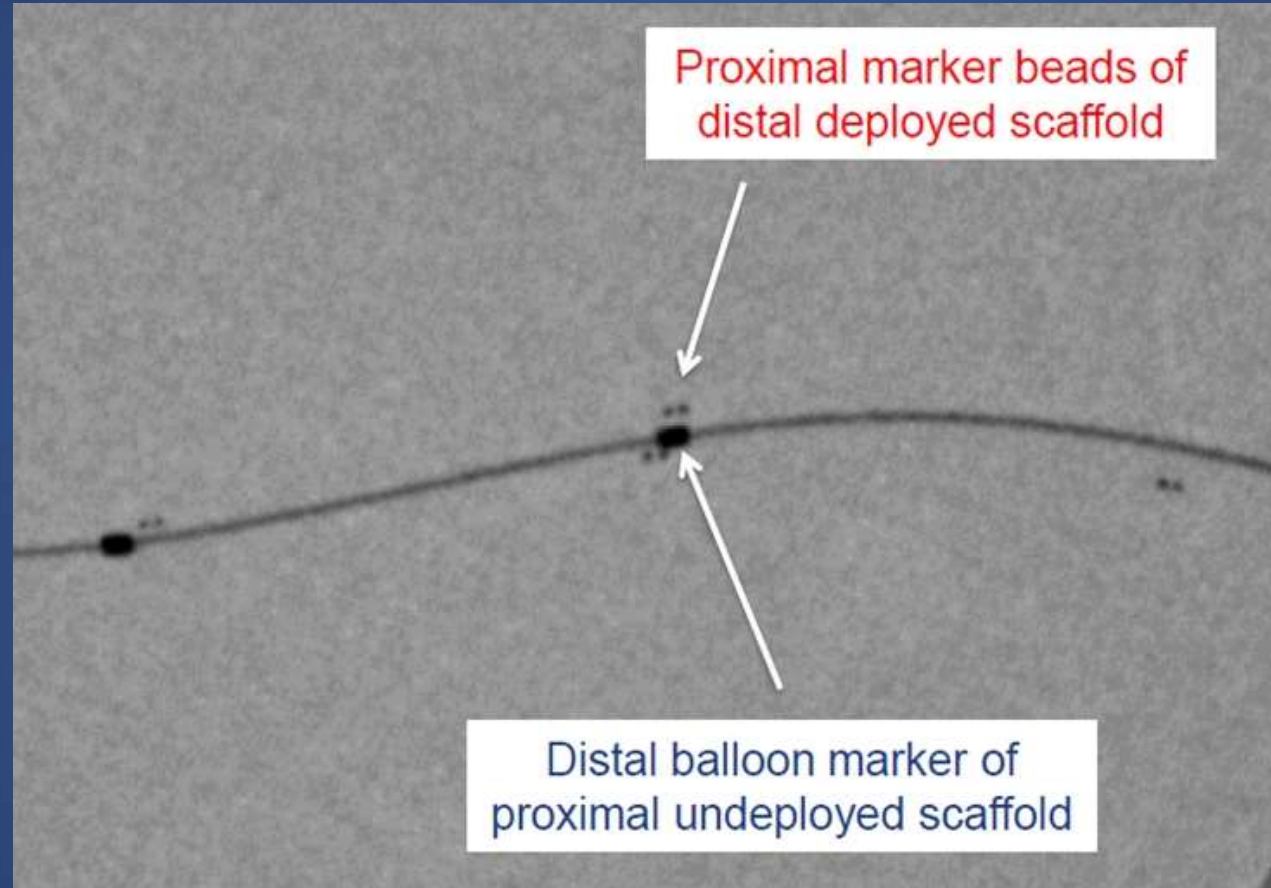

Line up the balloon marker band with the deployed scaffold marker beads; **this will result in ~1mm overlap**





# Scaffold design

## Guiding Catheter Compatibility

- At least  $\geq 6F$  / 0.070" / 1.8mm minimum inner diameter
- If challenges with crossing the lesion are anticipated
  - consider an extra back-up support guide catheter
  - consider a more supportive guide-wire
- Do not insert a guide sheath into a guiding catheter, as doing so will result in an inner diameter that is too small for use with Absorb

# Dual Layer Sheath Removal

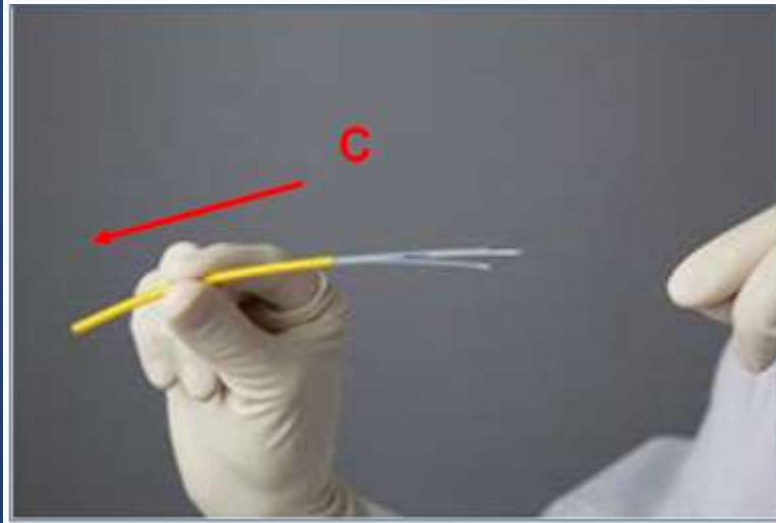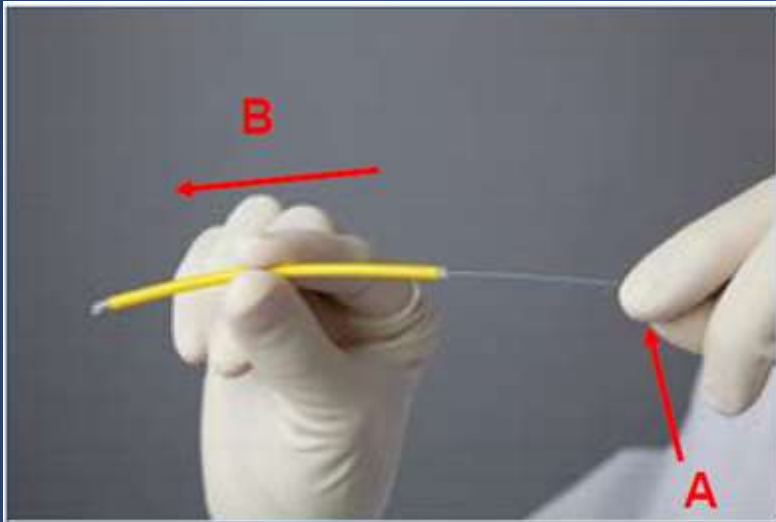

- **DO NOT** grab/pinch both the outer and inner sheaths together at the most proximal end as damage to the proximal balloon seal may occur.



# Optimal Implantation of **ABSORB: 5P**

1. Prepare the lesion
2. Properly size the Vessel
3. Pay Attention to Expansion Limits
4. Post-Dilate with a Non-Compliant Balloon
5. Prescribe Dual Anti-Platelet Therapy

# Prepare the lesion


- Absorb has a larger crimped profile than XIENCE; therefore, lesion preparation is key.
- Pre-dilatation is strongly recommended.
- Use of a non-compliant balloon is recommended.
- For highly resistant/calcified lesions, consider the use of cutting balloons, scoring balloons, or rotablator to optimize scaffold deployment.

# Crossing the lesion

- Following pre-dilatation, consider evaluating the vessel pathway with the deflated pre-dilatation balloon to assess to deliver scaffold to the lesion.
- An unexpanded scaffold should not be reintroduced into the artery once it has been pulled back into the guiding catheter or removed from the body.
- Use constant forward pressure to cross the lesion (Avoid the Dottering technique)

# Properly size the vessel

- IVUS or OCT are strongly recommended to size the vessel, particularly during the initial experience with the device

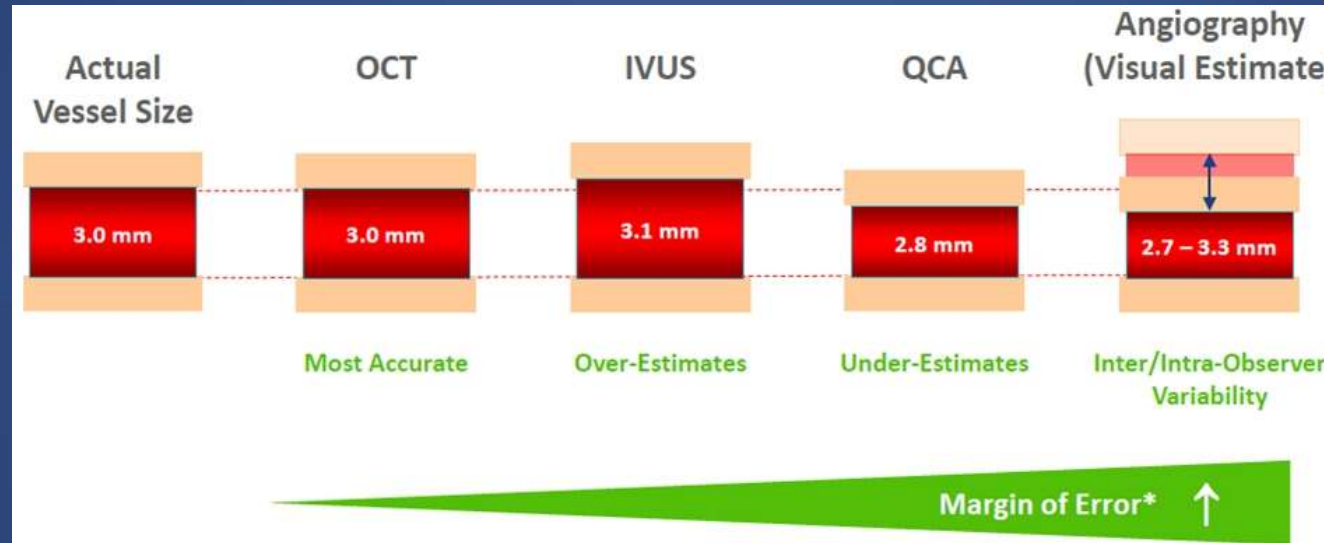

- When visually estimating vessel size, use the pre-dilatation balloon size when inflated in the lesion to more accurately size the vessel.
- It is recommended to administer a standard dose of intracoronary nitroglycerine prior to finalizing the RVD within the target zone.



# Pay attention to expansion limits


- It is important to stay within the expansion limits to avoid strut disruption and minimize the loss of radial strength.
- Scaffold expansion limits are nominal scaffold diameter + 0.5mm

	2.5 mm			3.0 mm			3.5 mm		
	ATM kPa ↔			ATM kPa ↔			ATM kPa ↔		
Clinical Trial Average Deployment Pressure*	6 (NOM)	608	2.53 mm	6	608	2.94 mm	6 (NOM)	608	3.50 mm
	7	709	2.60 mm	7 (NOM)	709	3.02 mm	7	709	3.59 mm
	8	811	2.66 mm	8	811	3.08 mm	8	811	3.66 mm
	9	912	2.71 mm	9	912	3.15 mm	9	912	3.73 mm
	10	1013	2.76 mm	10	1013	3.20 mm	10	1013	3.78 mm
	11	1115	2.79 mm	11	1115	3.24 mm	11	1115	3.83 mm
	12	1216	2.82 mm	12	1216	3.28 mm	12	1216	3.87 mm
	13	1317	2.86 mm	13	1317	3.31 mm	13	1317	3.91 mm
	14	1419	2.89 mm	14	1419	3.34 mm	14	1419	3.94 mm
	15	1520	2.91 mm	15	1520	3.37 mm	15	1520	3.98 mm
	16 (RBP)	1621	2.94 mm	16 (RBP)	1621	3.40 mm	16 (RBP)	1621	4.01 mm
	17	1723	2.97 mm	17	1723	3.43 mm			
	18	1824	2.99 mm	18	1824	3.46 mm			

- Maintain target deployment pressure for 30 seconds

# Post-Dilate with an NC Balloon

- If residual stenosis is  $>10\%$ , then consider using a non-compliant balloon that is up to + 0.5 mm larger than the nominal scaffold diameter (i.e. use a 3.5 mm NC balloon with a 3.0 mm scaffold)

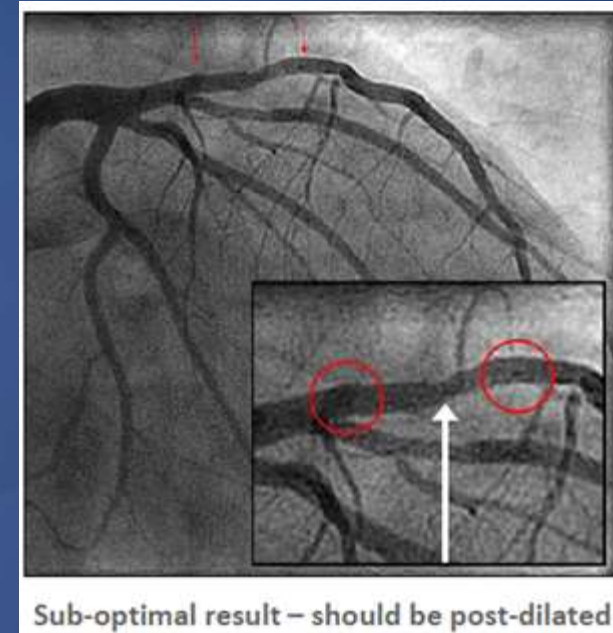

# Delivery system balloon removal Troubleshooting

- If resistance is experienced upon removal of the Absorb delivery system balloon from the deployed scaffold, re-inflate the balloon up to nominal pressure, deflate, and **change pressure to neutral** as balloon folds relax and soften allowing for easier withdrawal




Negative Pressure



Neutral Pressure

# Treating side branches

- If a clinical decision is made to dilate a side branch, use sequential balloon inflations
- Avoid scaffolding across any side branch  $\geq 2.0\text{mm}$
- Always finish with main branch balloon inflation


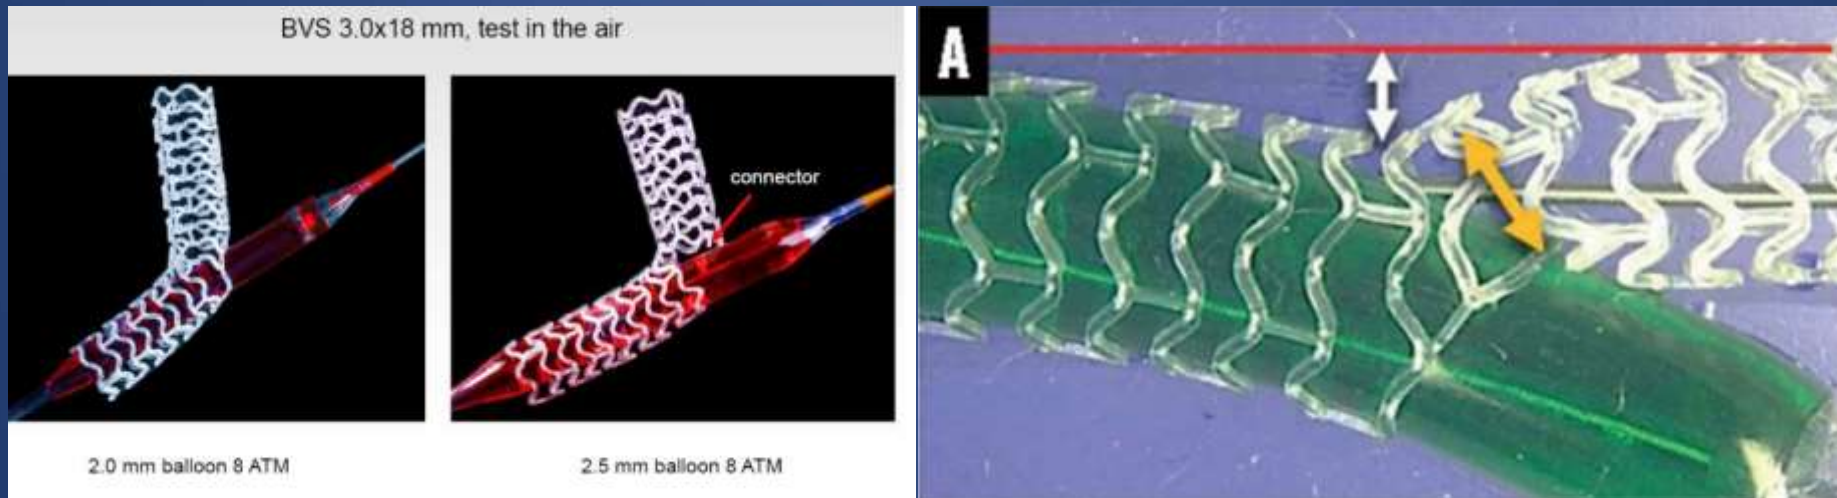


# Post-dilate with an NC balloon

- High pressure post-dilatation with a non-compliant balloon is ideal (<10% RS)
  - To achieve optimal scaffold apposition
  - Do not dilate the scaffold beyond its maximum expansion limit
- If residual stenosis is >10%, then consider using a non-compliant balloon that is up to + 0.5 mm larger than the nominal scaffold diameter
- Use imaging guidance (IVUS or OCT)



# Conventional kissing is prohibited

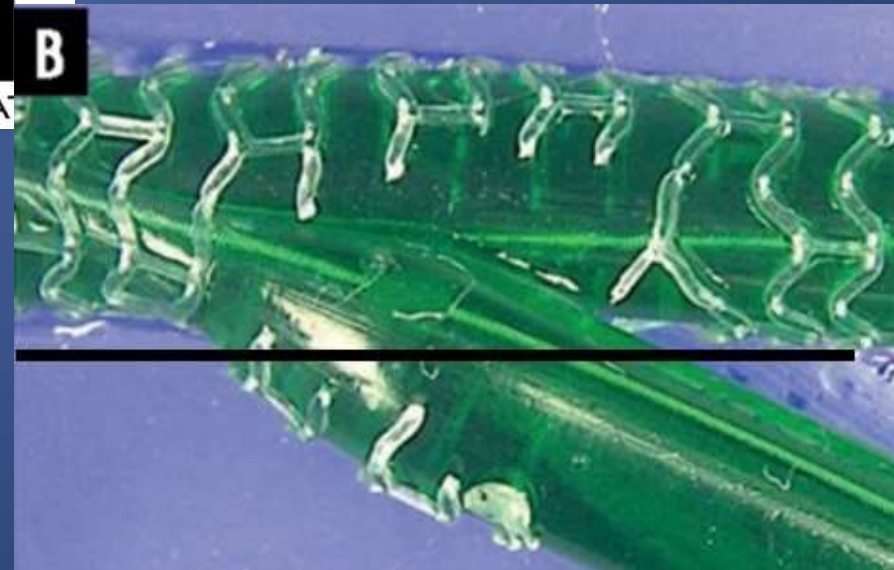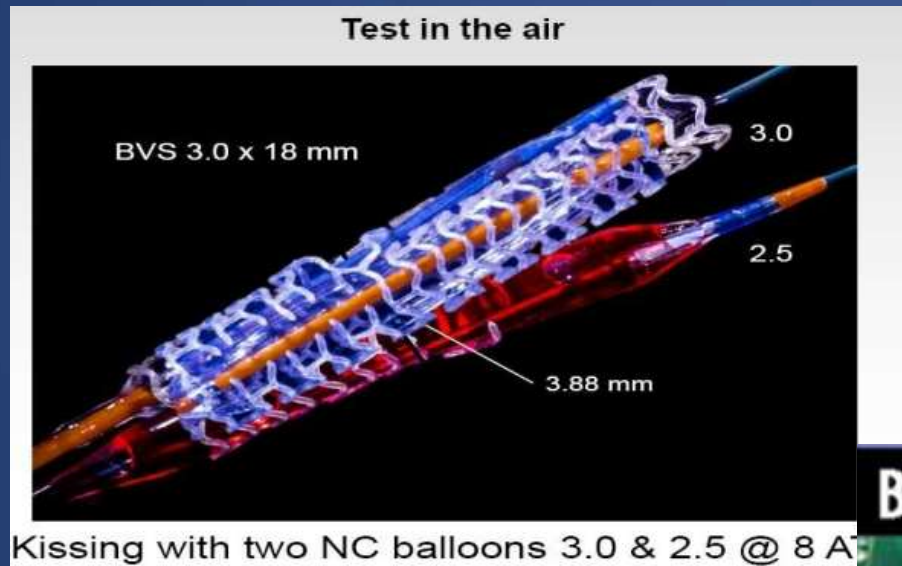

# DAPT prescription

- Consider current ACC/AHA and ESC DAPT guidelines
- **More potent P2Y12 inhibitors** (Ticagrelor or Prasugrel) are highly recommended for complex lesions requiring extensive lesion prep, ACS/STEMI patients, and overlapped scaffolds

# **Clinical outcomes of BRS**

# Absorb Comprehensive Abbott Vascular Sponsored Clinical Trial Program




# ABSORB Cohort A

## Introduction

**30 subjects**

(Non-randomized) 4 sites in Europe & New Zealand

**Clinical**

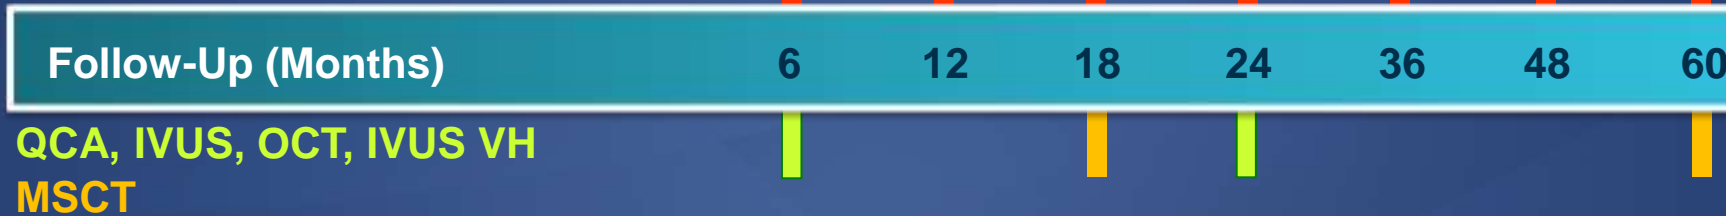

Study Objective	First In Man, Single Arm – safety/performance
Endpoints	Typical PCI clinical and imaging endpoints
Treatment	Single, <i>de novo</i> native coronary lesion in a vessel with a reference vessel diameter of 3.0 mm
Device Sizes	3.0 x 12 mm scaffolds (3.0 x 18 mm scaffolds available after enrollment start and used in 2 pts)



# ABSORB Cohort A

## Baseline Demographics and Lesion Characteristics

Male	58%
Diabetes Mellitus	4%
Location of Lesions	
LAD	50%
LCX	23%
RCA	27%
Lesion Classification	
Type B1	65%
Type B2	35%
Pre-Procedure	
Lesion length (mm)	8.66 ± 3.97
RVD (mm)	2.78 ± 0.47
MLD (mm)	1.10 ± 0.26
DS (%)	59 ± 12

# ABSORB Cohort A

## Excellent Long-Term Data Out to 5 Years

### ABSORB Cohort A Clinical Results at Each Phase: Intent to Treat

Hierarchical	6 Months 30 Patients	1 year 29 Patients**	2 Year 29 Patients**	5 Year 29 Patients**
Ischemia Driven MACE***	1 (3.3%)*	1 (3.4%)*	1 (3.4%)*	1 (3.4%)*
Cardiac Death	0 (0.0%)	0 (0.0%)	0 (0.0%)	0 (0.0%)
MI	1 (3.3%)*	1 (3.4%)*	1 (3.4%)*	1 (3.4%)*
Q-Wave MI	0 (0.0%)	0 (0.0%)	0 (0.0%)	0 (0.0%)
Non Q-Wave MI	1 (3.3%)*	1 (3.4%)*	1 (3.4%)*	1 (3.4%)*
Ischemia Driven TLR	0 (0.0%)	0 (0.0%)	0 (0.0%)	0 (0.0%)
by PCI	0 (0.0%)	0 (0.0%)	0 (0.0%)	0 (0.0%)
by CABG	0 (0.0%)	0 (0.0%)	0 (0.0%)	0 (0.0%)

Serruys, ABSORB Cohort A 5-year results; TCT, 2011

**No scaffold thrombosis by ARC or Protocol**

*Adapted from Serruys, PW, ABSORB Cohort A 2-year IVUS and OCT results; ACC 2009.*

# Temporal Lumen Dimensional Changes, Per Treatment



# ABSORB Cohort B

## Introduction

**101 subjects**

(Non-randomized) 12 sites in Europe, Australia, New Zealand

Group B1 ( $n = 45$ )

Imaging Follow-Up (Months)

6

12

18

24

36

Group B2 ( $n = 56$ )

QCA, IVUS, OCT, IVUS VH  
MSCT

Study Objective

First In Man, Single Arm – safety/performance

Endpoints

Typical PCI clinical and imaging endpoints

Treatment

Up to 2 *de novo* lesions in different epicardial vessels  
Reference vessel diameter of 3.0 mm, lesions  $\leq 14$  mm in length

Device Sizes

3.0 x 18 mm devices

# **ABSORB Cohort B**

## **Baseline Lesion Characteristics/ Acute Success**

### **Location of lesion (%)**

LAD	43
RCA	33
LCX	22
Ramus	1

### **Lesion classification (%)**

A	1
B1	55
B2	40
C	4

<b>Clinical Device Success (%)</b>	<b>100</b>
------------------------------------	------------

<b>Clinical Procedure Success (%)</b>	<b>98</b>
---------------------------------------	-----------

# ABSORB Cohort B

## Clinical Results - Intent to Treat

Non-Hierarchical	30 Days	1 Year	2 Years	3 Years
	N = 101	N = 101	N = 100*	N = 100*
Cardiac Death %	0	0	0	0
Myocardial Infarction % (n)	2.0 (2)	3.0 (3)	3.0 (3)	3.0 (3)
Q-wave MI	0	0	0	0
Non Q-wave MI	2.0 (2)	3.0 (3)	3.0 (3)	3.0 (3)
Ischemia driven TLR % (n)	0	4.0 (4)	6.0 (6)	7.0 (7)
CABG	0	0	0	0
PCI	0	4.0 (4)	6.0 (6)	7.0 (7)
Hierarchical MACE % (n)	2.0 (2)	6.9 (7)	9.0 (9)	10.0 (10)
Hierarchical TVF % (n)	2.0 (2)	6.9 (7)	11.0 (11)	13.0 (13)

MACE: Cardiac death, MI, ischemia-driven TLR, TVF: Cardiac death, MI, ischemia-driven TLR, ischemia-driven TVR

**No scaffold thrombosis by ARC or Protocol**



# ABSORB Cohort B1

## Clinical Results - Intent to Treat


	30 Days	6 Months	12 Months	2 Years	3 Years	4 Years
Non-Hierarchical	N = 45	N = 45	N = 45	N = 44*	N = 44*	N = 44*
Cardiac Death %	0	0	0	0	0	0
Myocardial Infarction % (n)	2.2 (1)	2.2 (1)	2.2 (1)	2.3 (1)	2.3 (1)	2.3 (1)
Q-wave MI	0	0	0	0	0	0
Non Q-wave MI	2.2 (1)	2.2 (1)	2.2 (1)	2.3 (1)	2.3 (1)	2.3 (1)
Ischemia driven TLR % (n)	0	2.2 (1)	4.4 (2)	4.5 (2)	4.5 (2)	4.5 (2)
CABG	0	0	0	0	0	0
PCI	0	2.2 (1)	4.4 (2)	4.5 (2)	4.5 (2)	4.5 (2)
Hierarchical MACE % (n)	2.2 (1)	4.4 (2)	6.7 (3)	6.8 (3)	6.8 (3)	6.8 (3)
Hierarchical TVF % (n)	2.2 (1)	4.4 (2)	6.7 (3)	6.8 (3)	9.1 (4)**	9.1 (4)**

**No new MACE between 1-year and 4-years**  
**No scaffold thrombosis by ARC or Protocol**

# ABSORB Cohort B

## -Year Follow Up – B. Chevalier

KM Estimate of MACE Rate in Patients Treated with Absorb vs. Patients Treated with a Single 3.0x 18 mm Metallic XIENCE V

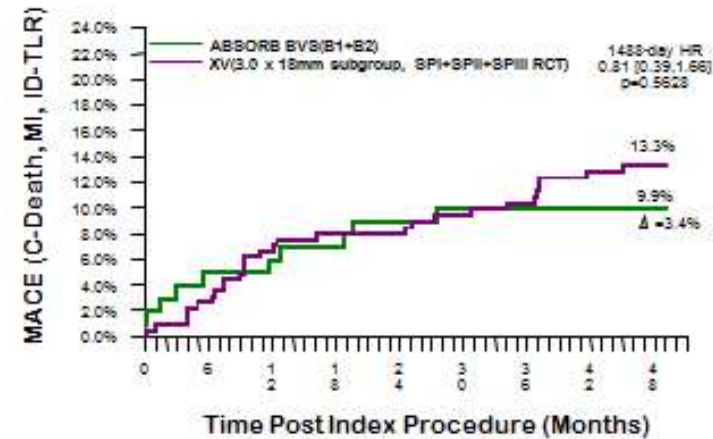

	Time After Index Procedure (days)							
	0	37	194	284	395	758	1123	1438
ABSORB BVS(B1+B2) At Risk	101	99	96	96	94	91	89	39*
XV(3.0 x 18mm subgroup, SPI+SPII+SPIII RCT) At Risk	227	224	219	211	204	191	182	178

**Absorb Demonstrates Similar Safety to XIENCE**


# ABSORB Cohort B

## 6, 12, 24 and 36-Month QCA – Intent to Treat (Groups 1 & 2)

The Evolution of Cumulative Frequency Distribution Curves for Late Loss Over Time:  
Absorb BVS and XIENCE V (Non-Matched Population)

Angiographic late loss similar to XIENCE V and remains  
relatively unchanged between 12 and 36 months\*


6 Months<sup>1</sup>

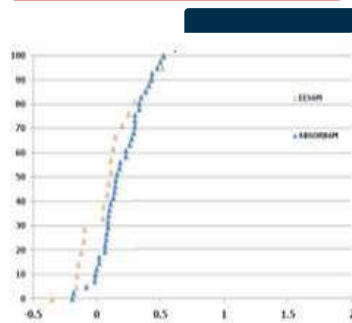

BVS:  $0.19 \pm 0.18$  mm (n=42)

XIENCE V:  $0.10 \pm 0.23$  mm (n=22)


12 Months<sup>1</sup>

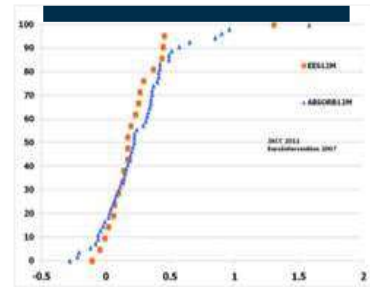

BVS:  $0.27 \pm 0.32$  mm (n=56)

XIENCE V:  $0.23 \pm 0.29$  mm (n=22)


24 Months<sup>1</sup>

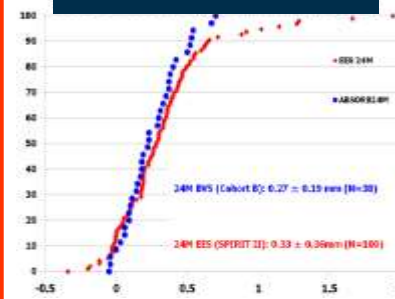

BVS:  $0.27 \pm 0.19$  mm (n=38)

XIENCE V:  $0.33 \pm 0.36$  mm (n=100)

36 Months<sup>2</sup>

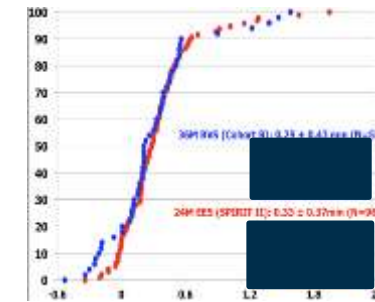


BVS:  $0.29 \pm 0.43$  mm (n=51)

XIENCE V:  $0.33 \pm 0.36$  mm (n=100)\*


# ABSORB Cohort B

## Serial IVUS Analysis (N=45)

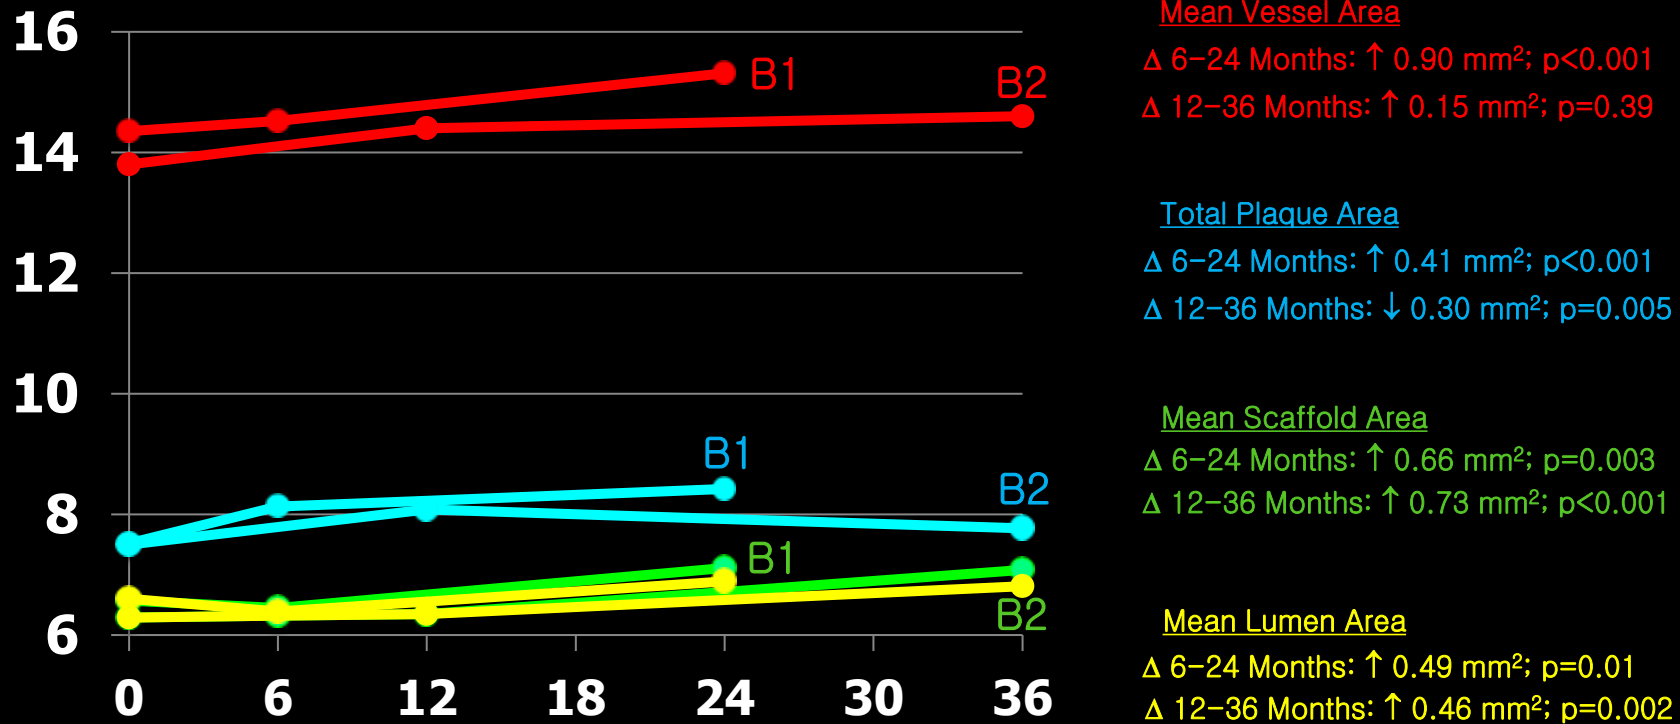

# ABSORB Cohort B

## Temporal Lumen Dimensional Changes

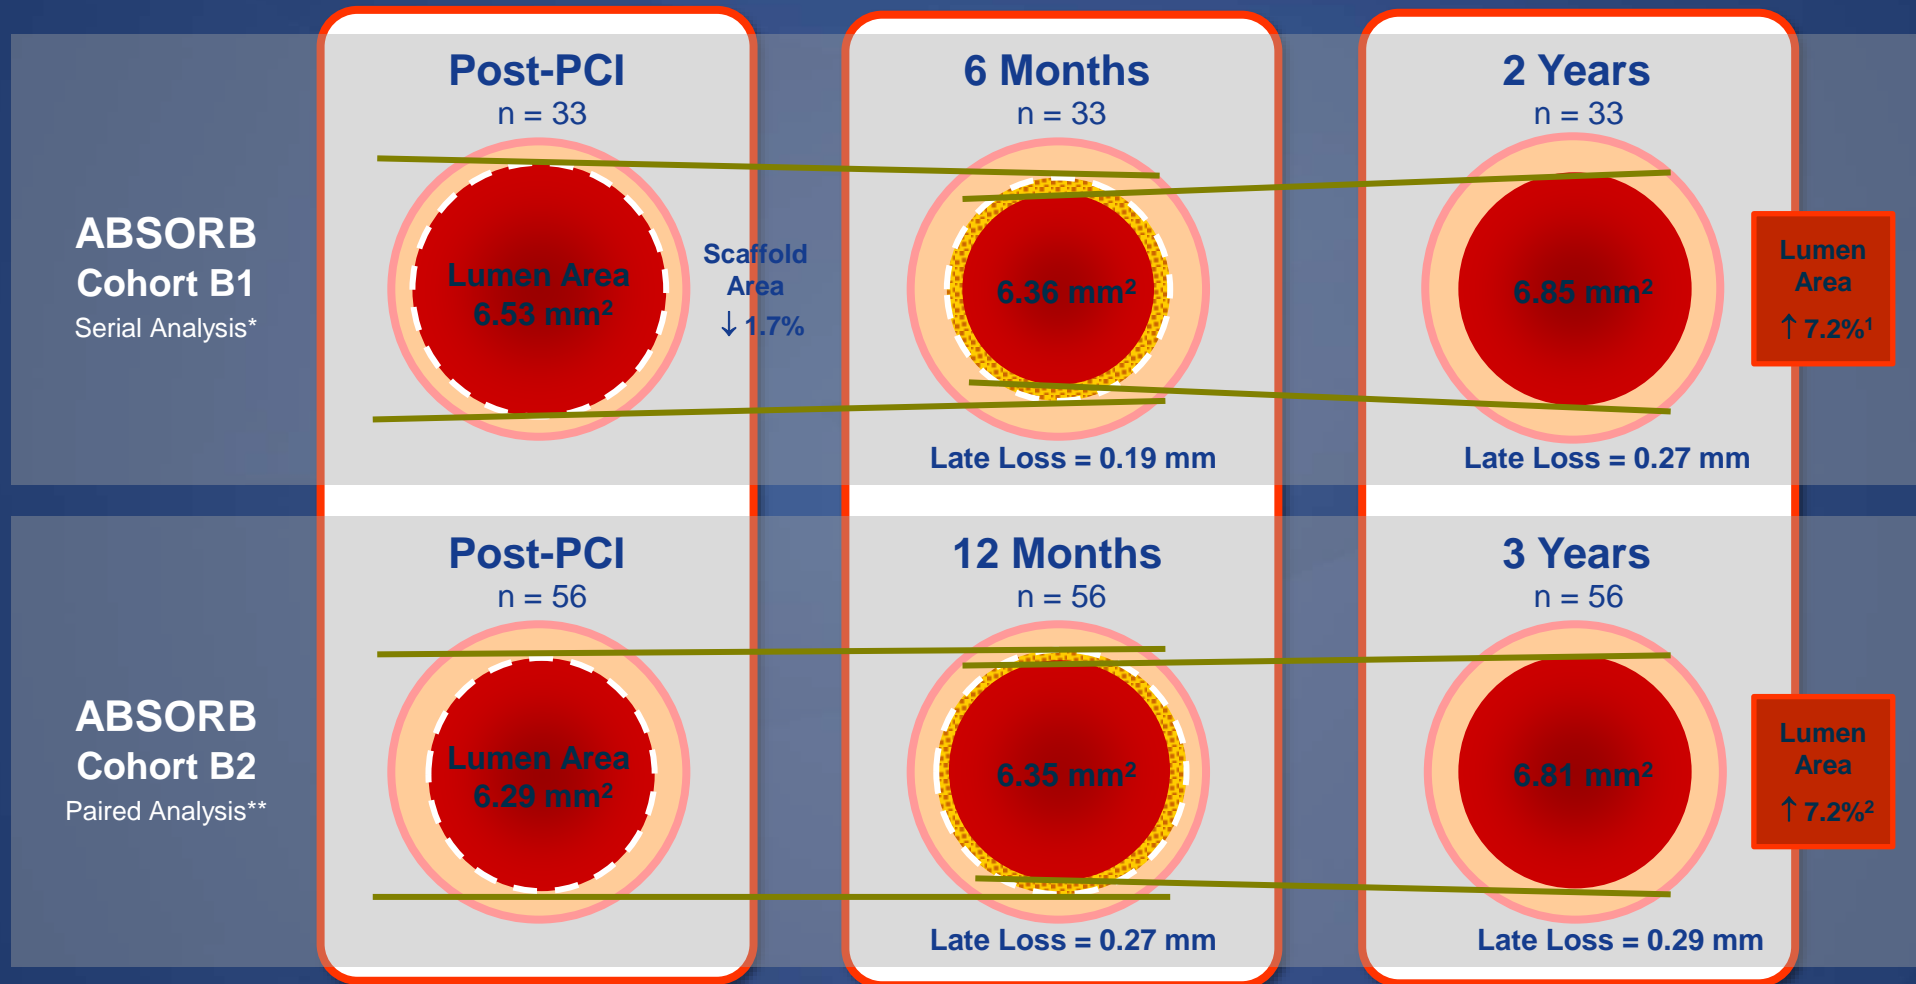

1. Patient-level serial analysis  
2. Calculated from overall mean values

\*Serruys, PW., ABSORB Cohort B 2-year results; TCT 2011

\*\*Serruys, PW., ABSORB Cohort B 3-year results; ACC 2013

# ABSORB EXTEND

**Non-Randomized, Single-Arm., Continued assess**

**~1,000 subjects**

Up to 100 global sites (non-US)

Clinical Follow-Up

Clinical Follow-up (months)	6	12	18	24	36
-----------------------------	---	----	----	----	----

MSCT follow up (n=100)

OCT follow up (n=50)

Study Objective	FPI: Jan 11, 2011
Endpoints	Typical PCI clinical endpoints
Treatment	Up to 2 <i>de novo</i> lesions in different epicardial vessels Planned overlapping allowed in lesions >22 and ≤ 28 mm
Device Sizes	Scaffold diameters: 2.5, 3.0, 3.5 mm Scaffold lengths: 12*, 18, 28 mm



# Pooled ABSORB Cohort B and EXTEND 1-Year, Propensity Score Adjusted Analysis vs. SPIRIT II/III – B. Chevalier

## Propensity Adjusted Clinical Outcomes At 1 Year

Non-Hierarchical	Absorb BVS (N = 558)	XIENCE V (N = 672)	P value
Cardiac Death %	0.3	0.6	0.35
Myocardial Infarction %	3.9	2.1	0.06
Ischemia Driven TLR %	1.6	3.2	0.08
Hierarchical MACE %	5.2	5.5	0.81
Hierarchical TVF %	5.5	8.6	0.04
Hierarchical TLF %	5.2	5.0	0.91
Scaffold Thrombosis (ARC Def/Prob) %	0.5	0.5	0.93

Information contained herein for presentation outside the U.S. only. Absorb is authorized for sale in CE Mark and certain independently regulated countries outside the United States. Please check the regulatory status of the device in your geographical location before distribution. AP2939135-005 Rev. A 10/13

Absorb BVS Cohort:  
XIENCE V Cohort:

Pooled from ABSORB EXTEND and ABSORB Cohort B trials  
Pooled from XIENCE V arms of SPIRIT FIRST, II, and III trials

# ABSORB EXTEND

## Clinical Results – Intent to Treat; Interim Snapshot

Non-Hierarchical % (n)	12 Months* (N = 250)	24 Months* (N = 250)
Cardiac Death % (n)	0.4	0.4
Myocardial Infarction % (n)**	2.8	4.0
Q-wave MI	1.2	1.2
Non Q-wave MI	1.6	2.8
Ischemia driven TLR % (n)	2.0	4.0
CABG	0.0	0.4
PCI	2.0	4.0
Hierarchical MACE % (n)	4.4	7.3
Hierarchical TVF %	4.8	8.1
Hierarchical TLF %	4.4	6.9
Scaffold Thrombosis (ARC <u>Def/Prob</u> ) % (n)	0.8	0.8

# 2-Year Propensity Scored Analysis ABSORB EXTEND vs. SPIRIT I/II/III - R. Whitbourn

## Absorb has comparable safety to XIENCE


### ABSORB EXTEND Propensity Score Matched Clinical Outcomes: 2 Years

	Absorb (EXTEND, N = 178)	XIENCE V (SP123, N = 293)	P Value
NON-HIERARCHICAL COMPONENTS			
Cardiac Death %	0.0	1.4	0.30
Myocardial Infarction %	4.5	4.4	1.00
Ischemia Driven TLR %	3.4	3.8	1.00
MACE %	6.7	8.9	0.49
TVF %	7.3	12.3	0.09
TLF %	6.2	8.2	0.47
Scaffold Thrombosis (ARC Def/Prob) %	0.6	1.4	0.65

# Pooled Analysis From ABSORB Cohort B and EXTEND 1-Year, Clinical Outcomes of Diabetic Patients vs. SPIRIT I/II/III/IV at 1-Year– T. Muramatsu


## Absorb Demonstrates Similar Safety to XIENCE

Absorb  
Patients with  
Diabetes  
vs.  
Absorb  
Patients  
without  
Diabetes

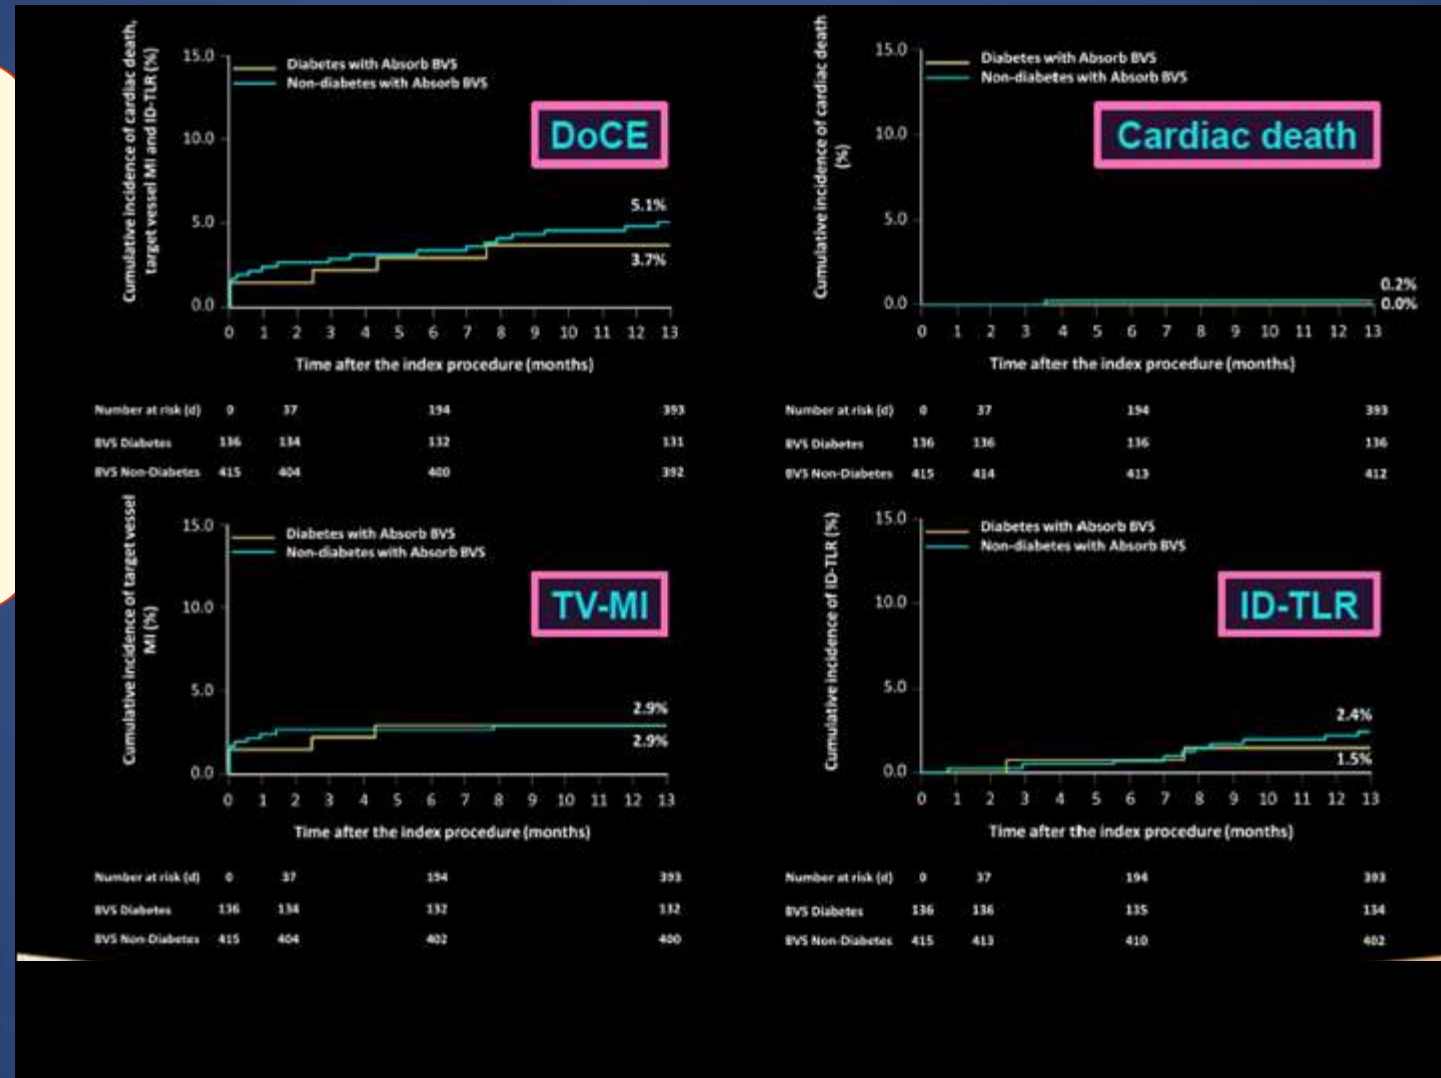

# **ABSORB EXTEND / XIENCE V**

## **Propensity Score Matched Analysis**

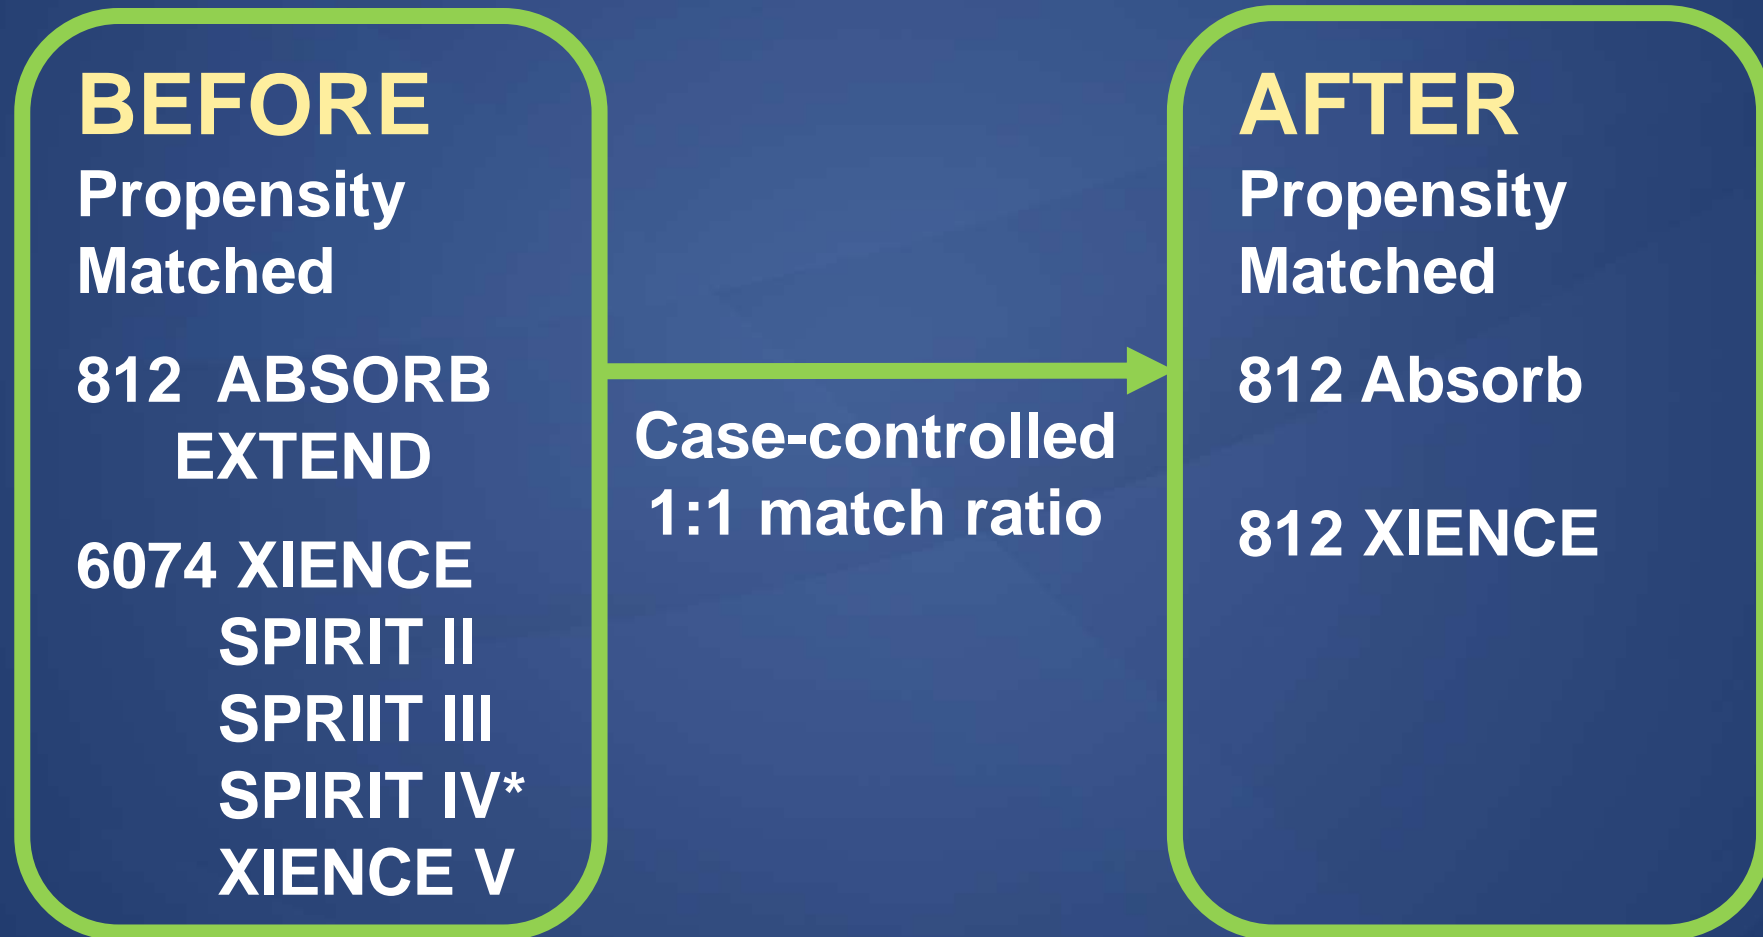

# **ABSORB EXTEND / XIENCE V**

## **Propensity Score Matched 1 Year Clinical Outcomes**

	<b>Absorb (EXTEND, N = 812)</b>	<b>XIENCE V (N = 812)</b>	<b>P Value</b>
<b>NON-HIERARCHICAL COMPONENTS</b>			
<b>Cardiac Death %</b>	<b>0.7</b>	<b>0.6</b>	<b>0.80</b>
<b>Myocardial Infarction %</b>	<b>3.3</b>	<b>1.5</b>	<b>0.02</b>
<b>Ischemia Driven TLR %</b>	<b>2.3</b>	<b>3.0</b>	<b>0.38</b>
<b>MACE %</b>	<b>5.0</b>	<b>4.8</b>	<b>0.83</b>
<b>TVF %</b>	<b>5.5</b>	<b>6.2</b>	<b>0.57</b>
<b>TLF %</b>	<b>5.0</b>	<b>4.7</b>	<b>0.74</b>
<b>Scaffold Thrombosis (ARC Def/Prob) %</b>	<b>1.0</b>	<b>0.3</b>	<b>0.11</b>



# **Propensity Score Matched Analysis of Site Diagnosed Angina**

## **Significant Difference in SDA at 1-Year**

### **Unadjusted**

<b>Unadjusted</b>	<b>Absorb (EXTEND)</b>	<b>XIENCE V (SPIRIT IV)</b>	<b>Difference [CI]</b>
1-Year	15.9% (60/378)	27.1% (542/2000)	11.2% [7.1%, 15.4%]


### **Propensity Score Matched**

<b>PS Matched</b>	<b>Absorb (EXTEND)</b>	<b>XIENCE V (SPIRIT IV)</b>	<b>Difference [CI]</b>
1-Year	16.0% (46/287)	27.9% (168/602)	11.9% [6.3%, 17.4%]

# Propensity Score Analysis ABSORB EXTEND vs. SPIRIT I/II/III Definite/Probable ST Through 24-Months – R. Whitbourn


## Absorb has comparable safety to XIENCE

Propensity Score Matched Analysis:  
ABSORB EXTEND/SPIRIT ST (def/prob) Through 24 Months

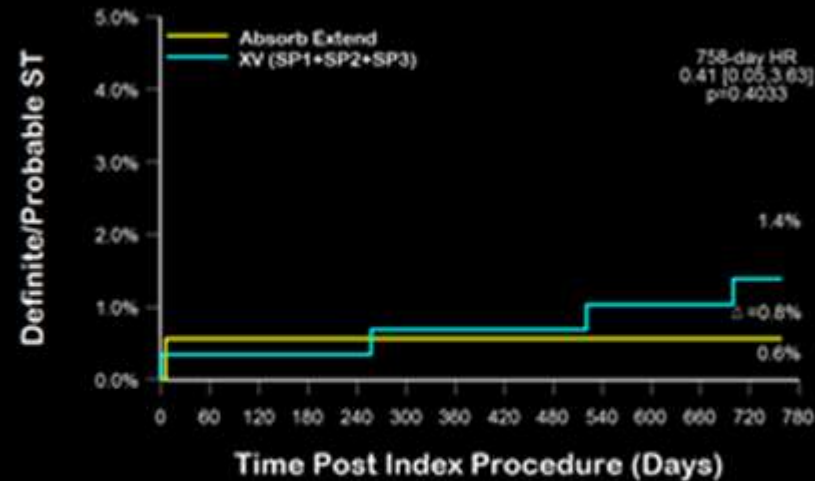

	0	37	194	393	758
ABSORB EXTEND At Risk:	178	177	177	177	177
XIENCE V (SPIRIT I, II and III) At Risk:	293	292	292	286	266


# Absorb Propensity Score-Matched Angina Through 1-Year ABSORB EXTEND vs. SPIRIT IV

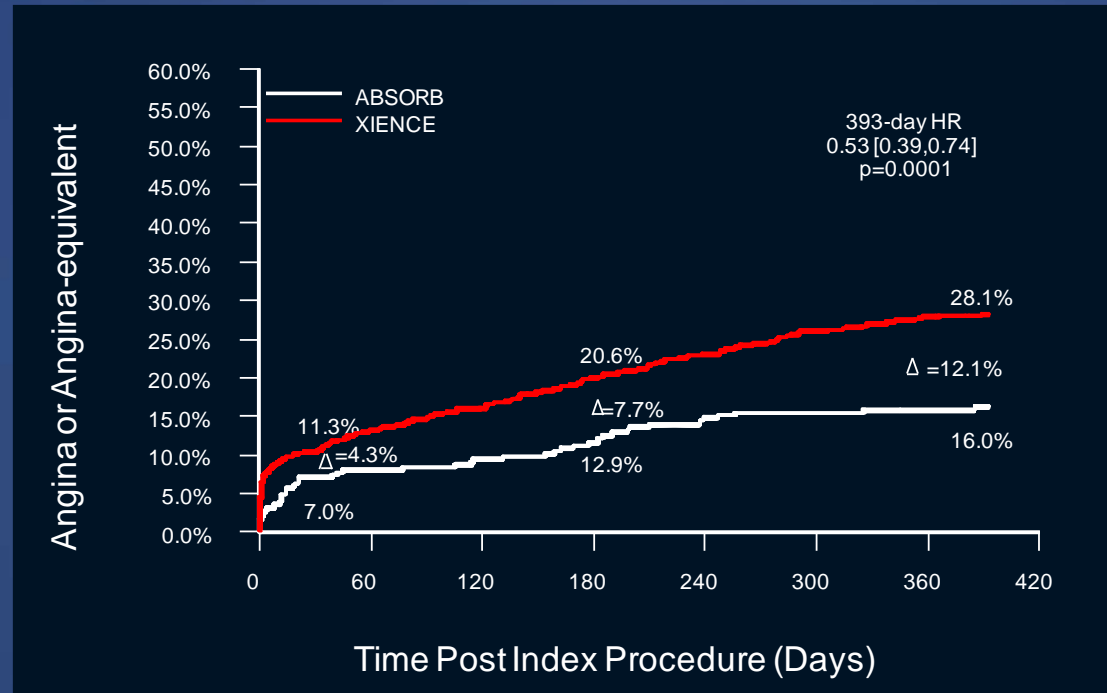

Time post-Index Procedure (days)	0	37	194	393
Absorb Subjects At Risk:	287	267	250	240
# Events	5	20	37	46
XIENCE Subjects At Risk:	602	535	478	429
# Events	26	68	124	169

# ABSORB EXTEND / XIENCE V

## Propensity Matched 1 Year Clinical Outcomes

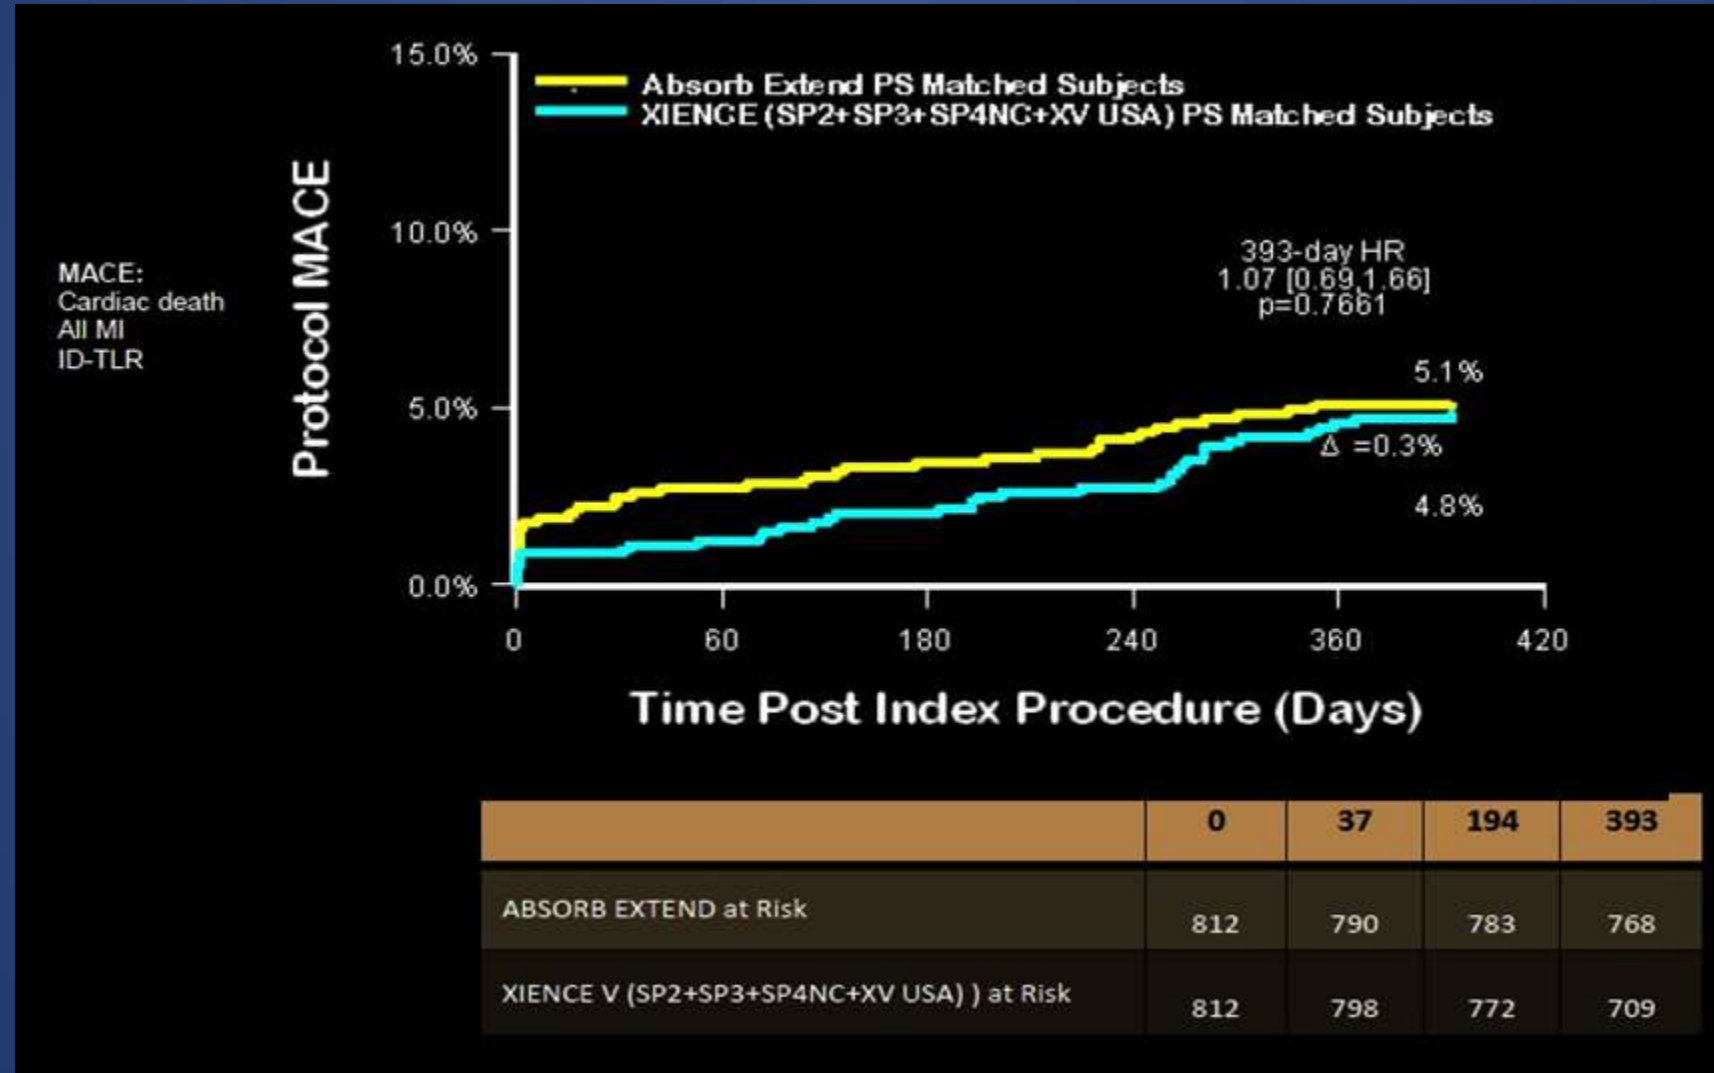


# ABSORB II RCT

**501 subjects**

(Randomized 2:1 Absorb versus XIENCE PRIME) Up to 40 European sites

## Clinical Follow-Up

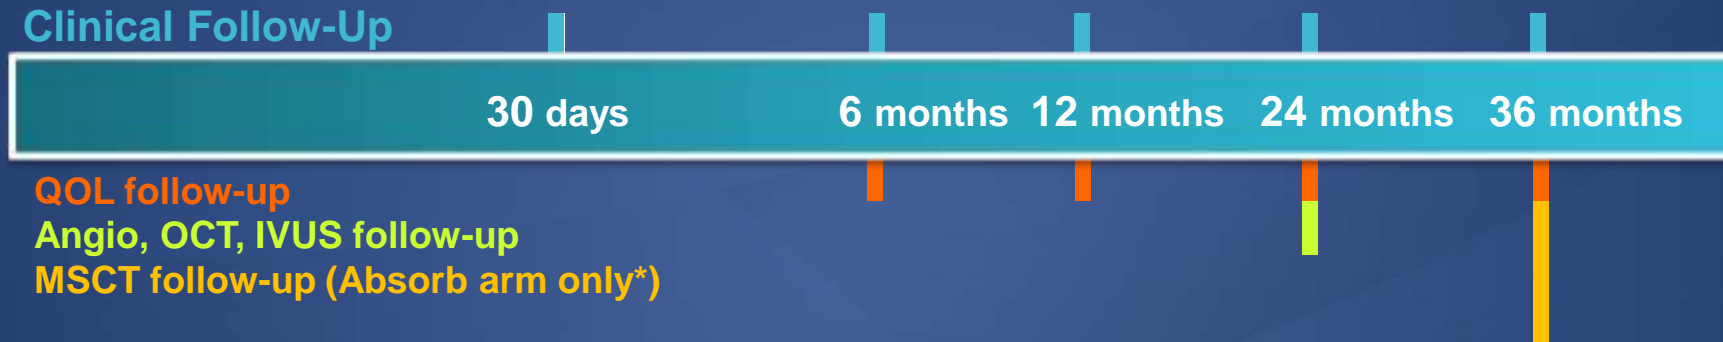

Study Objective	Randomized against XIENCE PRIME control. FPI 28-Nov-2011
Co-primary Endpoints	<ul style="list-style-type: none"><li>• Vasomotion assessed by change in Mean Lumen Diameter between pre- and post-nitrate at 2 years (superiority)</li><li>• Minimum Lumen Diameter (MLD) at 2 years post nitrate minus MLD post procedure post nitrate (non-inferiority, reflex to superiority)</li></ul>
Treatment	Up to 2 <i>de novo</i> lesions in different epicardial vessels Planned overlapping allowed in lesions $\leq 48$ mm

# ABSORB II


## One Year Clinical Results

	Absorb (N=335 patients)	XIENCE (N=166 patients)	P-value
<b>DoCE (Device-Oriented Composite Endpoint)</b>	<b>4.8</b>	<b>3.0</b>	<b>0.35</b>
Cardiac Death (%)	0	0	1.00
Target Vessel MI (%)	4.2	1.2	0.07
Clinically Indicated TLR (%)	1.2	1.8	0.69
All TLR (%)	1.2	1.8	0.69
Definite Scaffold/Stent Thrombosis (%)	0.6	0.0	1.00
<b>PoCE (Patient-Oriented Composite Endpoint)</b>	<b>7.3</b>	<b>9.1</b>	<b>0.47</b>
All Death (%)	0	0.6	0.33
All MI (%)	4.5	1.2	0.06
All NQMI (%)	3.9	1.2	0.16
All QMI (%)	0.6	0	1.00
All Revascularizations (%)	3.6	7.3	0.08



# ABSORB II

## One Year Angina Outcome

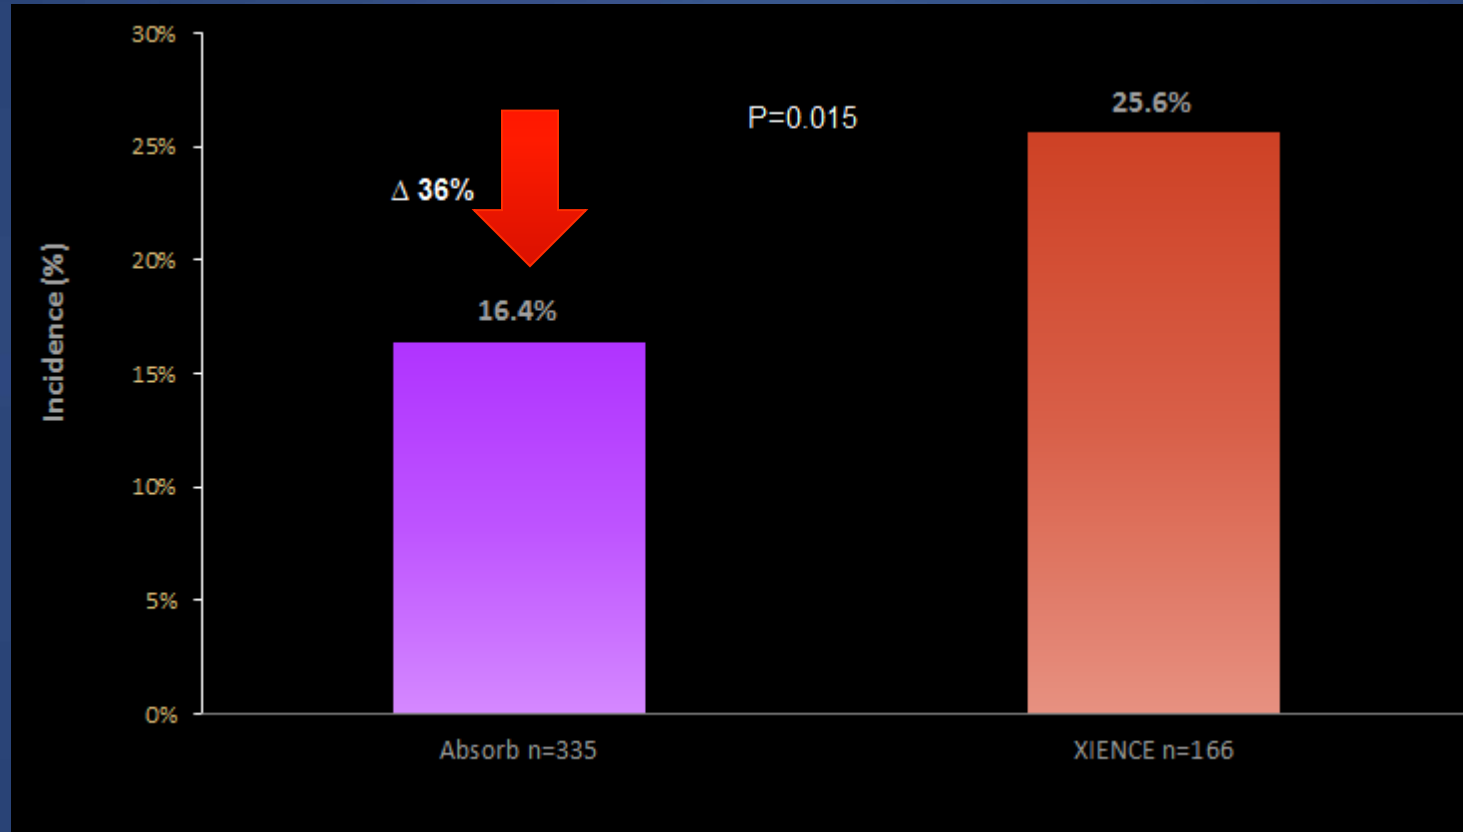

# ABSORB II 2-years

	2 years		
	Absorb BVS N=335	XIENCE N=166	p value
<b>Death* (%)</b>	<b>1.2</b>	<b>0.6</b>	<b>0.67</b>
Cardiac	0.6	0.0	0.55
Non cardiovascular	0.6	0.6	1.00
<b>Myocardial Infarction (%)</b>	<b>5.8</b>	<b>2.4</b>	<b>0.10</b>
Q-wave	1.5	0.6	0.67
Non Q-wave	4.3	1.8	0.16
<b>Definite/Probable ST* (%)</b>	<b>1.5</b>	<b>0.0</b>	<b>0.17</b>
Acute/sub-acute (0-30 days)	0.6	0.0	1.00
Late (31-365 days)	0.3	0.0	1.00
Very late (365 – 758 days)	0.6	0.0	0.55
<b>TLR (%)</b>	<b>2.7</b>	<b>1.8</b>	<b>0.76</b>
<b>NTL-TVR (%)</b>	<b>1.5</b>	<b>2.4</b>	<b>0.49</b>
<b>NTVR (%)</b>	<b>2.7</b>	<b>5.5</b>	<b>0.13</b>
<b>All revascularization</b>	<b>5.8</b>	<b>9.1</b>	<b>0.17</b>

# ABSORB II 2-years

	Absorb BVS N=335	XIENCE N=166	<i>p</i> value
PoCE (%)	11.6	12.8	0.70
MACE (%)	7.6	4.3	0.16
DoCE, TLF (%)	7.0	3.0	0.07
TVF (%)	8.5	6.7	0.48

**PoCE (Patient oriented Composite Endpoint):**

All death, all myocardial infarction, and all revascularisation

**MACE (Major Adverse Cardiac Events):**

Cardiac death, all myocardial infarction, and clinically indicated target-lesion revascularisation (TLR)

**DoCE (Device oriented Composite Endpoint)/ TLF (Target Lesion Failure):**


Cardiac death, target-vessel myocardial infarction, and clinically indicated target-lesion revascularisation (TLR)

**TVF (Target Vessel Failure):**

Cardiac death, all myocardial infarction, clinically indicated target-vessel revascularisation (TVR)

# ABSORB II 2-years


## Patient oriented Composite Endpoint (PoCE)

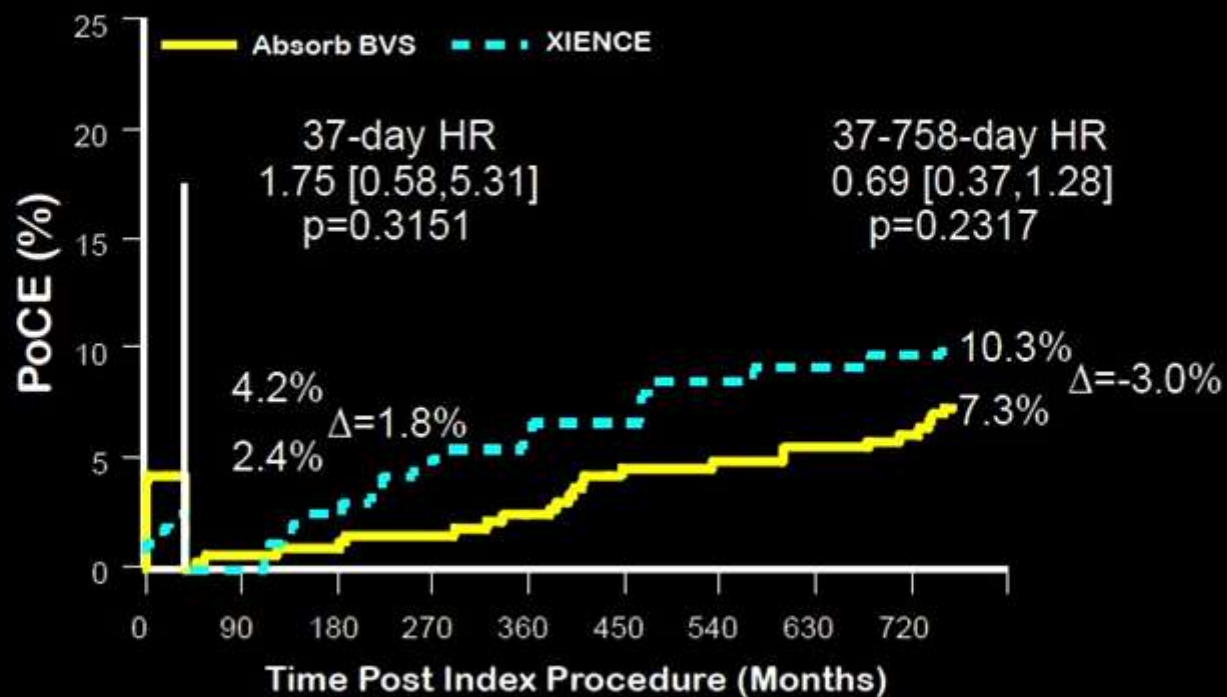

PoCE: All death, all myocardial infarction, and all revascularisation

# ABSORB II 2-years


Device oriented Composite Endpoint (DOCE)/  
Target Lesion Failure (TLF)

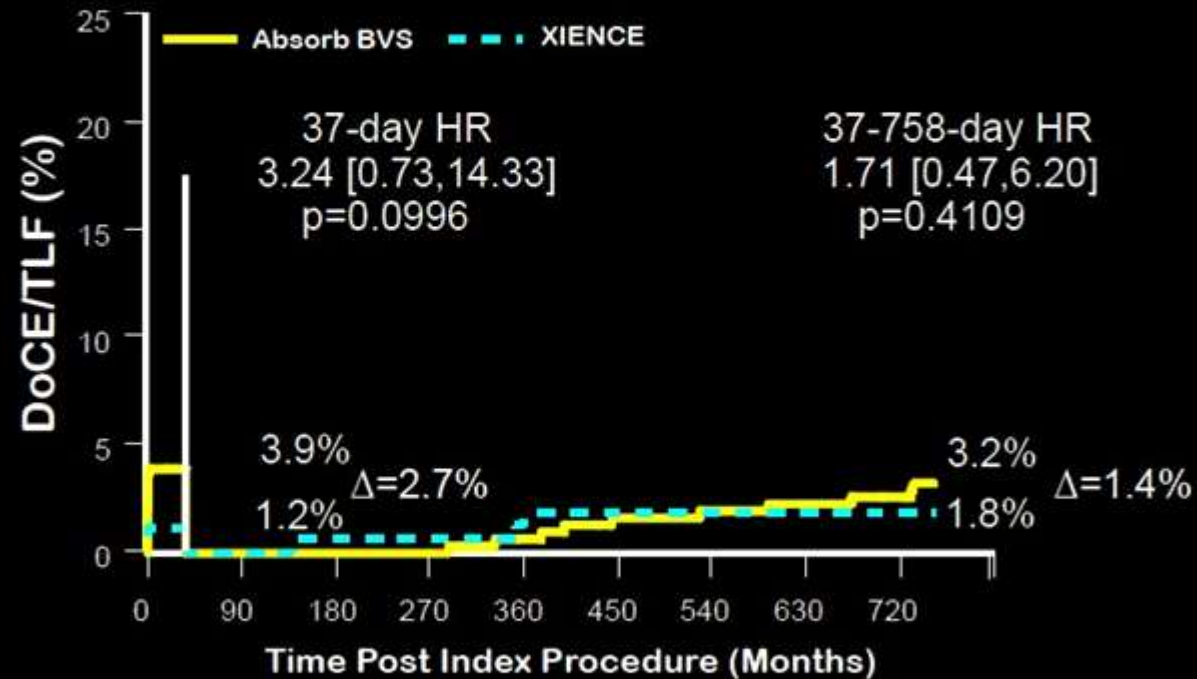

DoCE/TLF : Cardiac death, target-vessel myocardial infarction, and clinically indicated target-lesion revascularisation (TLR)

# ABSORB II 2-years

## Target Vessel Failure (TVF)

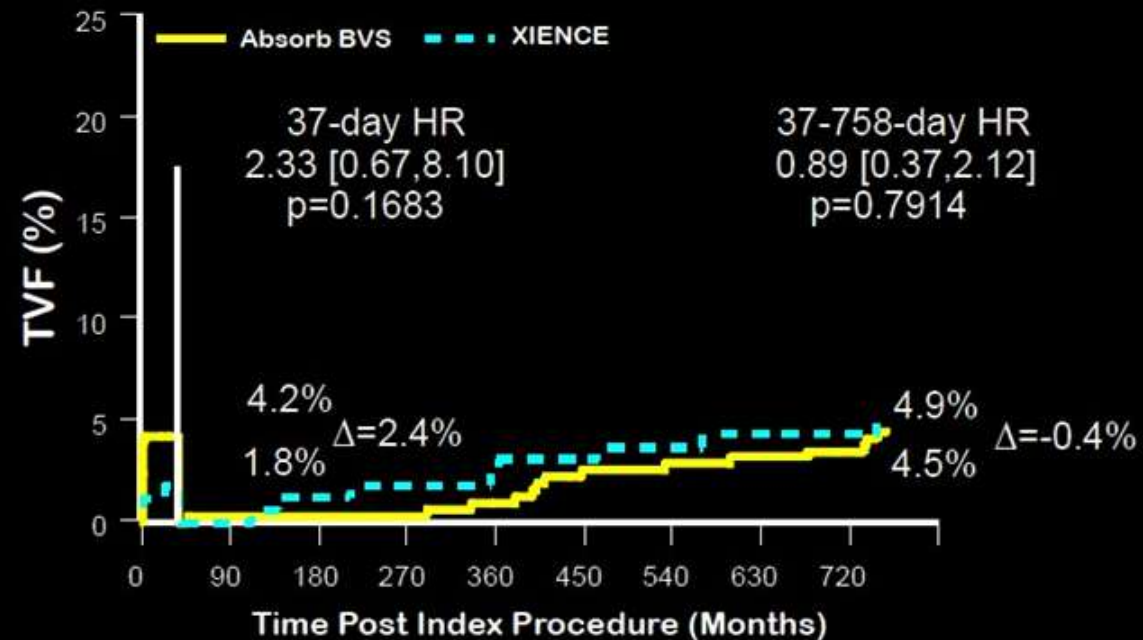


TVF : Cardiac death, all myocardial infarction, clinically indicated target-vessel revascularisation




# ABSORB II 3-years

Device-Oriented  
Composite Endpoints  
(Cardiac Death, TV-MI, CI-TLR)

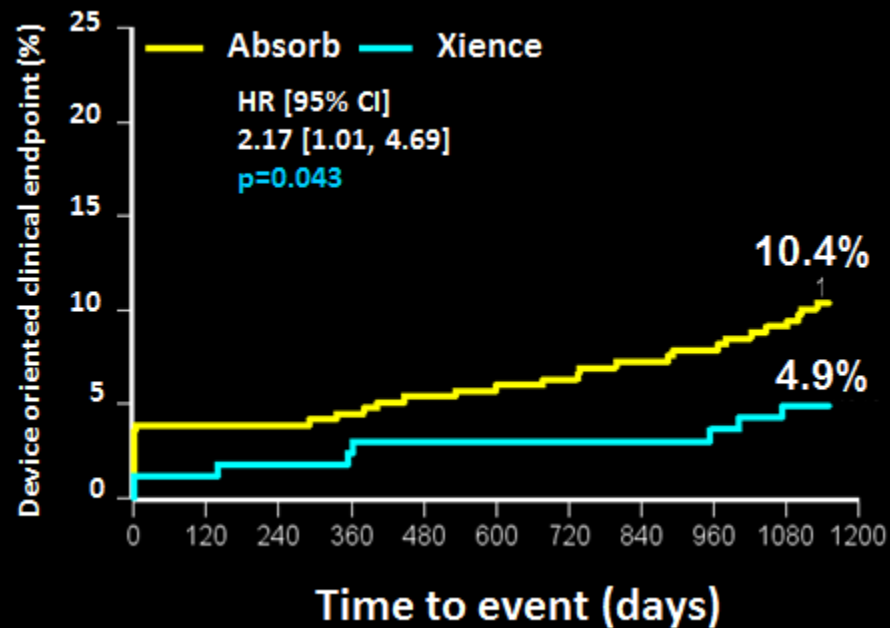

Patient-Oriented  
Composite Endpoints  
(Any Death, Any-MI,  
Any Revascularization)

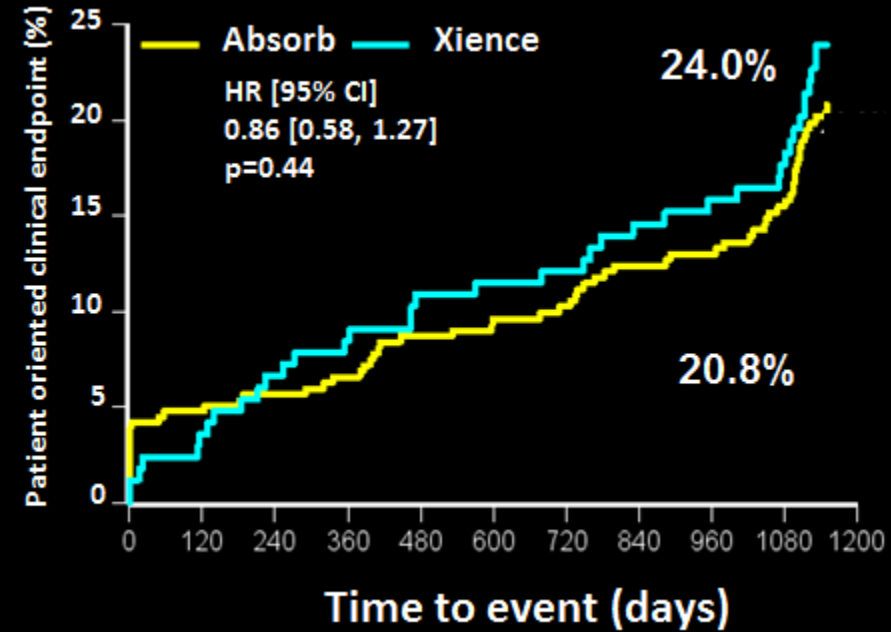

# ABSORB II 3-years

## *Scaffold or Stent Thrombosis*

	Absorb 335 patients	Xience 166 patients	p value
<b>Definite</b>	<b>2.5% (8)</b>	<b>0.0% (0)</b>	<b>0.06</b>
Acute (0–1 day)	0.3% (1)	0.0% (0)	1.0
Sub-acute (2–30 days)	0.3% (1)	0.0% (0)	1.0
Late (31–365 days)	0.0% (0)	0.0% (0)	1.0
Very late (>365 days)	1.8% (6)	0.0% (0)	0.19
<b>Definite or probable</b>	<b>2.8% (9/320)</b>	<b>0.0% (0/159)</b>	<b>0.03</b>
Acute (0–1 day)	0.3% (1)	0.0% (0)	1.0
Sub-acute (2–30 days)	0.3% (1)	0.0% (0)	1.0
Late (31–365 days)	0.3% (1)	0.0% (0)	1.0
Very late (>365 days)	1.8% (6)	0.0% (0)	0.19


# ABSORB II 3-years

## Secondary Clinical Endpoints

	Absorb 325 patients	Xience 161 patients	Relative Risk	p value
<b>Device-oriented composite endpoint [DOCE]</b>	<b>10.5%</b>	<b>5.0%</b>	<b>2.11 [1.00, 4.44]</b>	<b>0.04</b>
Cardiac death	0.9%	1.9%	0.50 [0.10, 2.43]	0.40
Target vessel MI	<b>7.1% (23)</b>	<b>1.2% (2)</b>	<b>5.70 [1.36, 23.87]</b>	<b>0.0061</b>
Periprocedural MI (WHO)	3.9%(13)	1.2% (2)	3.22 [0.74, 14.11]	0.16
Spontaneous MI (WHO extended)	3.1% (10)	0% (0)	NC [NC]	0.06
Clinically indicated TLR	<b>6.2%(20)</b>	<b>1.9% (3)</b>	<b>3.30 [1.00, 10.95]</b>	<b>0.036</b>
<b>Patient-oriented composite endpoint [POCE]</b>	<b>20.9%</b>	<b>24.2%</b>	<b>0.86 [0.61, 1.22]</b>	<b>0.40</b>
All-cause death	2.5%	3.7%	0.66 [0.23, 1.87]	0.57
<b>Any MI</b>	<b>8.3%</b>	<b>3.1%</b>	<b>2.68 [1.05, 6.82]</b>	<b>0.03</b>
Any revascularization	15.1%	20.5%	0.74 [0.49, 1.10]	0.13

# ABSORB II 3-years

## In-device Vasomotion

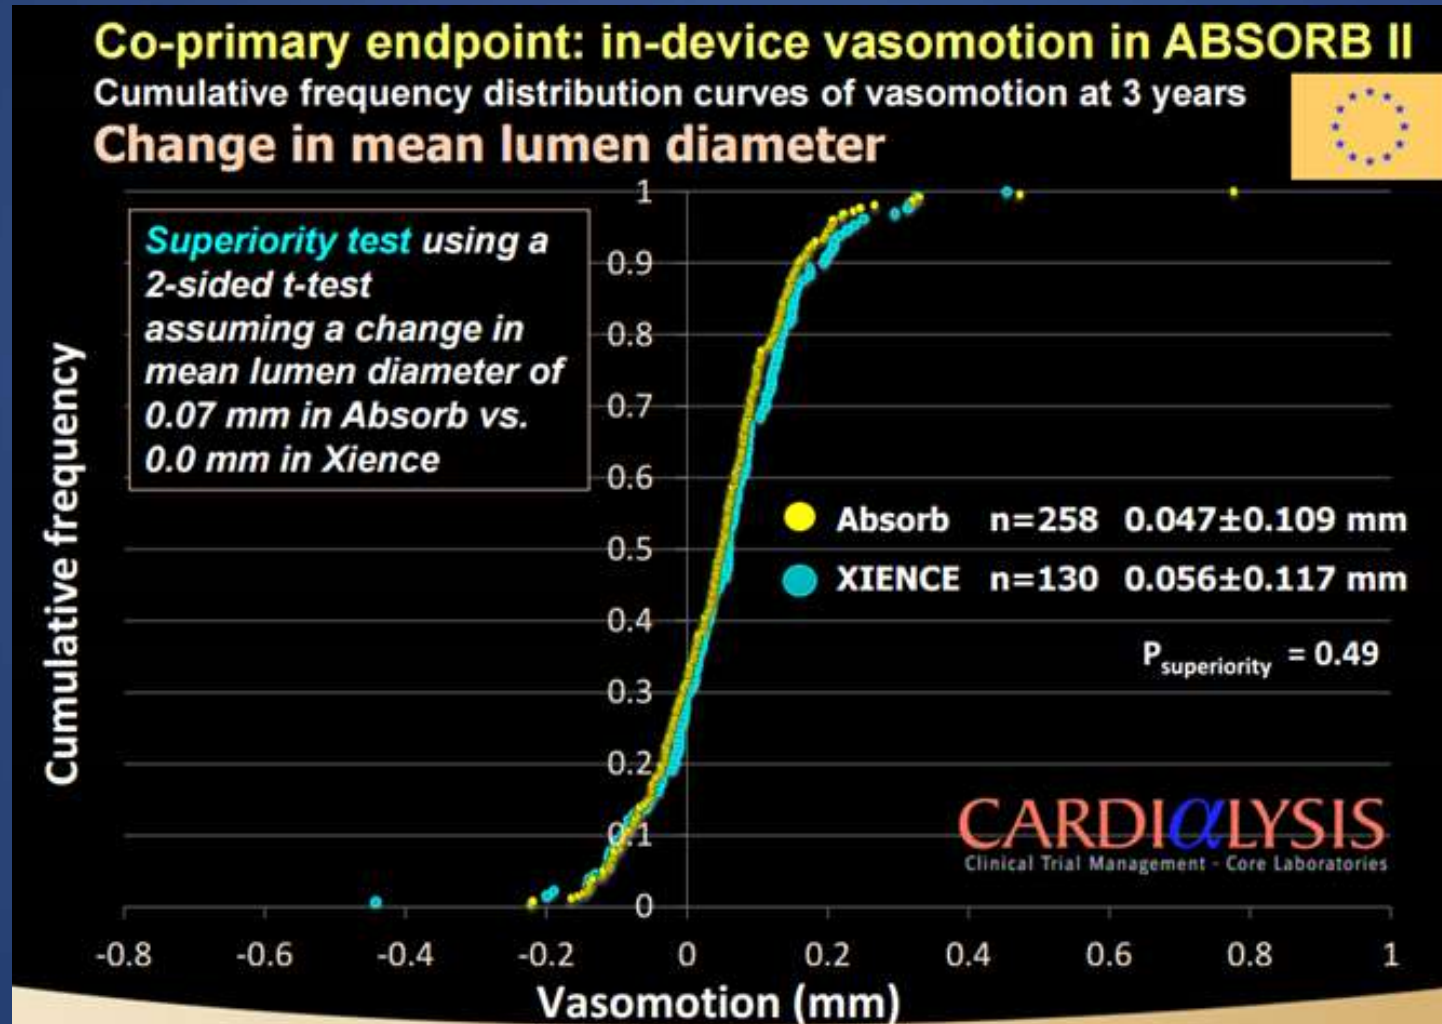


# ABSORB II 3-years

## Radial Strength


### Recoil and acute gain in Absorb II

Acute gain was smaller in Absorb than Xience on QCA and IVUS.

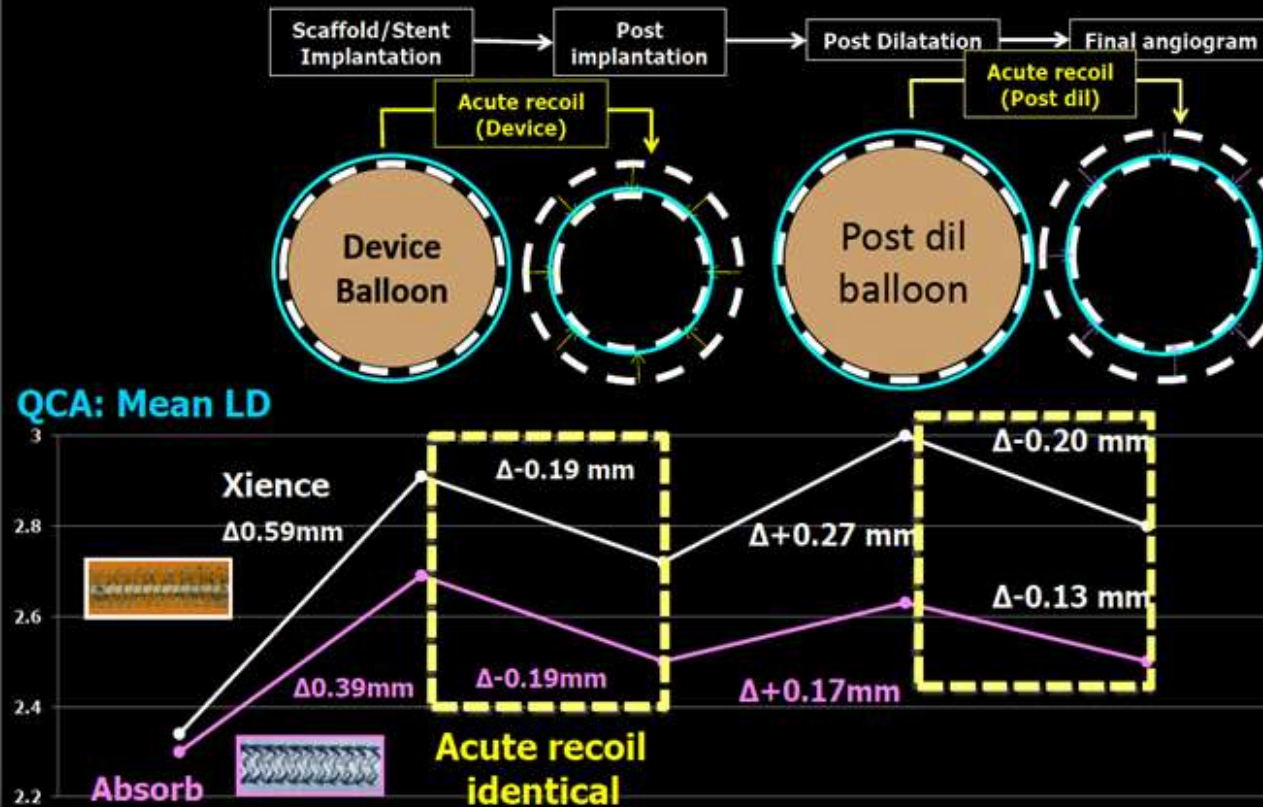

# ABSORB II 4-years

Device-oriented Composite Endpoint (DoCE) at 4 Years  
Target Lesion Failure (TLF)

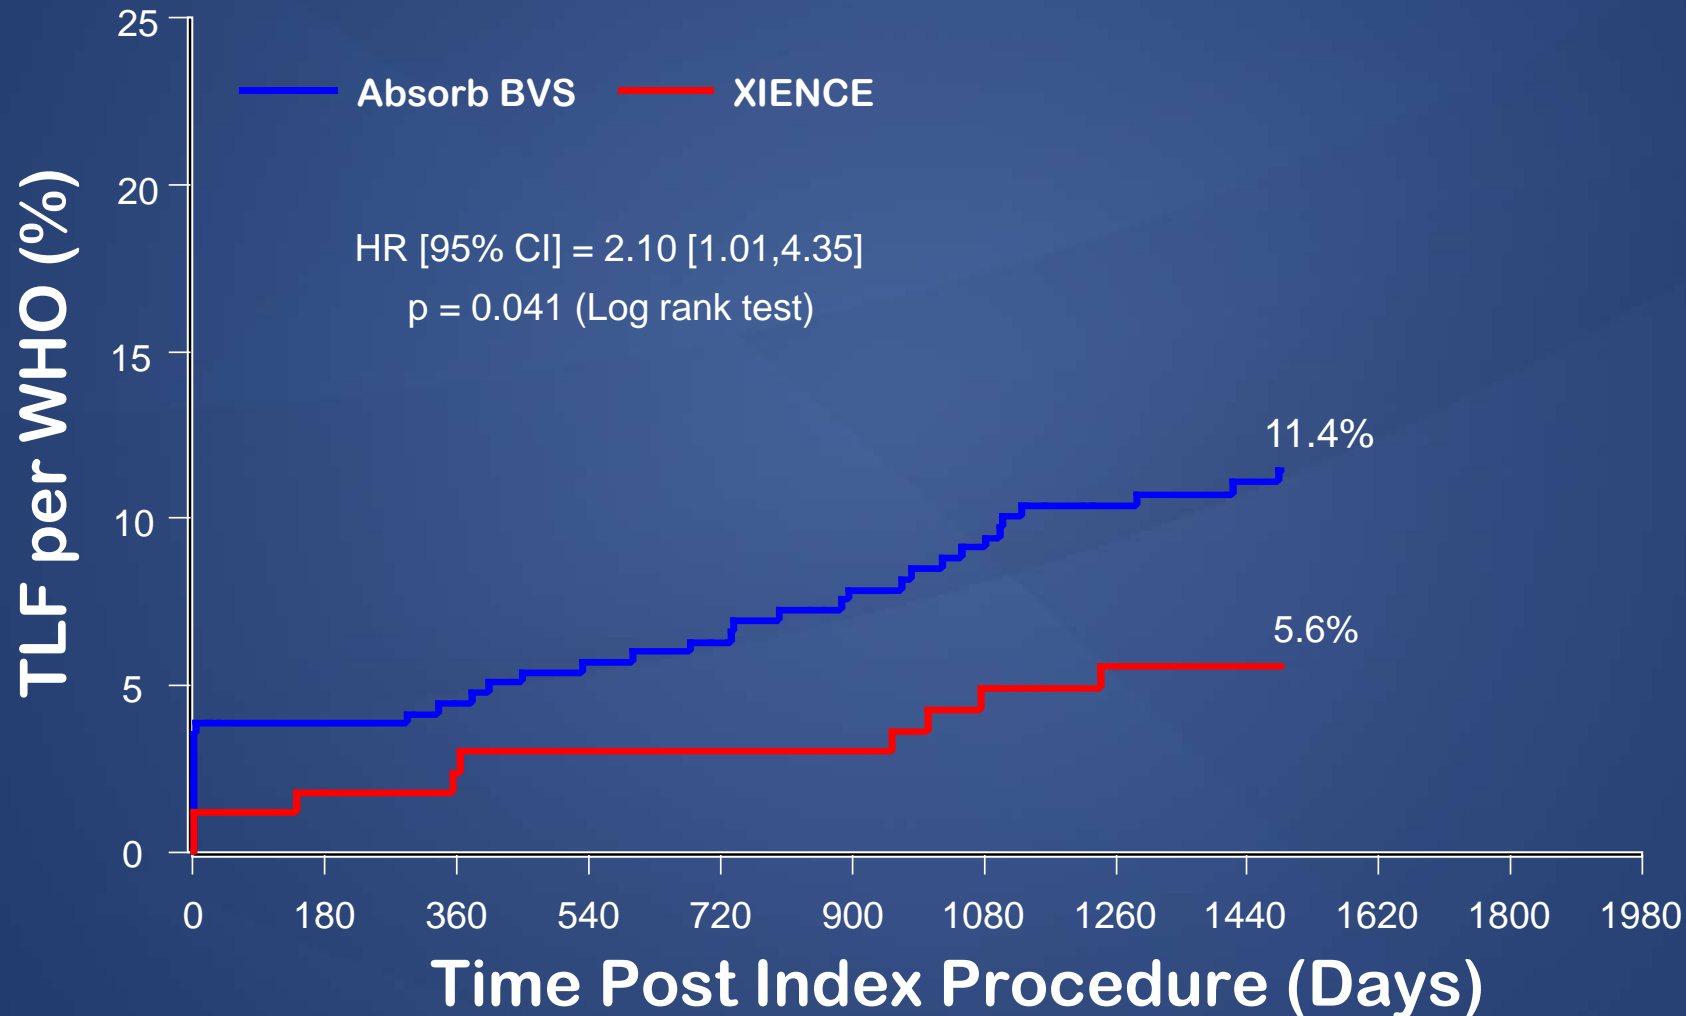


CI=confidence interval, DoCE=device-oriented composite endpoint, HR=hazard ratio, TLF=target lesion failure, WHO=World Health Organization



# ABSORB II 5-years

## Device-oriented Composite Endpoint (DoCE) at 5 Years Target Lesion Failure (TLF)

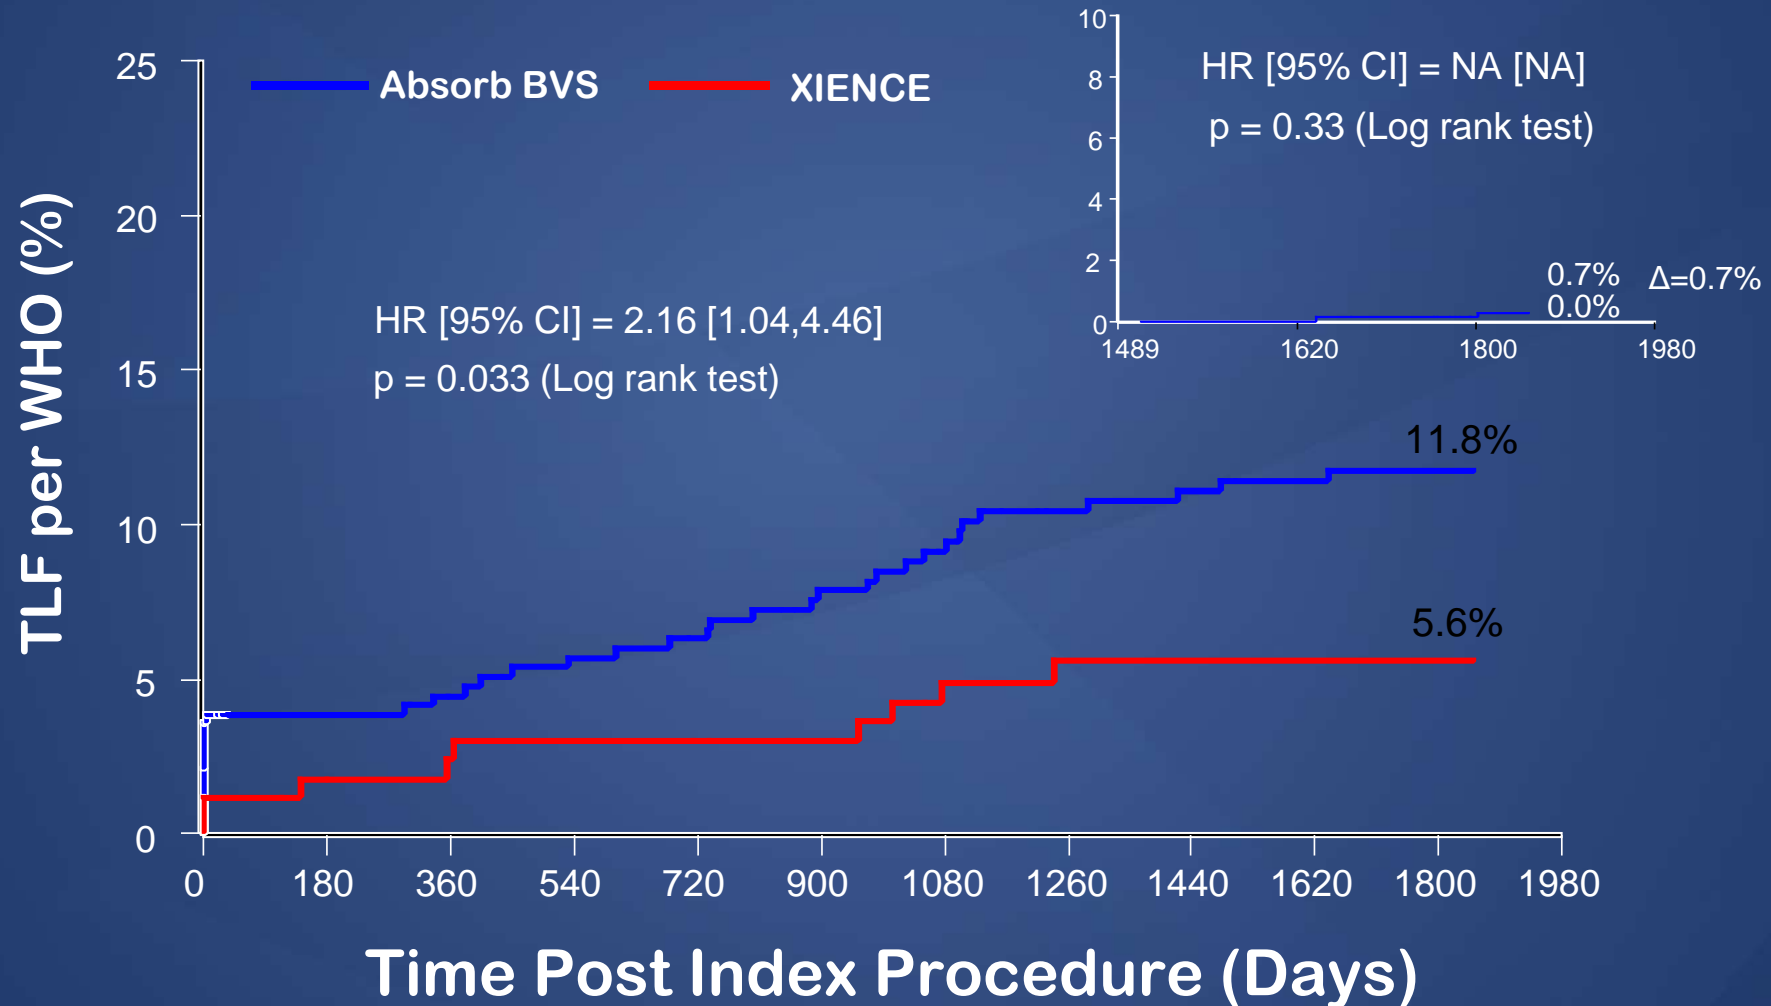


DoCE/TLF : Cardiac death, target-vessel myocardial infarction, and clinically indicated target-lesion revascularisation (TLR)

CI=confidence interval, DoCE=device-oriented composite endpoint, HR=hazard ratio,  
TLF=target lesion failure, WHO=world health organization

# ABSORB II 4-years


Patient-oriented Composite Endpoint at 4 Years  
(PoCE) / DMR

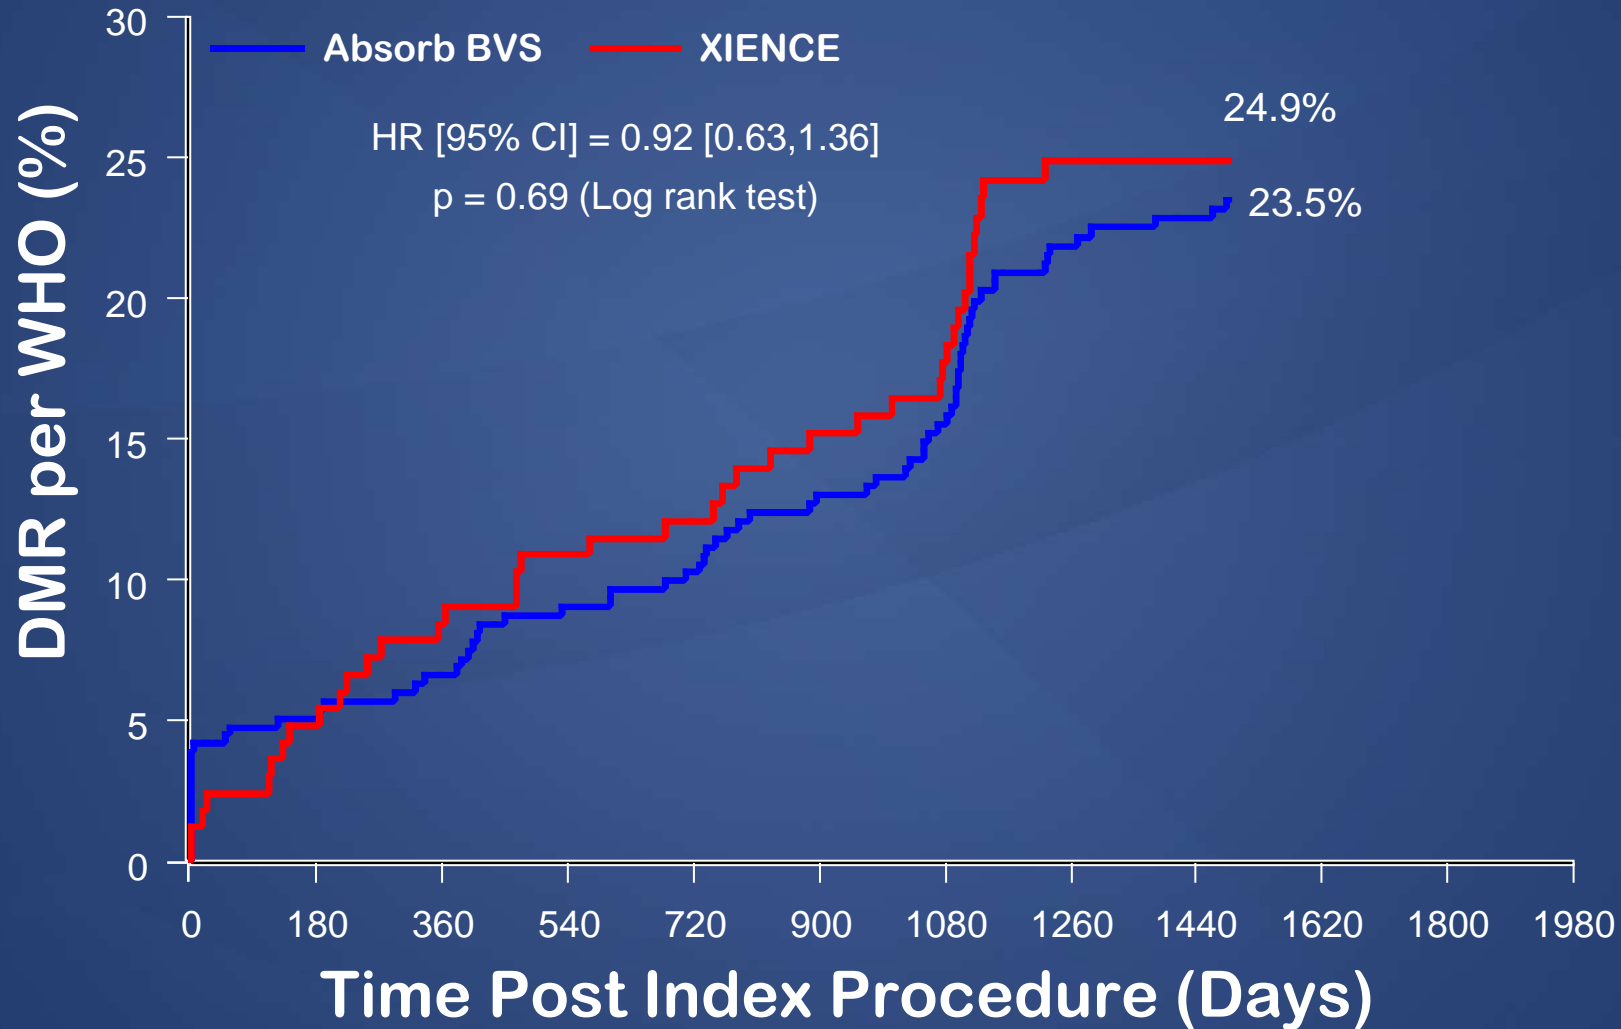

CI=confidence interval, HR=hazard ratio, PoCE=DMR: All Death, all Myocardial infarction, and all Revascularization, WHO=World Health Organization

# ABSORB II 5-years

Patient-oriented Composite Endpoint at 5 Years  
(PoCE) / DMR

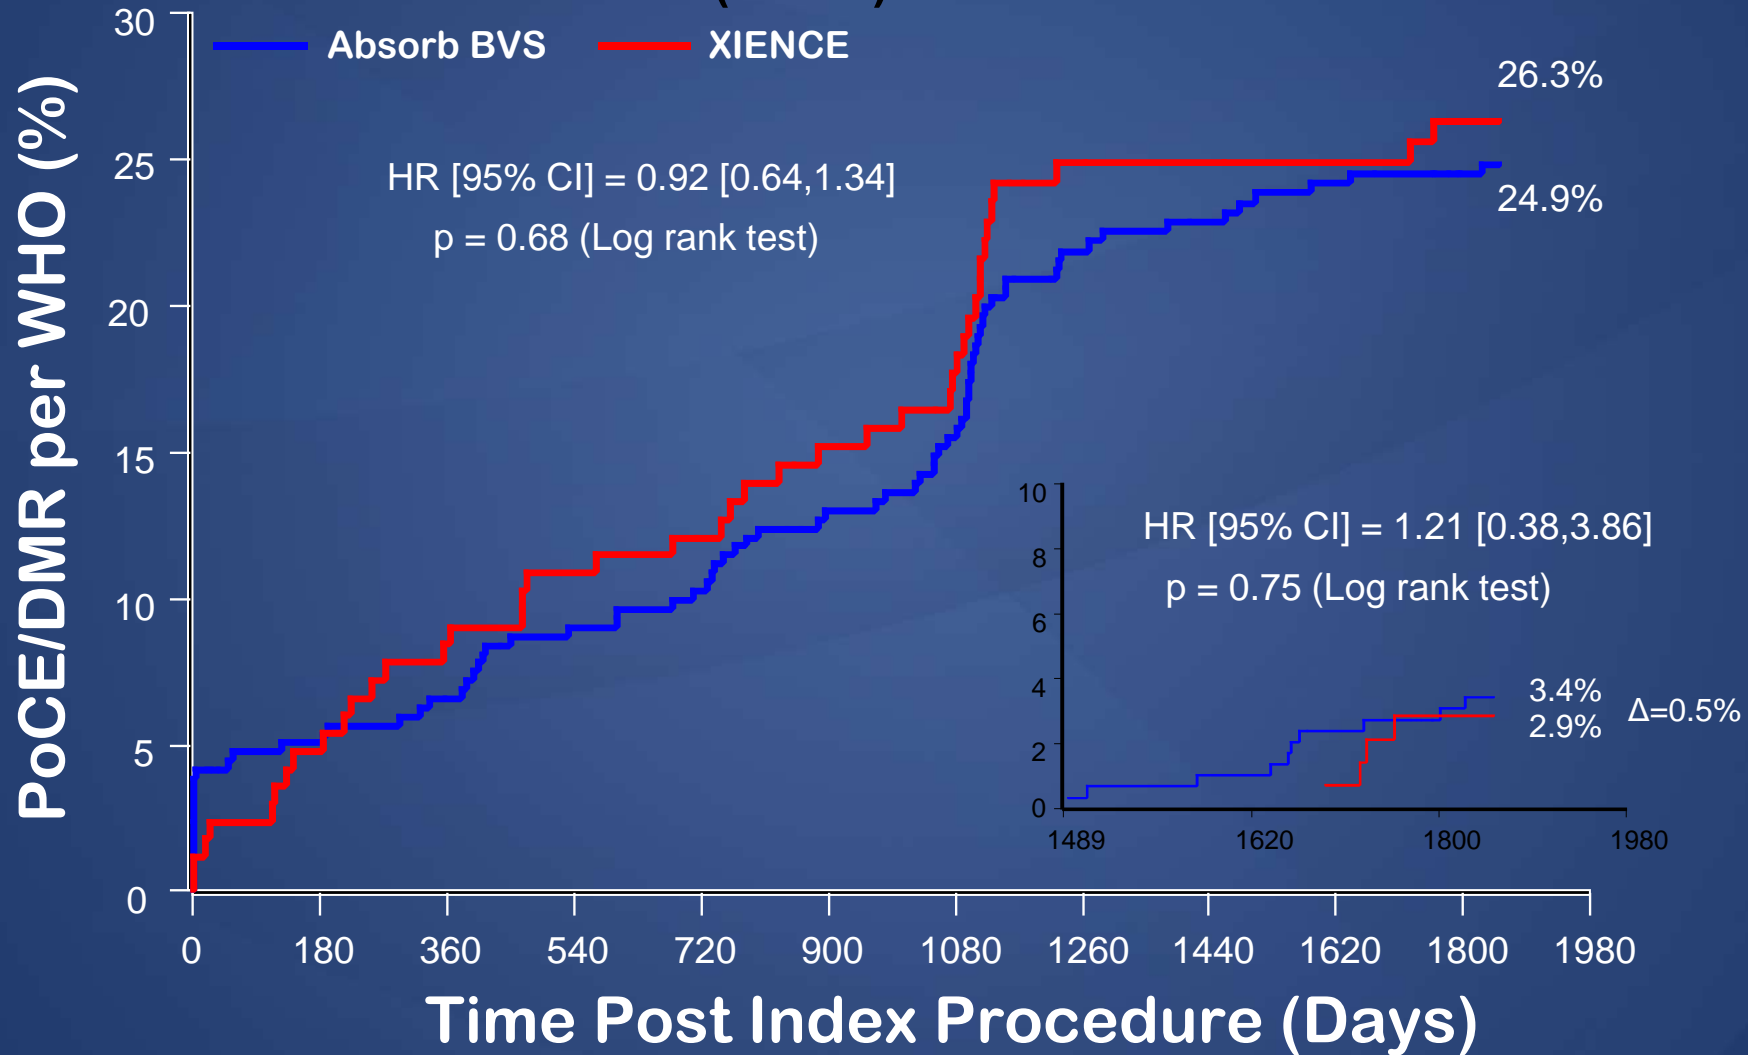

# ABSORB II 5-years

## Clinical Outcomes Composite Endpoints at 5 Years

	Absorb BVS N=335	XIENCE N=166	<i>p</i> value
<b>PoCE (%)</b>	26.3	28.6	0.6132
<b>MACE (%)</b>	13.5	8.8	0.1545
<b>DoCE, TLF (%)</b>	12.5	6.1	0.0377
<b>TVF (%)</b>	15.5	15.0	0.8912

**PoCE (Patient-oriented Composite Endpoint):**

All death, all myocardial infarction, and all revascularisation

**MACE (Major Adverse Cardiac Events):**

Cardiac death, all myocardial infarction, and clinically indicated target-lesion revascularisation (TLR)

**DoCE (Device-oriented Composite Endpoint)/ TLF (Target Lesion Failure):**


Cardiac death, target-vessel myocardial infarction, and clinically indicated target-lesion revascularisation (TLR)

**TVF (Target Vessel Failure):**

Cardiac death, all myocardial infarction, clinically indicated target-vessel revascularisation (TVR)

# ABSORB II 4-years


Definite/Probable Scaffold/Stent Thrombosis\* at 4 Years

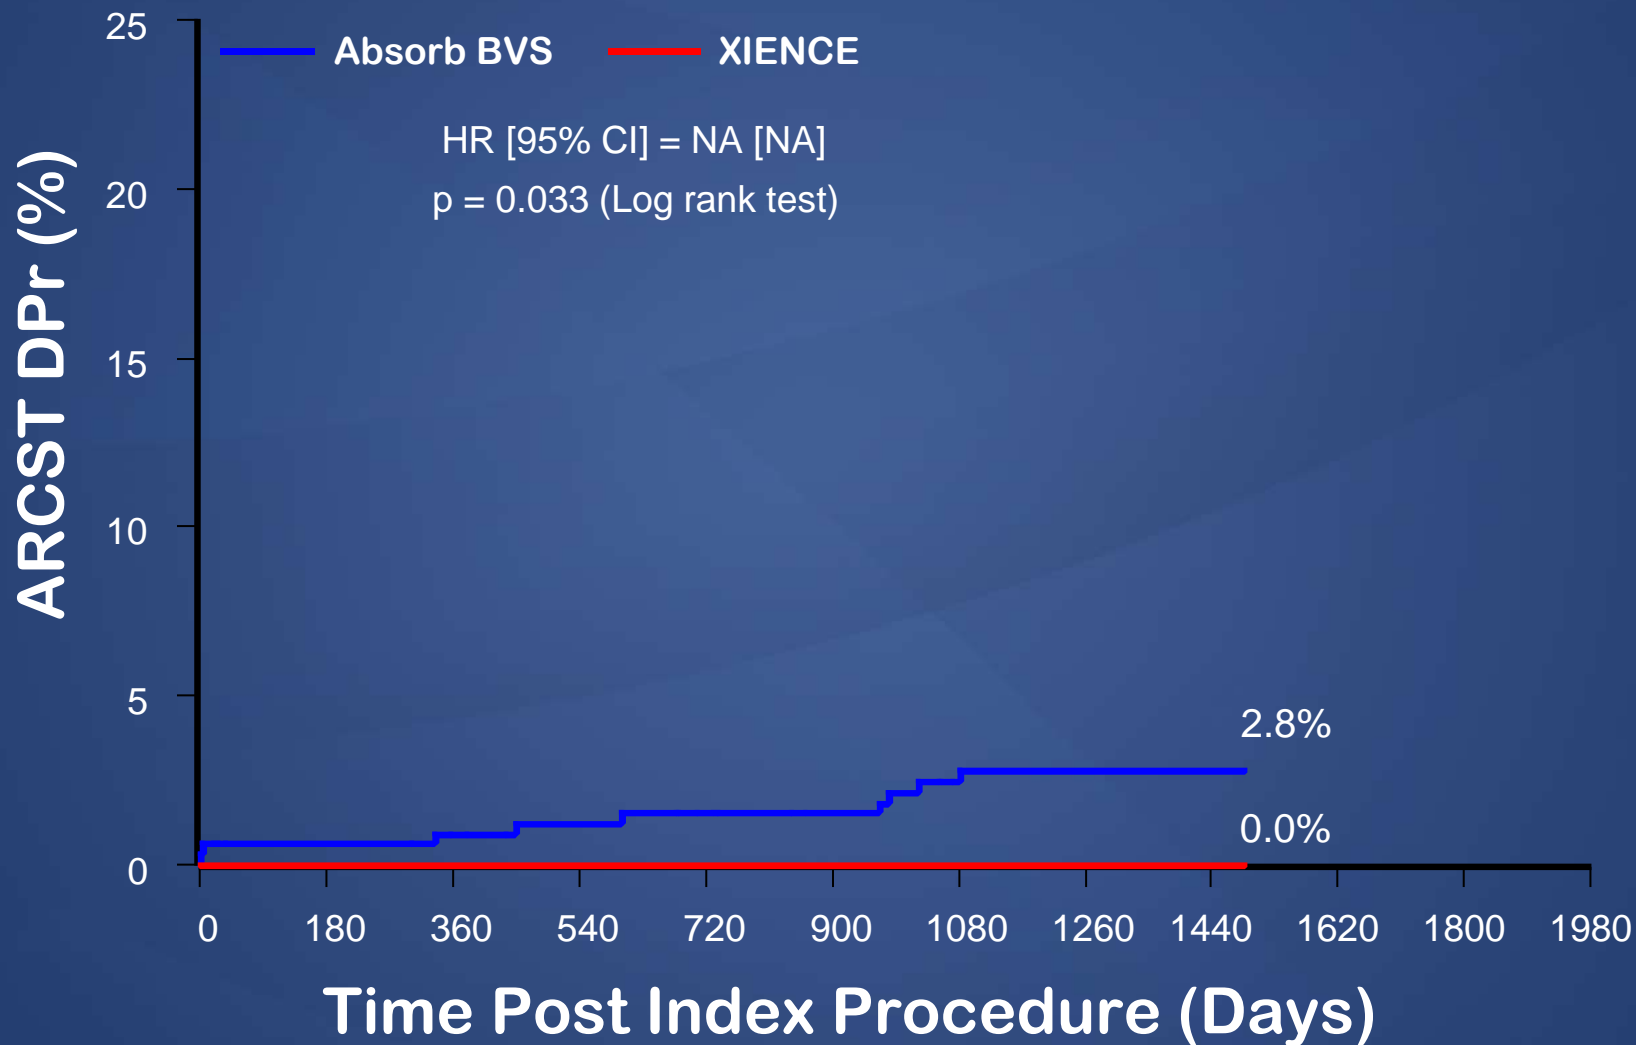

ARCST=academic research consortium scaffold/stent thrombosis, CI=confidence interval,  
DPr=definite/probable, HR=hazard ratio, NA=not applicable

# ABSORB II 5-years

Definite/Probable Scaffold/Stent Thrombosis\* at 5 Years

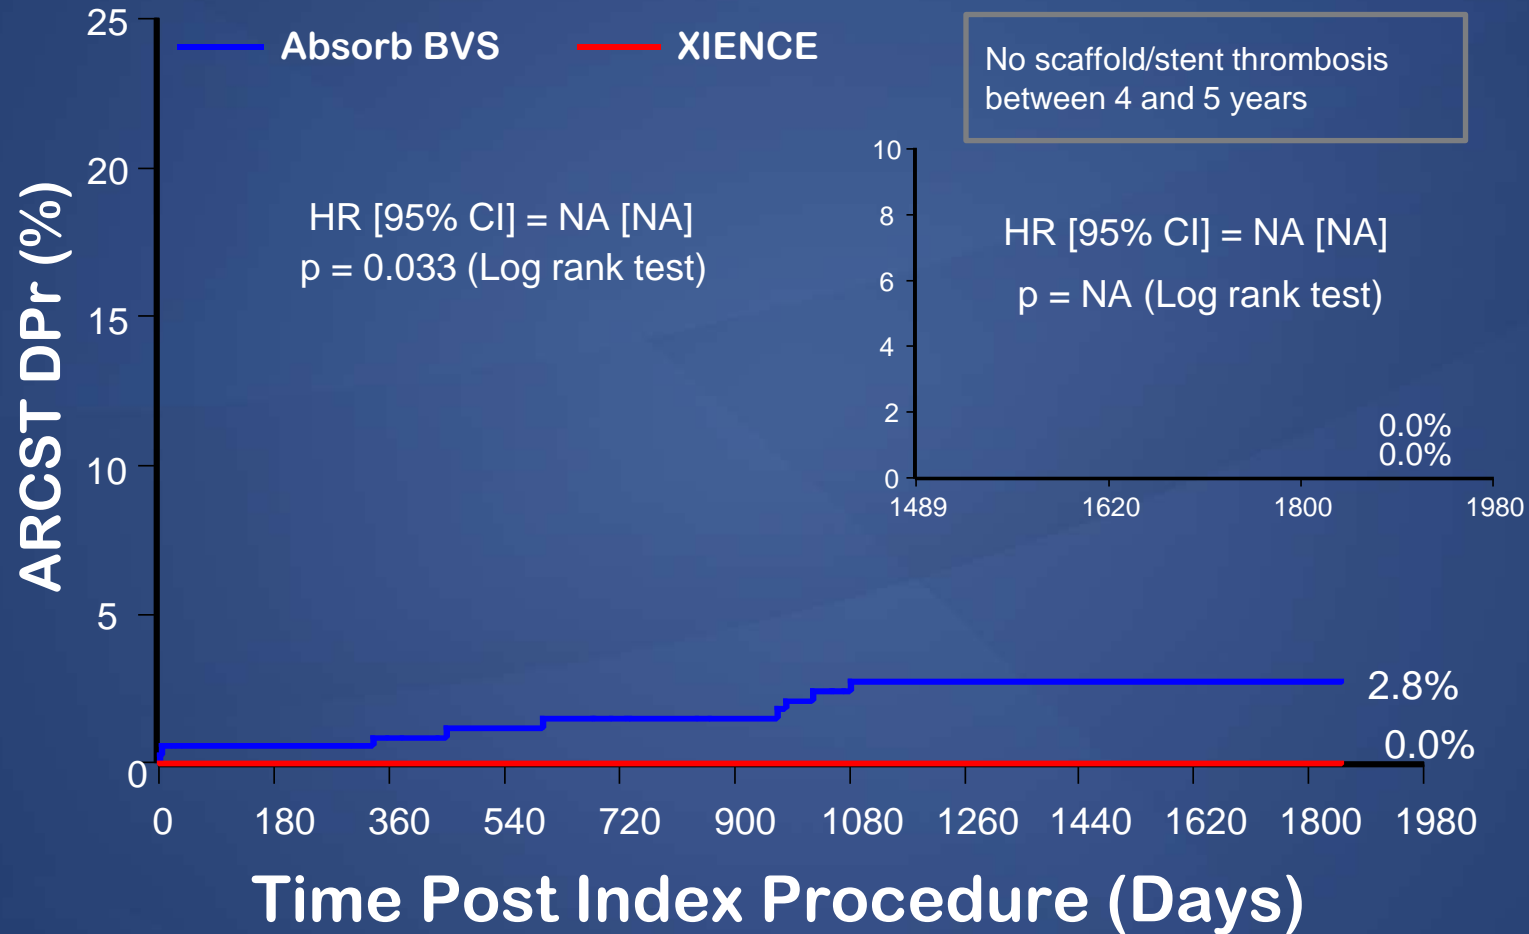


ARCST=academic research consortium scaffold/stent thrombosis, CI=confidence interval, DPR=definite/probable, HR=hazard ratio, NA=not applicable



# ABSORB III RCT

~2250 subjects in up to 220 sites (predominantly US)  
 Lead-in (n≤50); Clinical (n~2000); Imaging (n~200)  
 PI: Dean Kereiakes, Steve Ellis; Chairman: Gregg Stone

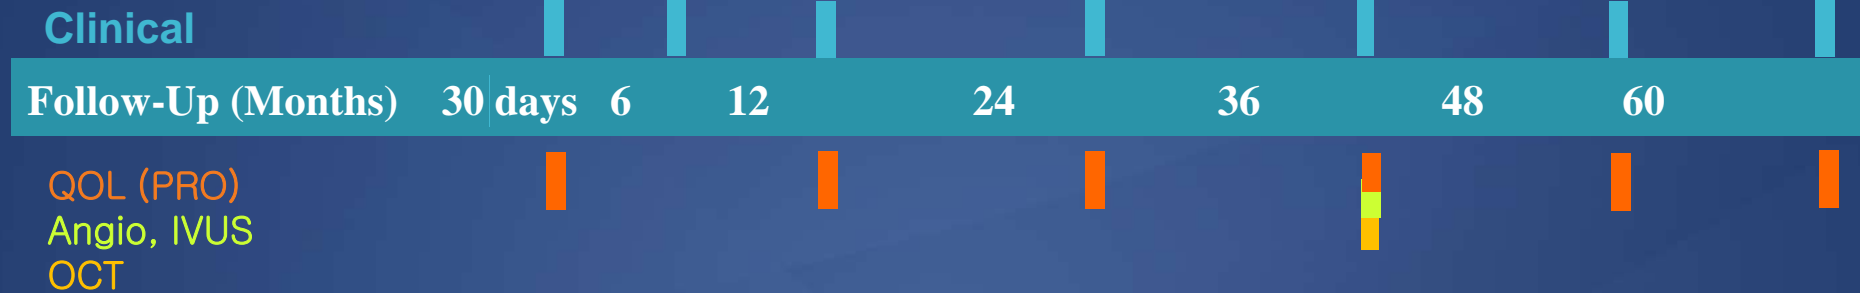

<b>Study Objective</b>	Randomized against XIENCE control. 2:1. FPI Lead-in 28 Dec 201230
<b>Primary Endpoint</b>	Target Lesion Failure at 1 year, non-inferiority to XIENCE (n~2000)
<b>Major Secondary Endpoints</b>	<ul style="list-style-type: none"> <li>Vasomotion assessed by change in angiographic Mean Lumen Diameter between pre- and post-nitrate at 3 years (superiority)</li> <li>Change in Mean Lumen Area by IVUS, from post-procedure to 3 years (Mean Lumen Area measured post-nitrate, superiority)</li> </ul>
<b>Treatment</b>	Up to 2 <i>de novo</i> lesions in different epicardial vessels, Lesion lengths $\leq 24$ mm, RVD $\geq 2.5$ mm and $\leq 3.75$ mm

# ABSORB III

## Baseline Characteristics

Characteristic	Absorb (N=1322)	Xience (N=686)	p-value
Age (mean)	63.5 ±10.6	63.6±10.3	0.75
Male	70.7%	70.1%	0.80
Race (Caucasian)	87.1%	88.3%	0.44
Current tobacco use	21.3%	20.7%	0.77
Hypertension	84.9%	85.0%	0.95
Dyslipidemia	86.2%	86.3%	0.97
Diabetes	31.5%	32.7%	0.60
Insulin-treated	10.5%	11.2%	0.60
Prior MI	21.5%	22.0%	0.79
Prior coronary intervention	38.7%	38.0%	0.75
Stable angina	57.3%	60.8%	0.13
Unstable angina	26.9 %	24.5%	0.25
Silent ischemia	10.0%	10.2%	0.88
Single vessel disease	69.5%	67.2%	0.29

# ABSORB III

## Angiographic Characteristics

Characteristic	Absorb (N=1322) (L=1385)	Xience (N=686) (L=713)	p-value
ACC/AHA lesion class B2/C	68.7%	72.5%	0.08
# of target lesions treated	1.0 ± 0.2	1.0 ± 0.2	0.38
One	95.1%	96.1%	0.32
Two	4.8%	3.9%	0.36
Target lesion			
LAD	44.5%	42.2%	0.31
RCA	29.2%	27.2%	0.35
Circumflex	26.2%	30.6%	0.03
Lesion length, mm	12.60 ± 5.41	13.12 ± 5.82	0.05
RVD, mm	2.67 ± 0.45	2.65 ± 0.46	0.36
RVD <2.25 mm	18%	19%	0.39
MLD, mm	0.92 ± 0.37	0.90 ± 0.34	0.11
%DS	65.3 ± 12.5	65.9 ± 11.7	0.24

# ABSORB III

## Procedural Characteristics

Characteristic	Absorb (N=1322) (L=1385)	Xience (N=686) (L=713)	p-value
Per Subject			
Bivalirudin use	60.7%	58.7%	0.39
GP IIb/IIIa inhibitor use	10.1%	12.4%	0.11
Only unassigned devices implanted	4.4%	0.6%	<0.001
Unplanned overlapping devices	6.2%	8.5%	0.06
Post-dilatation performed	65.5%	51.2%	<0.001
Intravascular imaging guidance	11.2%	10.8%	0.81
Procedure duration (min)	42.2 ± 23.1	38.3 ± 20.9	<0.001
Per Lesion			
Total study device length (mm)	20.5 ± 7.2	20.7 ± 9.0	0.56
Max device/balloon diameter (mm)	3.18 ± 0.43	3.12 ± 0.45	0.007
Max device/balloon to vessel diameter ratio	1.21 ± 0.15	1.19 ± 0.14	0.05
Maximum device/balloon pressure (atm.)	15.4 ± 3.0	15.4 ± 3.2	0.83




# ABSORB III

## Postprocedural QCA

Measurement	Absorb (N=1322) (L=1385)	Xience (N=686) (L=713)	p-value
RVD	2.70 ± 0.45	2.68 ± 0.47	0.33
In-Device			
MLD	2.37 ± 0.40	2.49 ± 0.40	<0.0001
Acute gain	1.45 ± 0.45	1.59 ± 0.44	<0.0001
%DS	11.6 ± 8.77	6.4 ± 8.91	<0.0001
In-Segment			
MLD	2.15 ± 0.41	2.14 ± 0.43	0.58
Acute gain	1.23 ± 0.46	1.24 ± 0.44	0.50
%DS	20.0 ± 7.94	19.8 ± 8.20	0.55

# ABSORB III


## Primary Endpoint-TLF

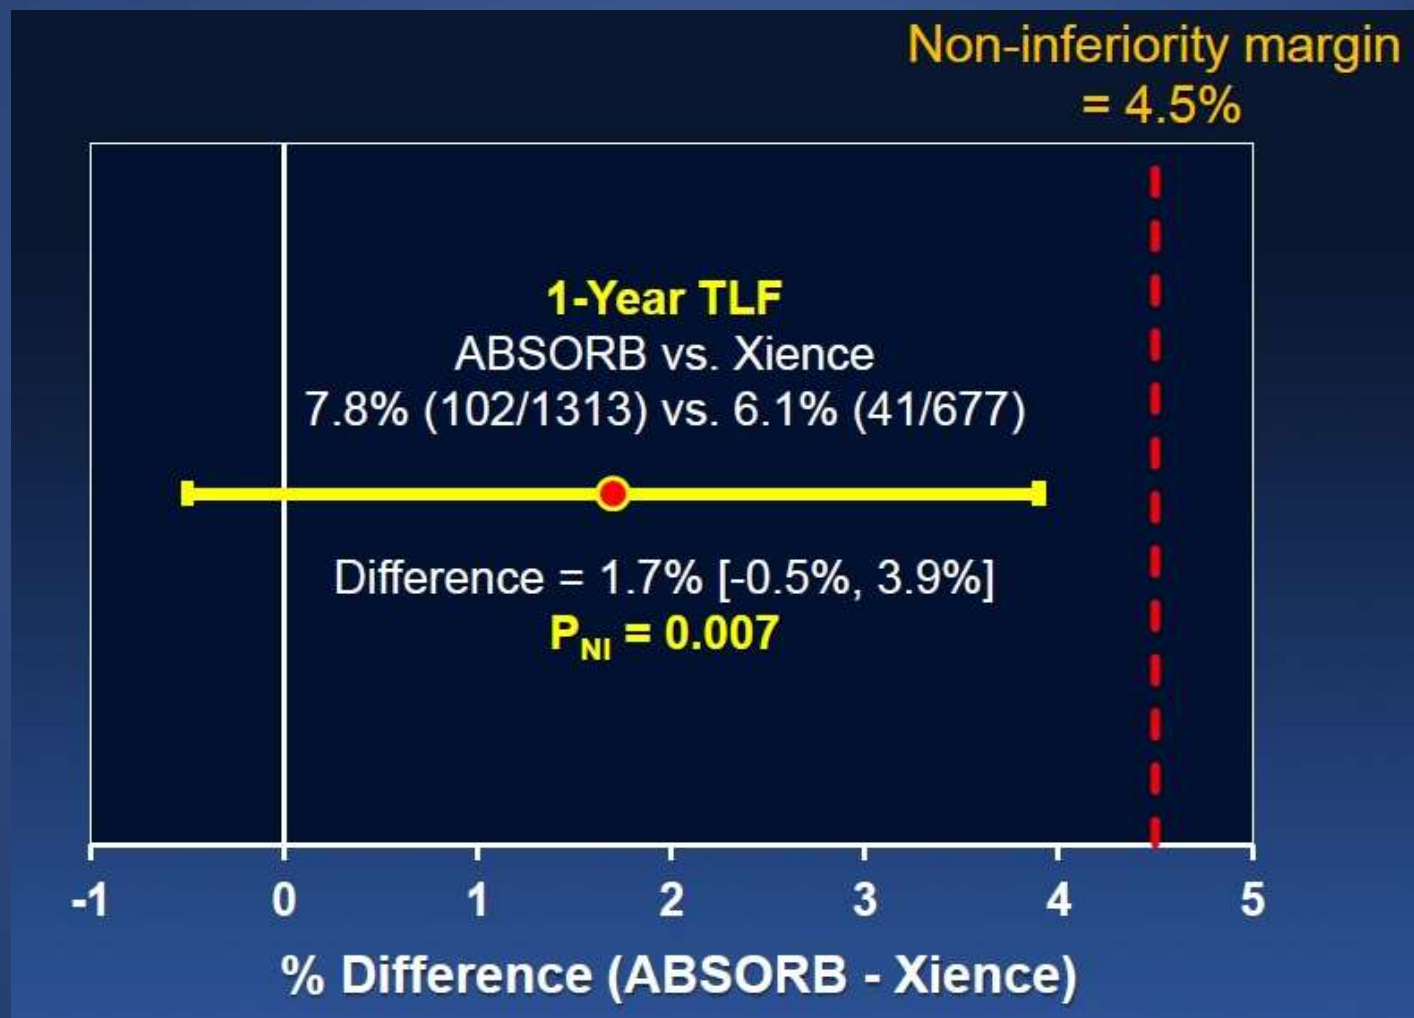




# ABSORB III

## Primary Endpoint-TLF

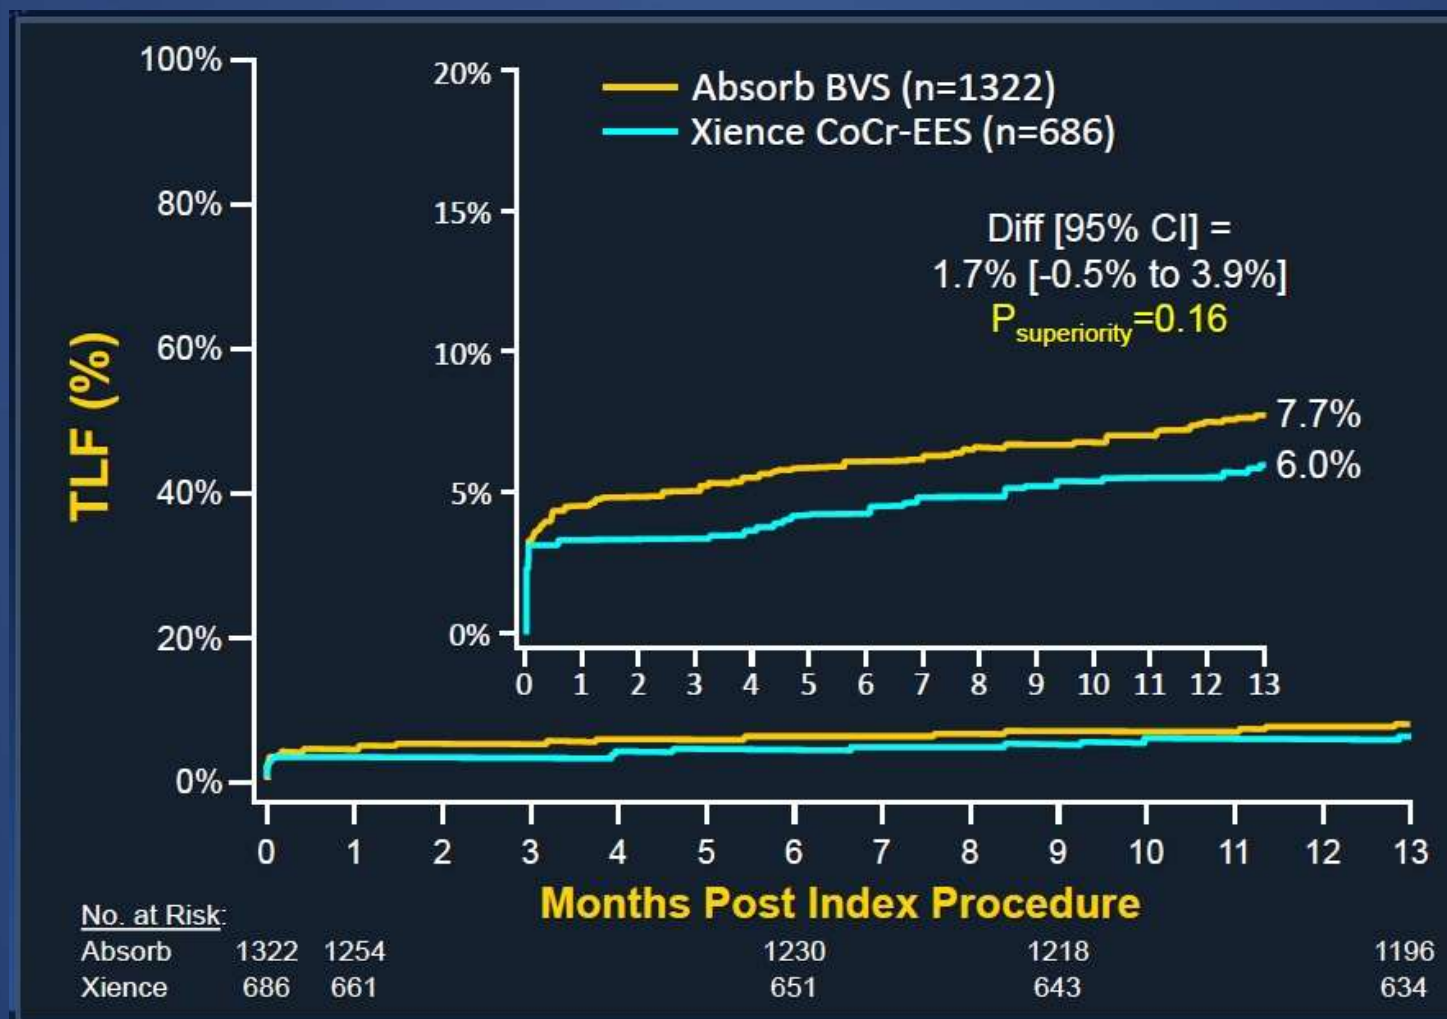


# ABSORB III

## Primary Endpoint-TLF

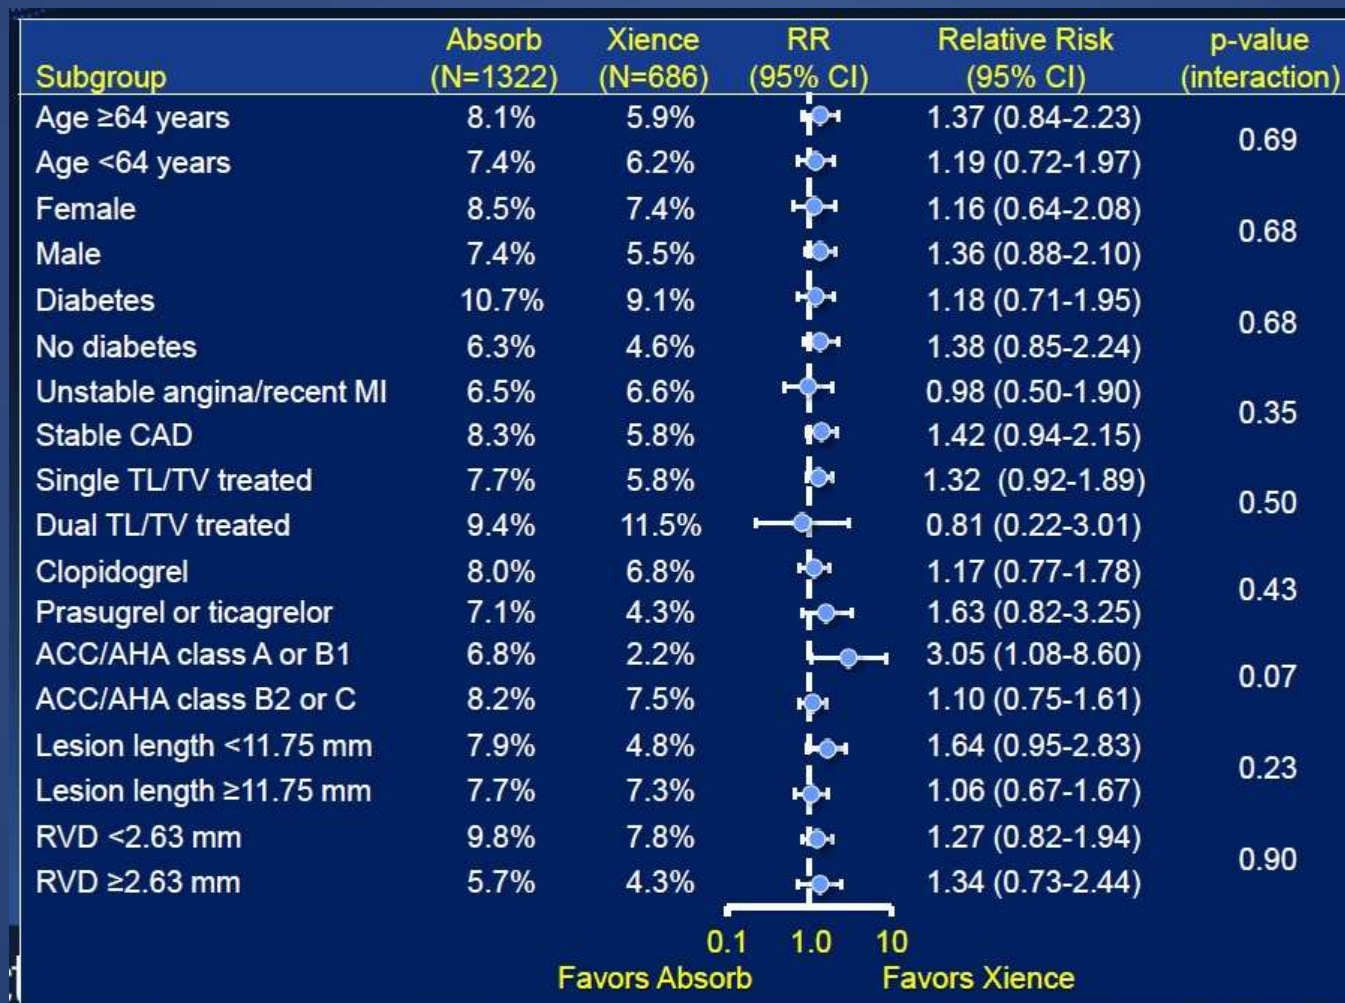

# ABSORB III

## Component of TLF

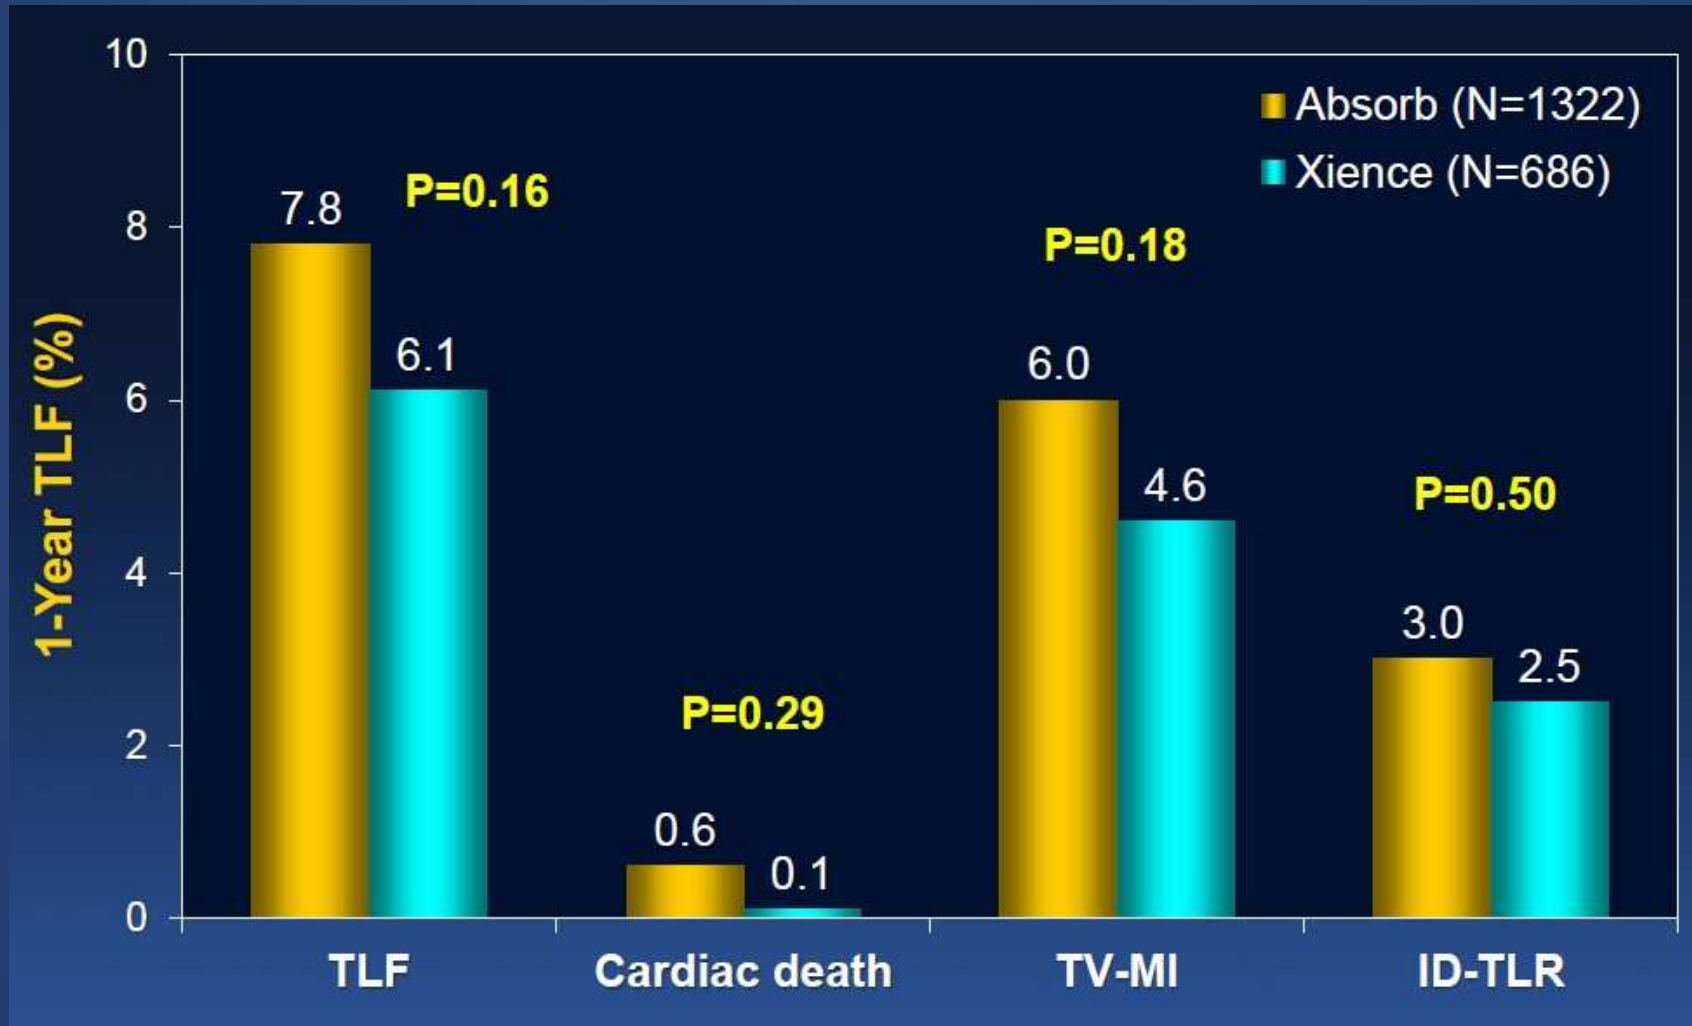

# ABSORB III

## Device Thrombosis

	Absorb (N=1322)	Xience (N=686)	p-value
Device Thrombosis (def/prob)	1.54%	0.74%	0.13
- Early (0 to 30 days)	1.06%	0.73%	0.46
- Late (> 30 to 1 year)	0.46%	0.00%	0.10
- Definite* (1 year)	1.38%	0.74%	0.21
- Probable (1 year )	0.15%	0.00%	0.55





# **ABSORB III**

## **Secondary Endpoints**

	<b>Absorb (N=1322)</b>	<b>Xience (N=686)</b>	<b>p-value</b>
<b>Angina</b>	<b>18.3%</b>	<b>18.4%</b>	<b>0.93</b>
<b>All Revascularization</b>	<b>9.1%</b>	<b>8.1%</b>	<b>0.50</b>
<b>ID-TVR</b>	<b>5.0%</b>	<b>3.7%</b>	<b>0.21</b>


# ABSORB III, 1-year outcome

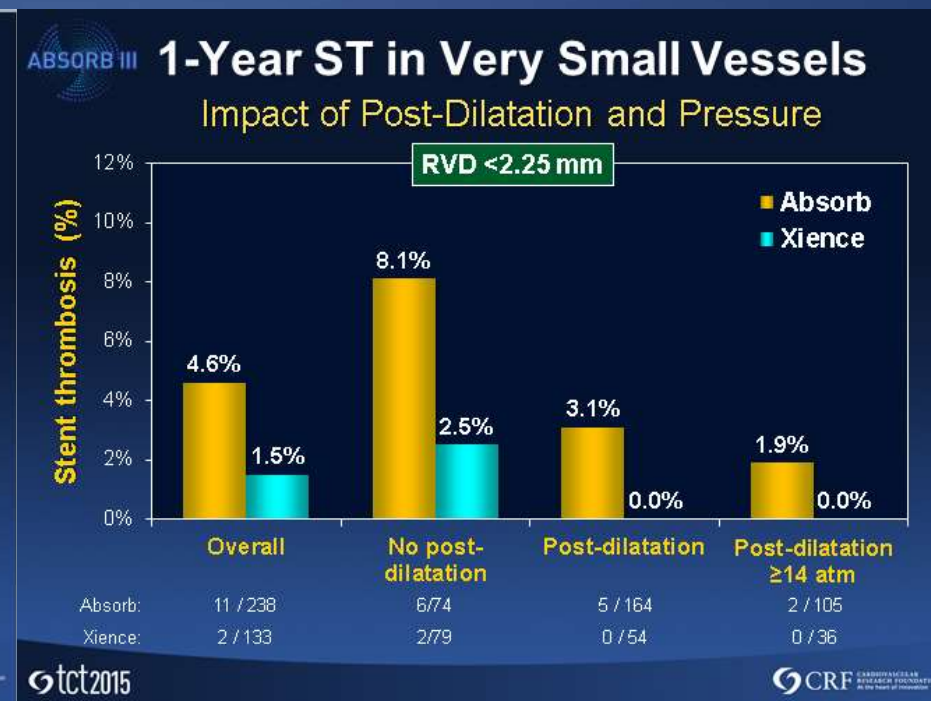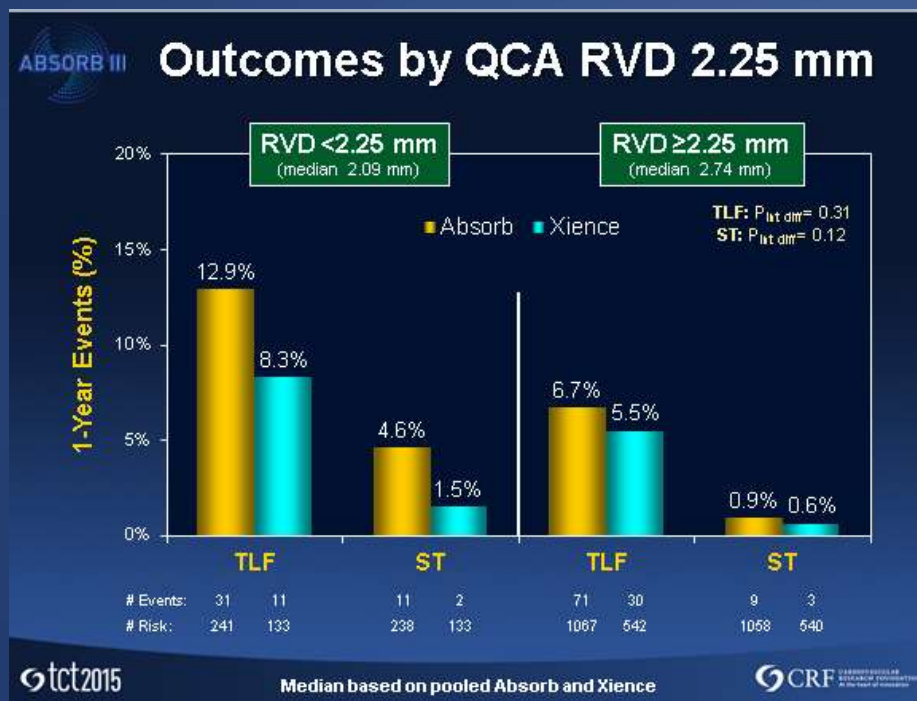

# ABSORB III 2-years



## TLF Between 1 and 2 Years (13 – 25 Months)

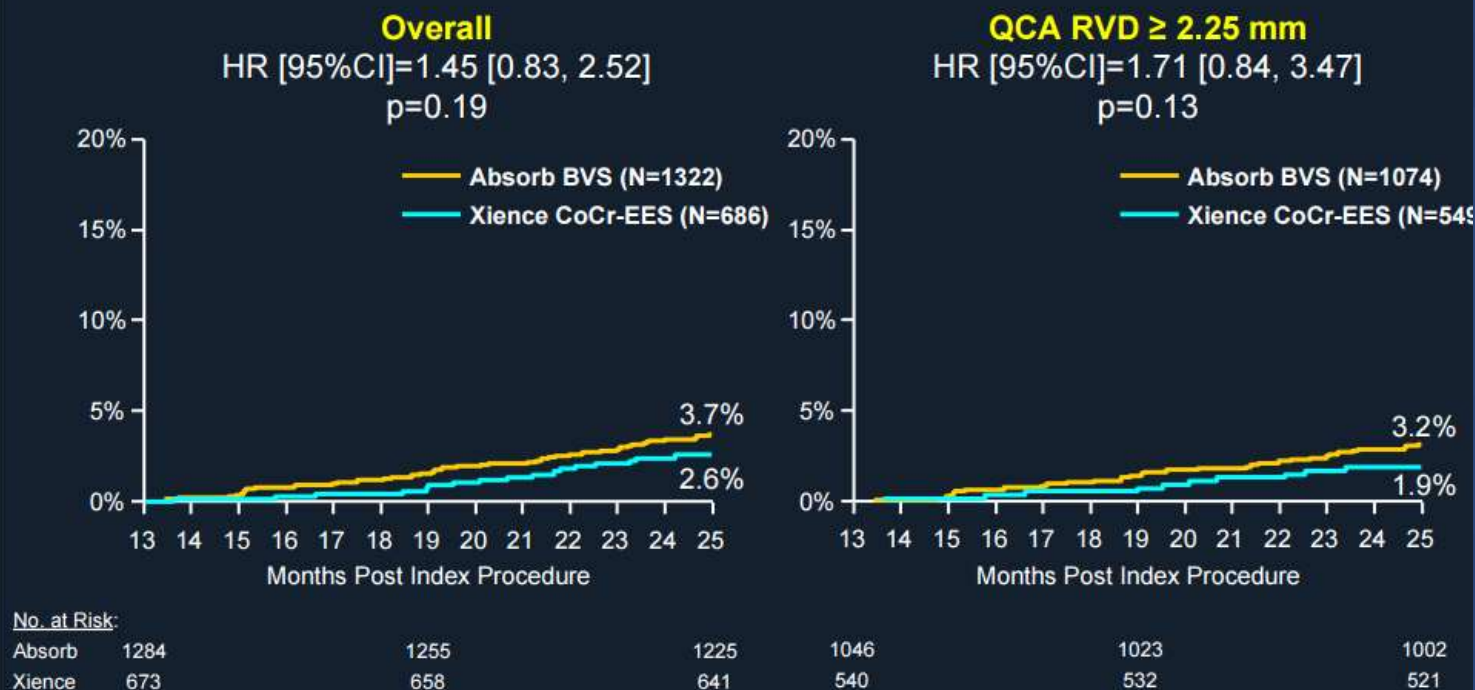

Note: The 1-year window allowed follow-up through 13 months, and the 2-year window allowed follow-up through 25 months



# ABSORB III 2-years




## Clinical Endpoints from 1 to 2 Years (13 to 25 Months)

	Overall		QCA RVD $\geq 2.25$ mm	
	Absorb (N=1322)	XIENCE (N=686)	Absorb (N=1074)	XIENCE (N=549)
TLF	3.7% (47)	2.5% (17)	3.2% (33)	1.9% (10)
Cardiac Death	0.5% (6)	0.4% (3)	0.4% (4)	0.2% (1)
TV-MI	1.3% (17)	0.7% (5)	1.3% (14)	0.4% (2)
ID-TLR	2.6% (33)	1.8% (12)	2.2% (23)	1.5% (8)
ST (Def/Prob)	0.3% (4)	0.0% (0)	0.4% (4)	0.0% (0)

P-value  $>0.05$  for all comparisons

Note: The 1-year window allowed follow-up through 13 months, and the 2-year window allowed follow-up through 25 months


# ABSORB III 2-years

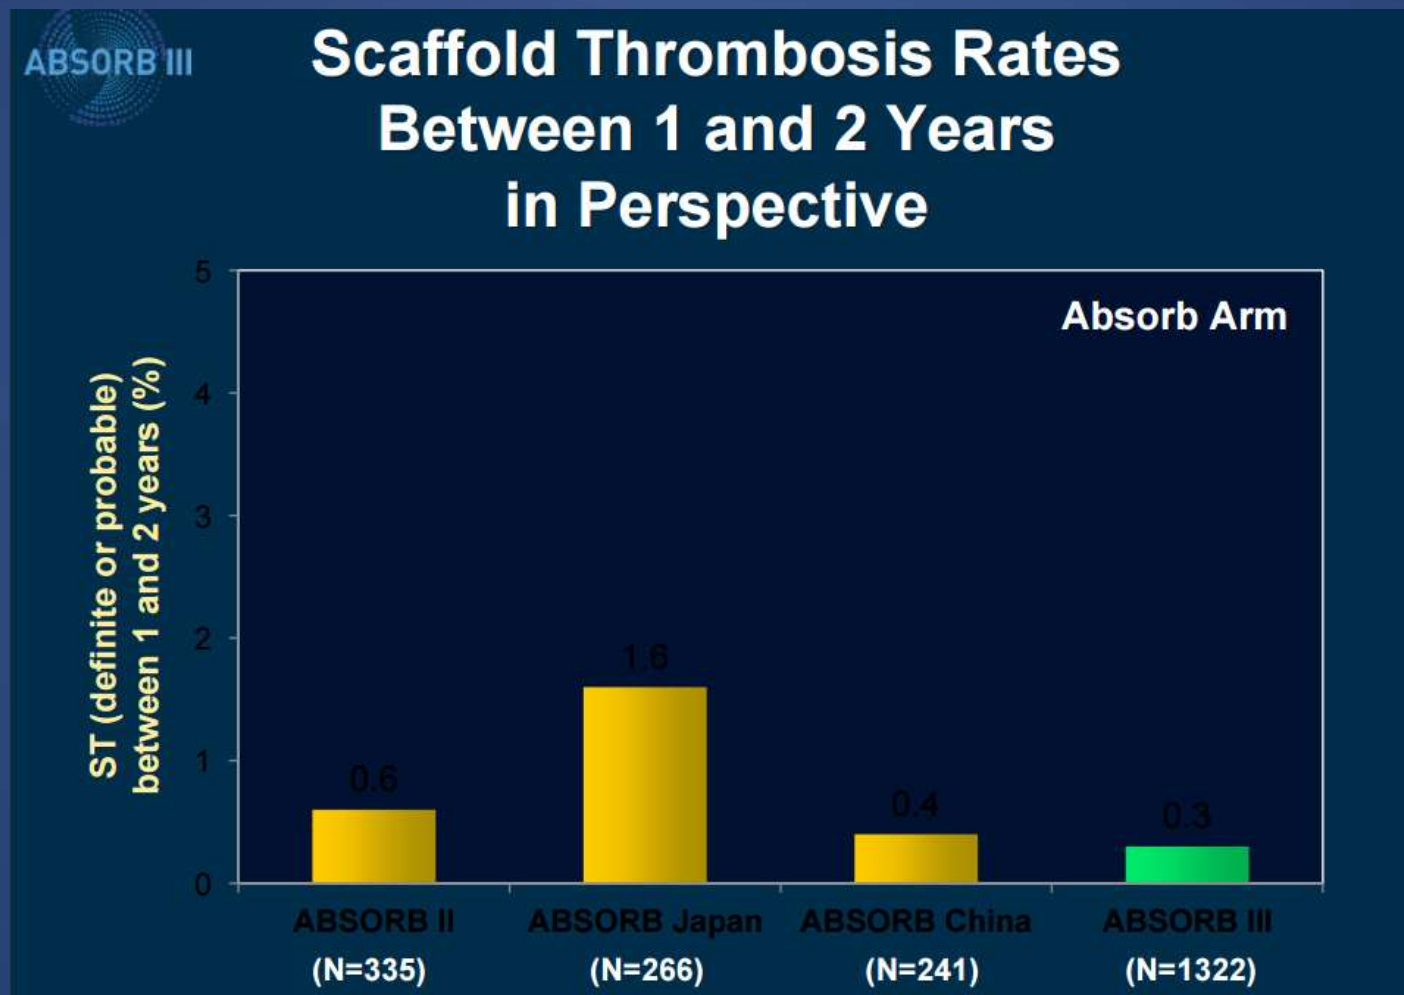

# ABSORB III 2-years




## TLF by 2 Years (25 Months)

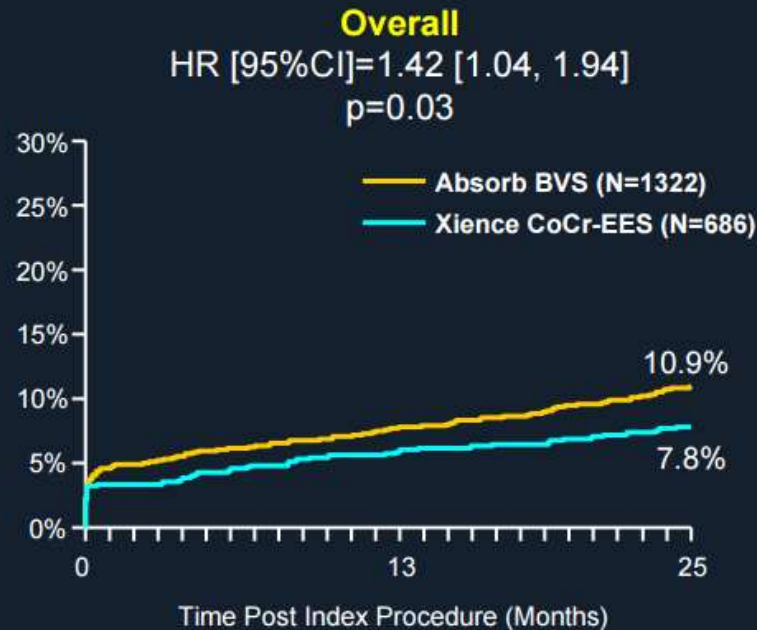

No. at Risk:

Absorb	1322	1193	1141
Xience	686	634	608

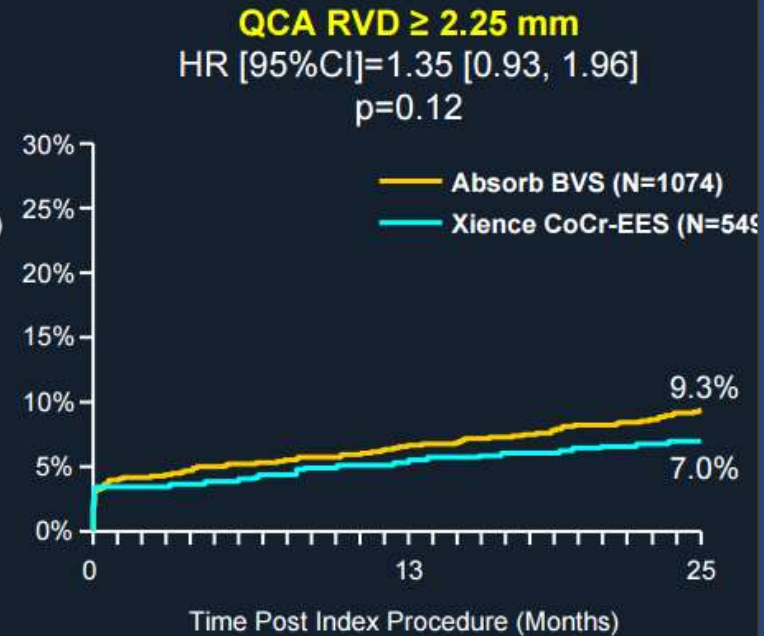

Absorb	1074	982	943
Xience	549	512	496

Note: The 2-year window allowed follow-up through 25 months

# ABSORB III 2-years



## Clinical Endpoints by 2 Years (25 Months)

	Overall		QCA RVD $\geq 2.25$ mm	
	Absorb (N=1322)	XIENCE (N=686)	Absorb (N=1074)	XIENCE (N=549)
TLF	11.0% (143)*	7.9% (53)*	9.4% (99)	7.0% (38)
Cardiac Death	1.1% (14)	0.6% (4)	0.9% (10)	0.4% (2)
TV-MI	7.3% (95)**	4.9% (33)**	6.5% (68)	4.8% (26)
ID-TLR	5.3% (69)	4.3% (29)	4.1% (43)	3.0% (16)
ST (Def/Prob)	1.9% (24)	0.8% (5)	1.3% (13)	0.6% (3)


\* P-value=0.03. \*\* P-value=0.04. P-value >0.05 for all other comparisons

Note: The 2-year window allowed follow-up through 25 months

# ABSORB III 3-years




## Target Lesion Failure

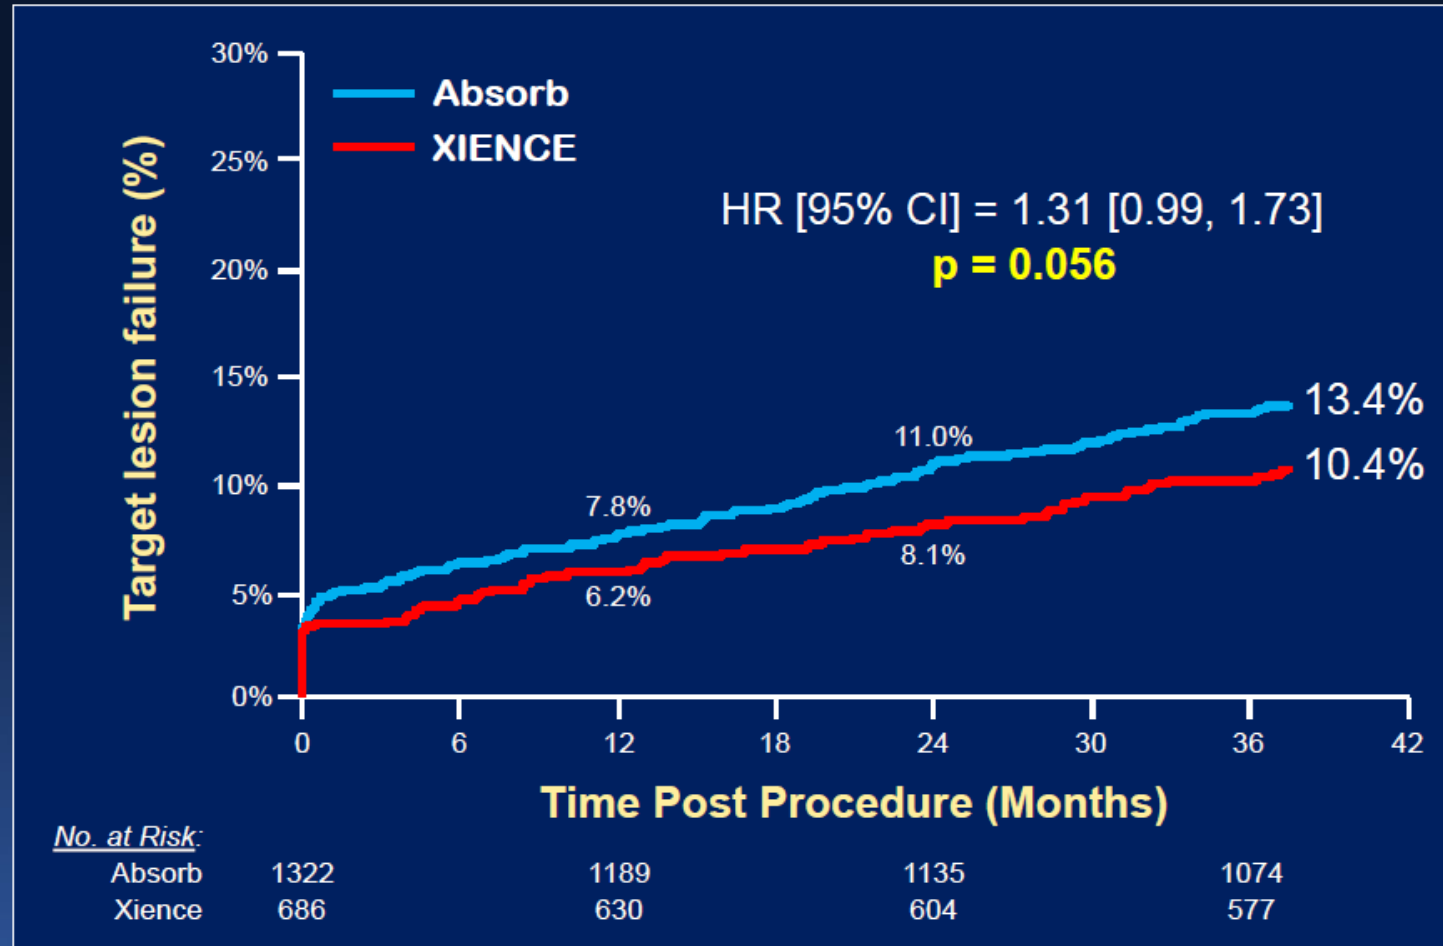




# ABSORB III 3-years

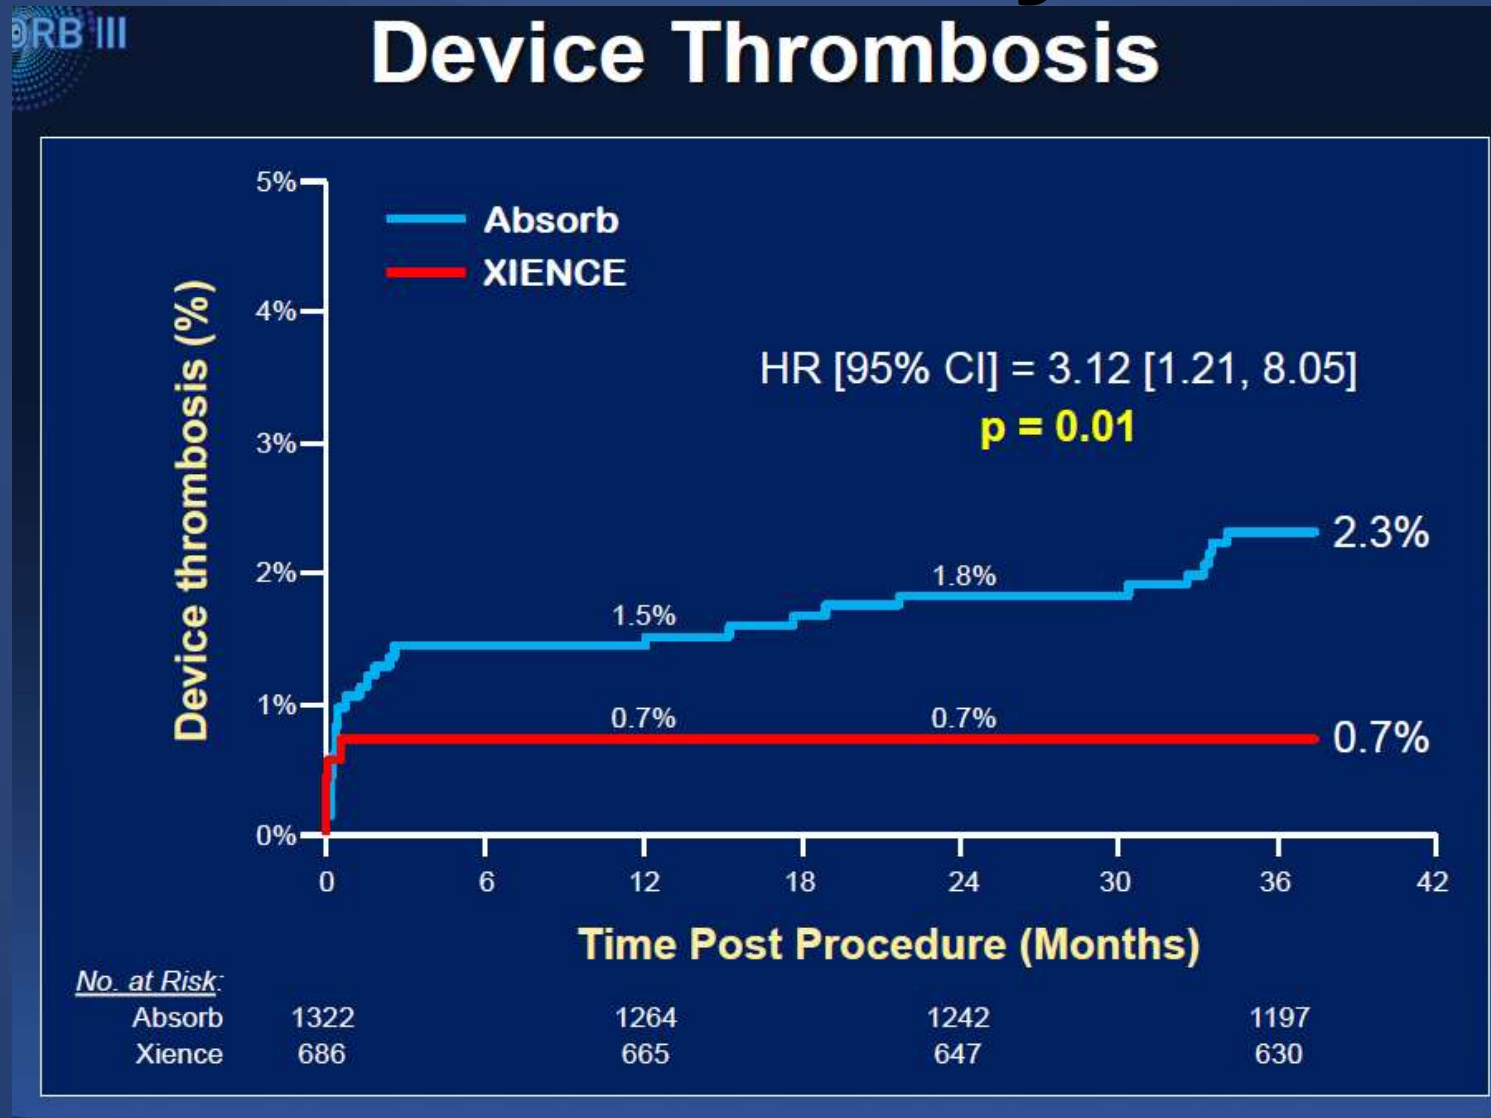

# ABSORB III 4-years

## 4-Year Target Lesion Failure

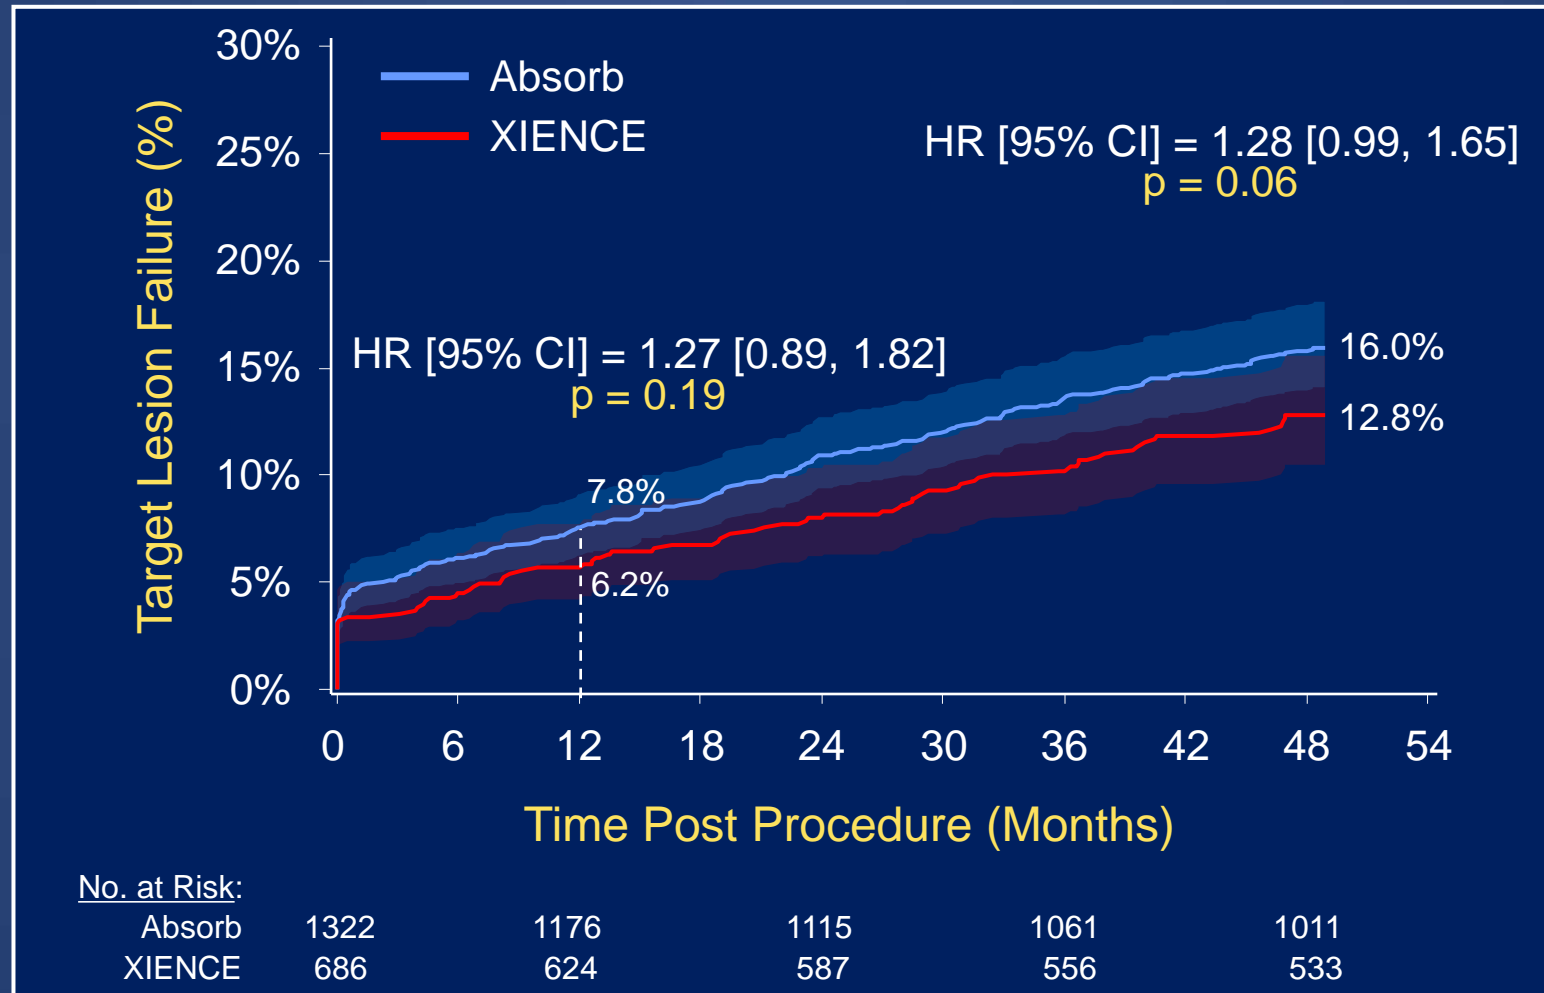


Note: 4-year window includes follow-up through 49 months.



# ABSORB III 4-years

## 4-Year Device Thrombosis

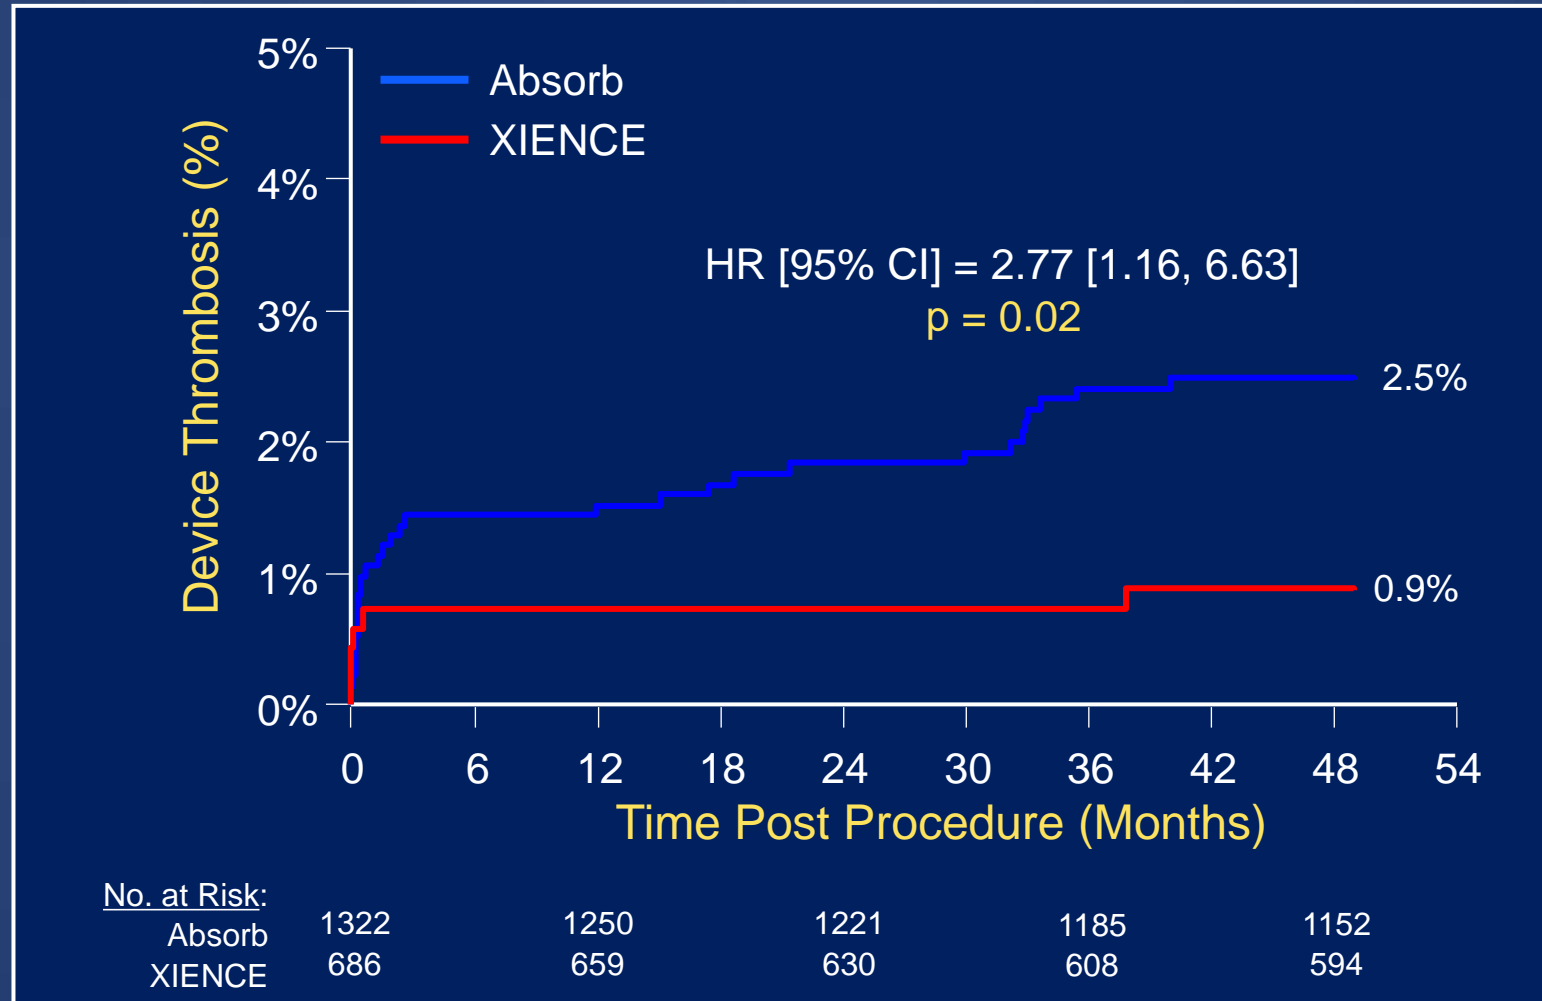


Note: 4-year window includes follow-up through 49 months.

# ABSORB JAPAN RCT

## JAPAN Approval Trial

~400 subjects (267 Absorb, 133 XIENCE)  
~30 Japan Sites. Follow-up out to 5 years  
PI: Takahashi Kimura

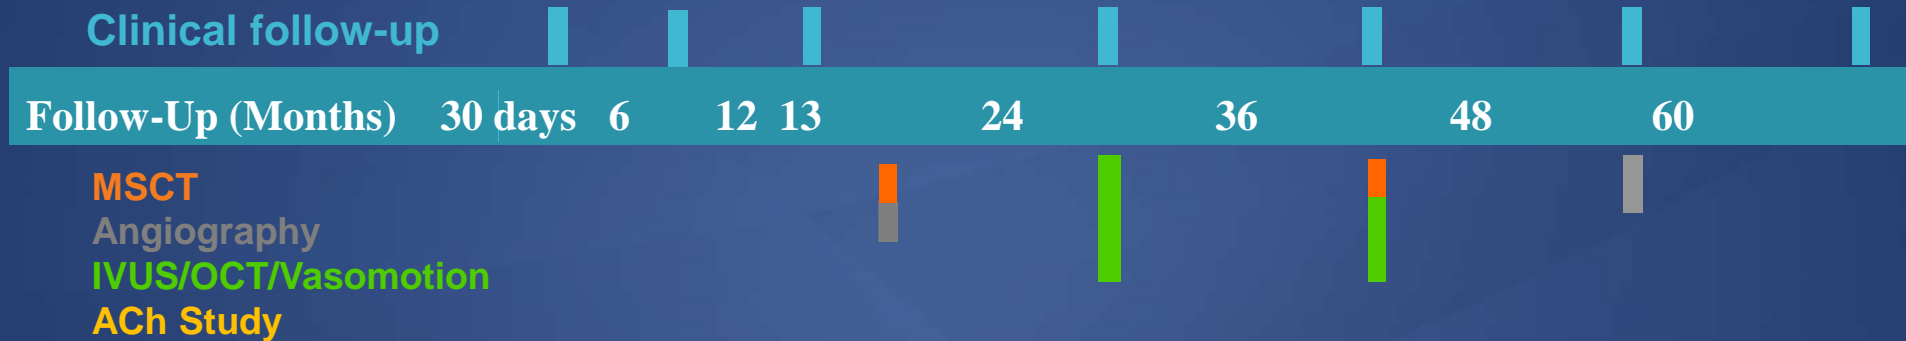

### Study Objective

Randomized against XIENCE V 2:1

### Primary Endpoint

Clinically indicated target lesion failure at 1-year (composite of cardiac death, target vessel MI or clinically indicated TLR)


### Treatment

Up to two *de novo* lesions in different epicardial vessels. No planned overlap allowed

# ABSORB Japan

ABSORB Japan

## Primary Endpoint: 12-Month TLF (through 393 days)

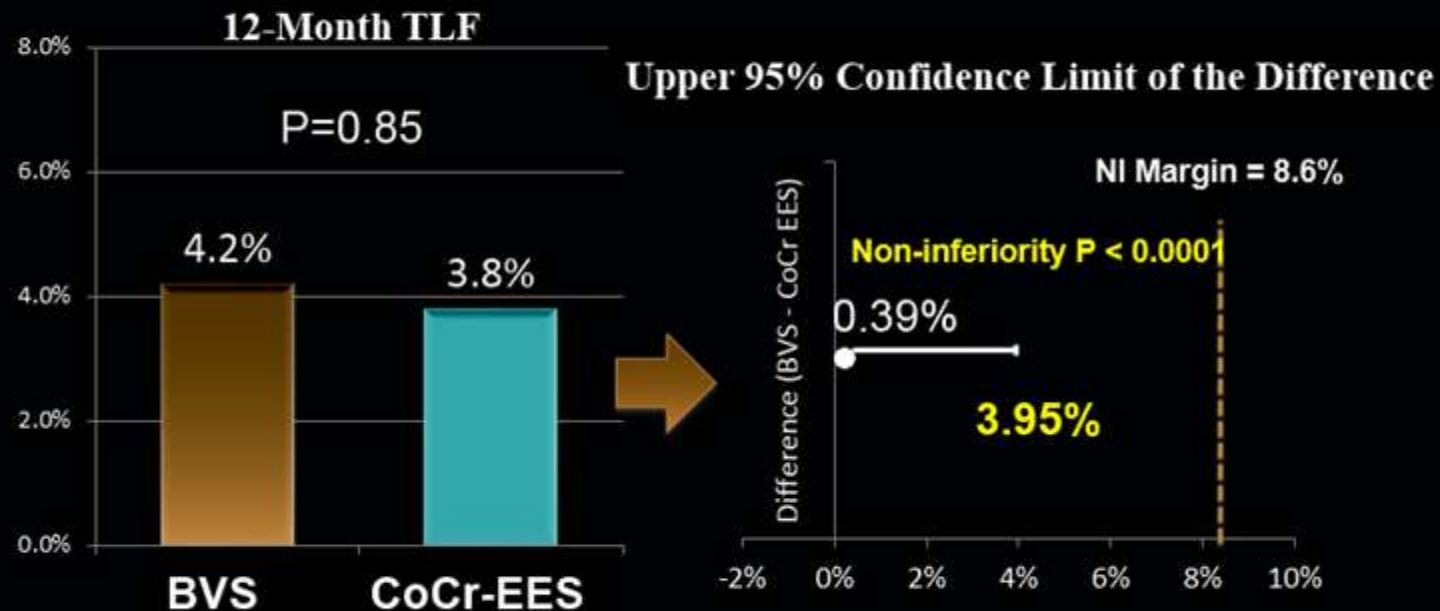

The one-sided upper 95% confidence limit for the 0.39% observed difference in event rates was 3.95%, suggesting that any absolute difference between the 2 devices is likely to be small.


Likelihood score method by Farrington and Manning

# ABSORB Japan

ABSORB Japan

Primary Endpoint:

12-Month TLF (through 393 days)

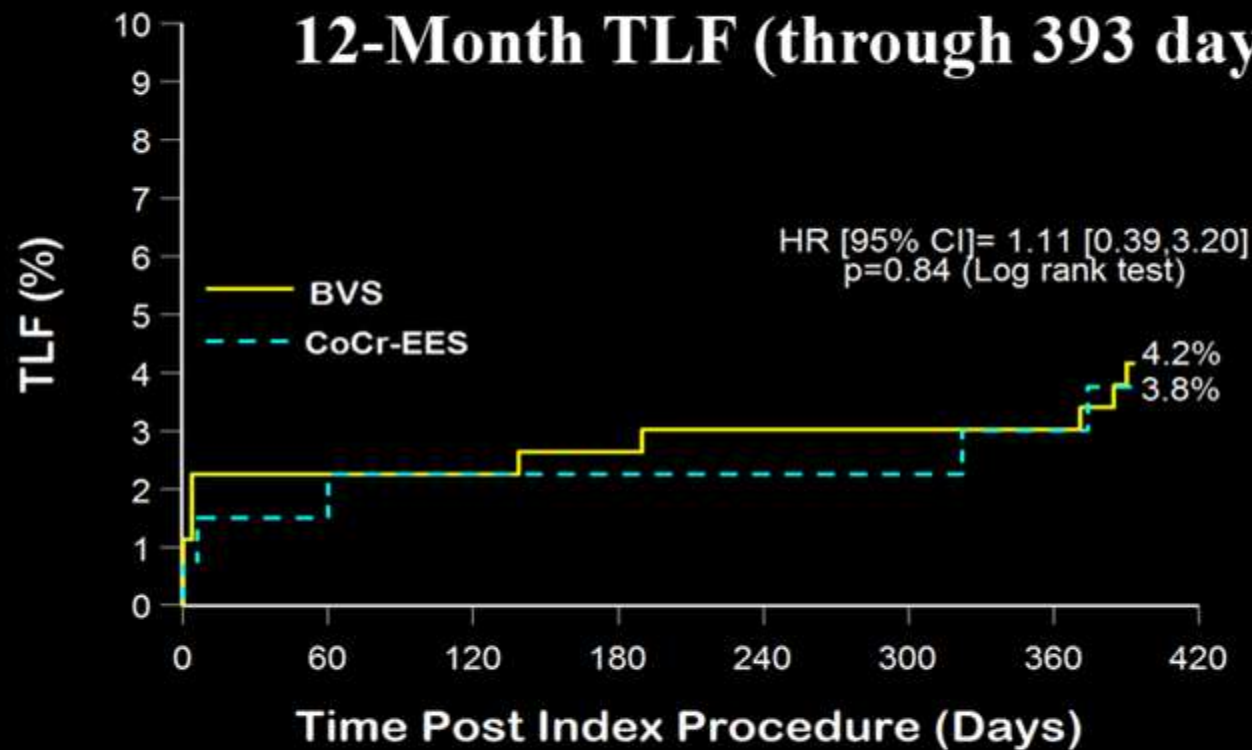


	0 days	37 days	208 days	393 days
BVS at Risk	266	259	256	251
CoCr-EES at Risk	134	131	130	128

# ABSORB Japan

ABSORB Japan


## Major Secondary Angiographic Endpoint: 13-Month In-Segment LLL

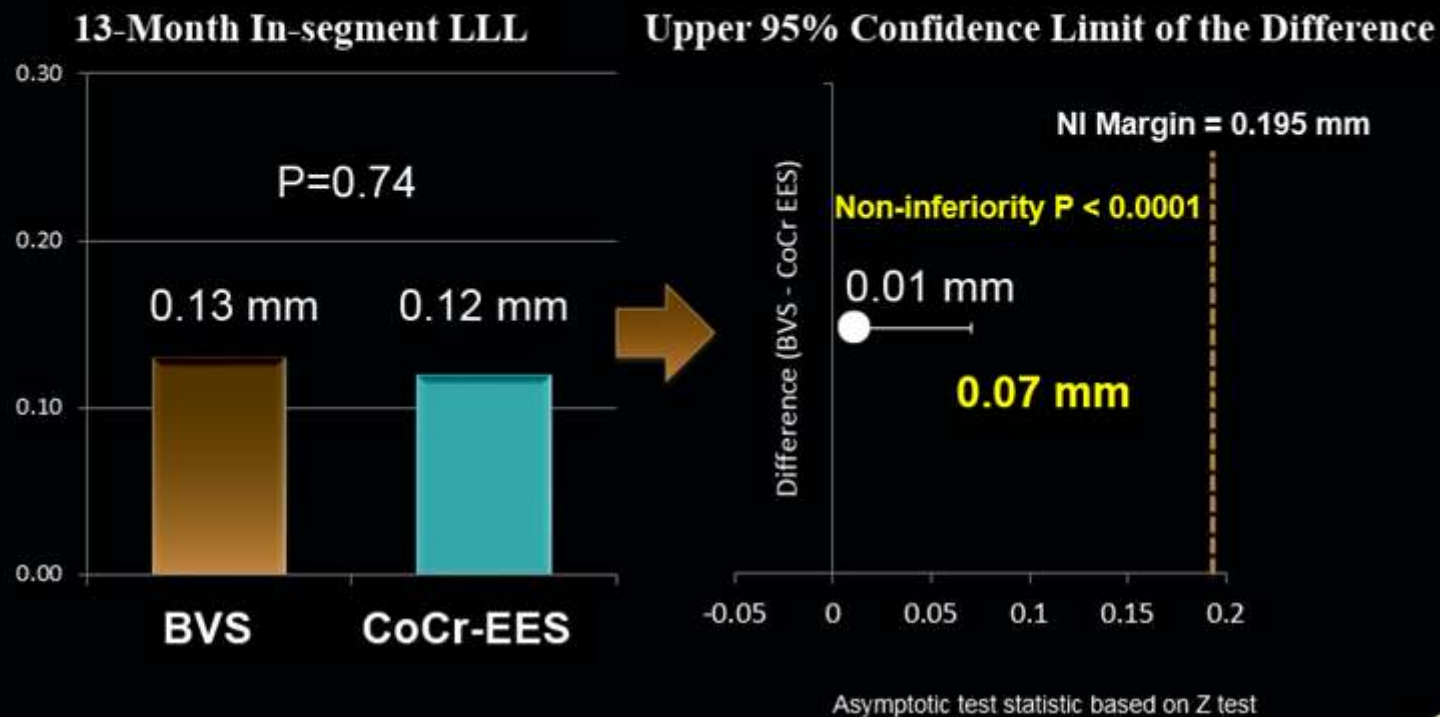

# ABSORB Japan

ABSORB Japan

## Cumulative Distribution Function Curves for In-segment MLD

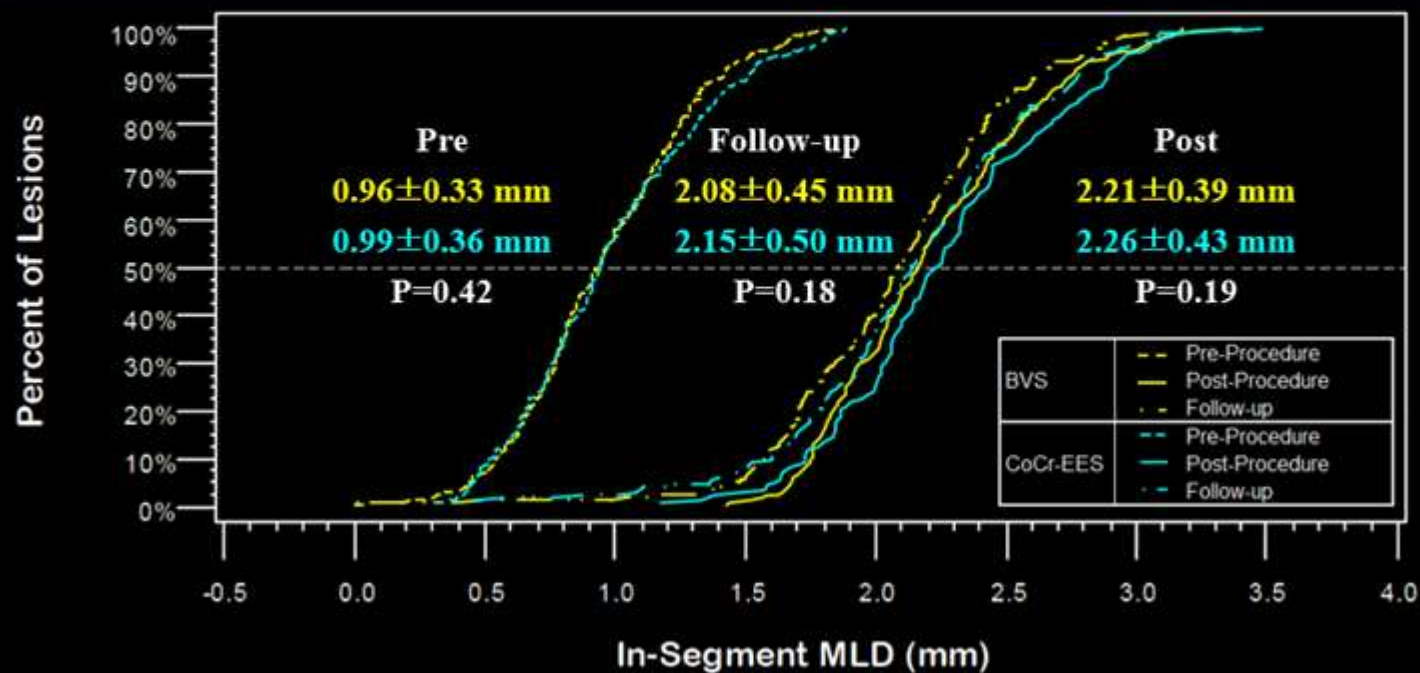




# ABSORB Japan

ABSORB Japan


## Impact of Post-procedure Intracoronary Imaging In-device MLD

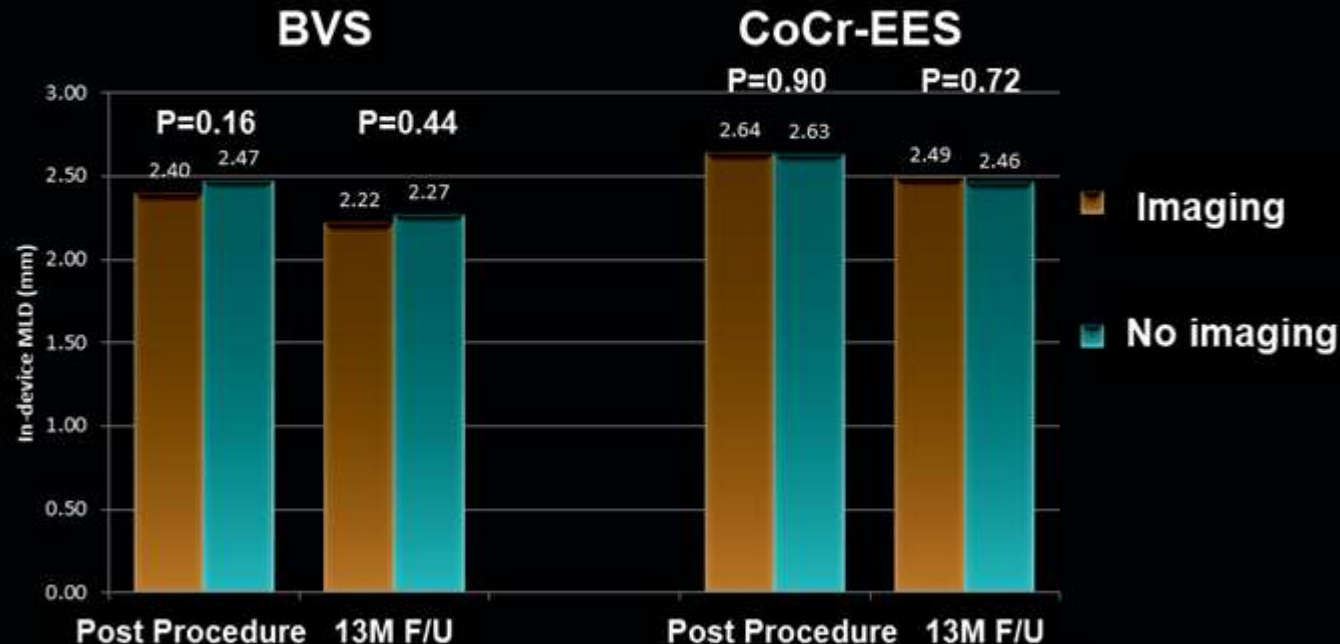

No complications were noted by the post-procedure intracoronary imaging after BVS implantation. However, in both BVS and EES groups, post-procedure intracoronary imaging did not affect the in-device MLD at post-procedure and at 13-month follow-up.




# ABSORB Japan

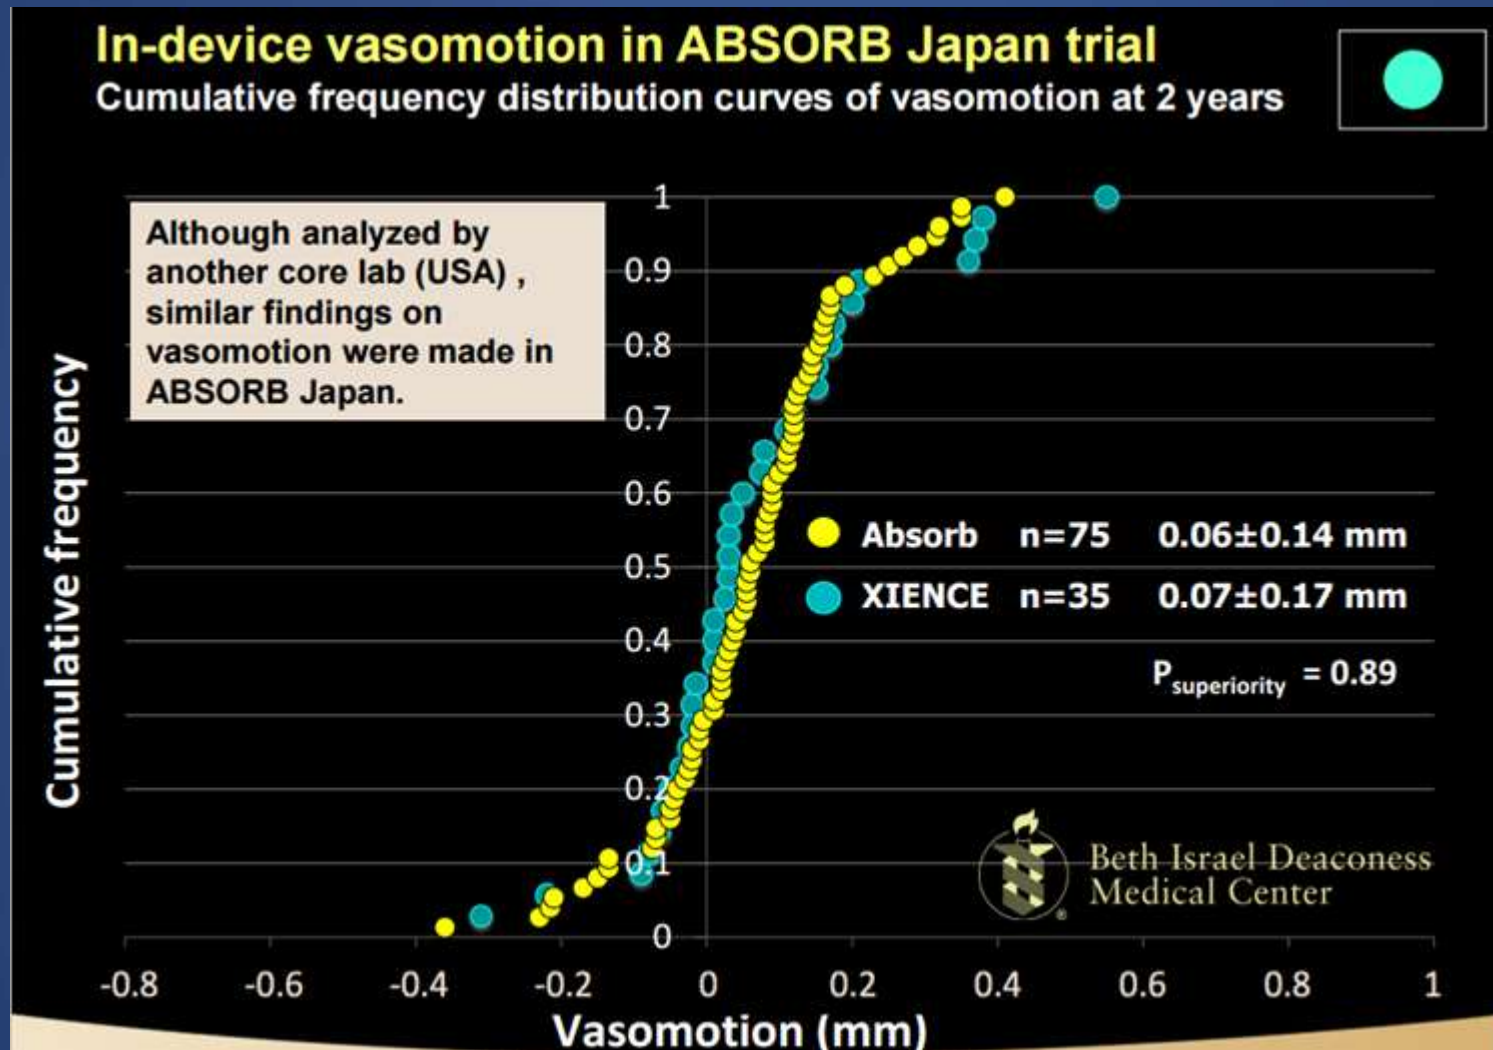


# ABSORB Japan

## Kaplan-Myer TLF to 4 Years

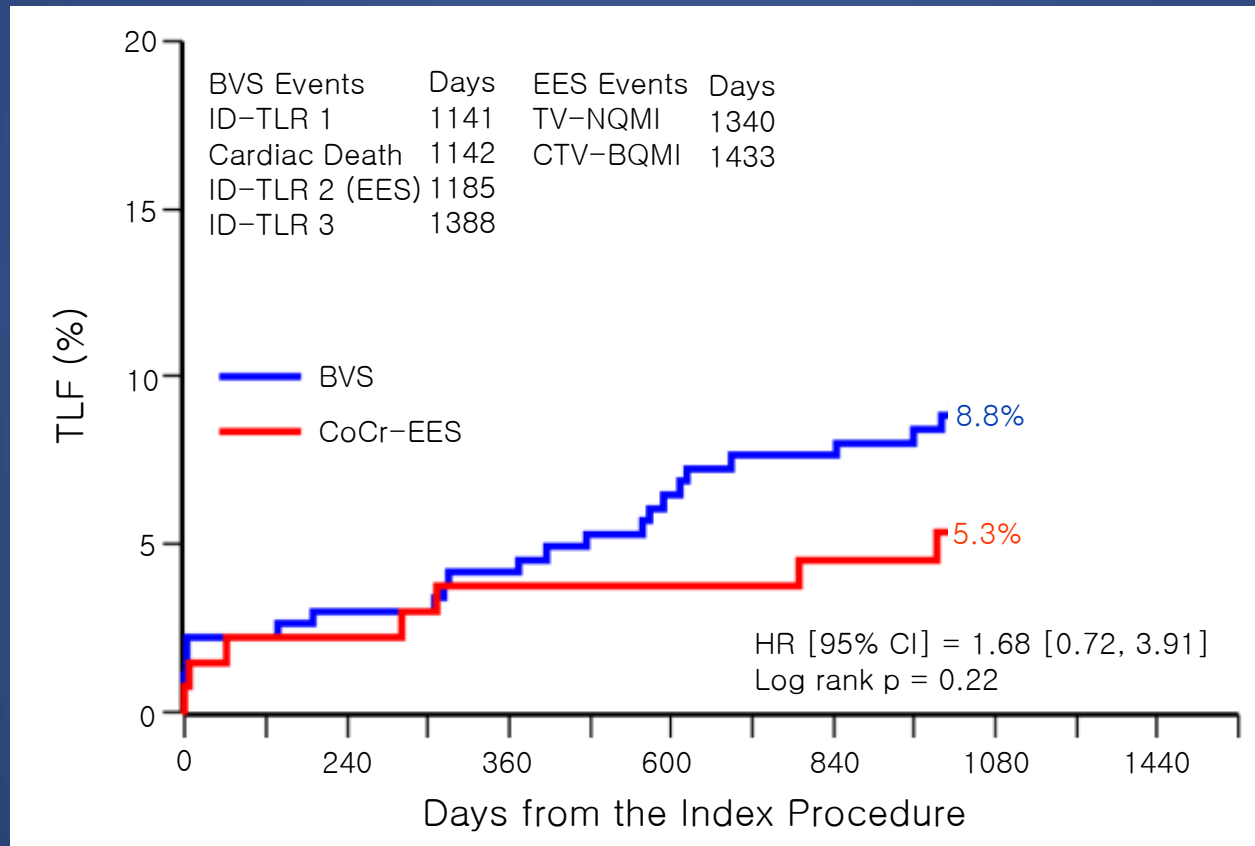

# ABSORB Japan

## Kaplan-Myer Stent/Scaffold Thrombosis to 4 Years

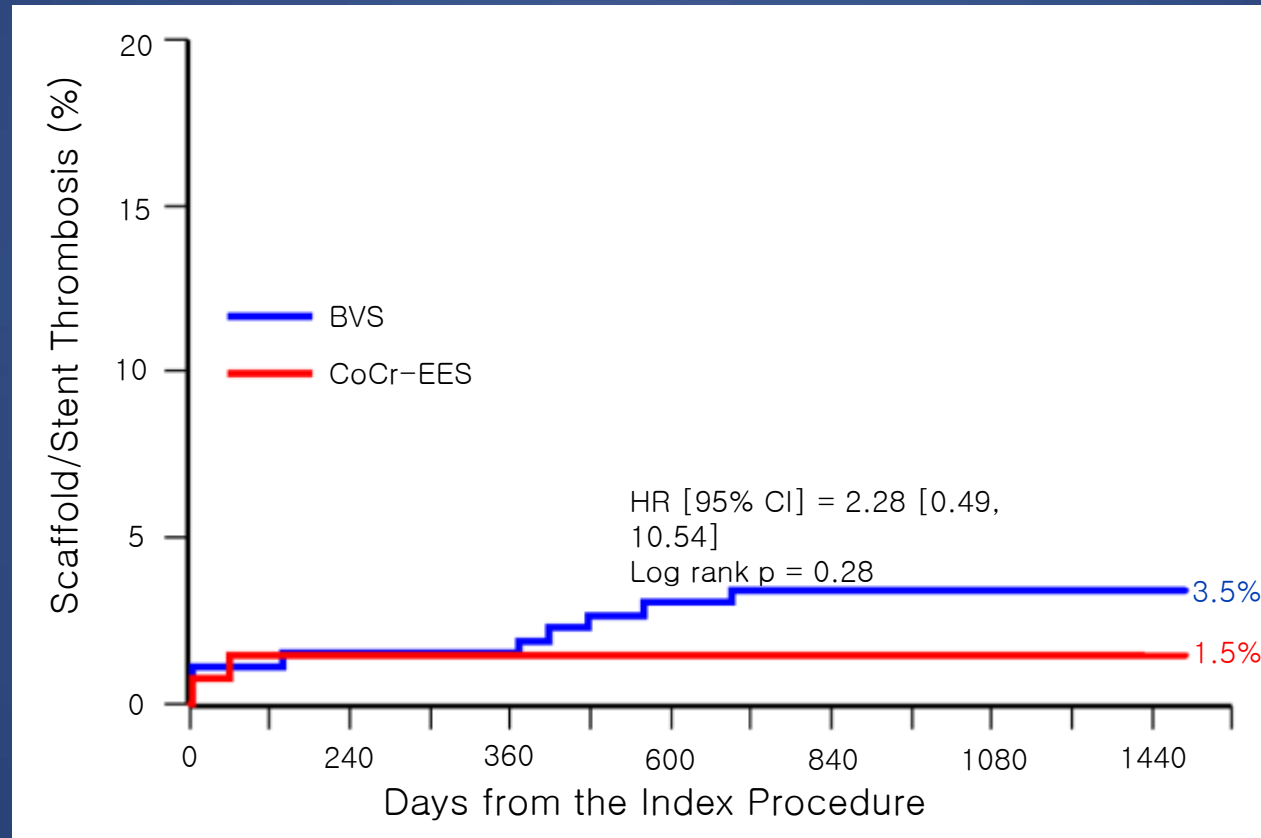

# ABSORB Japan

## Clinical Outcomes at 4 Years

	<b>BVS N=255</b>	<b>EES N=127</b>	<b>P</b>
Cumulative TLF	10.6% (27)	7.1% (9)	0.27
- Cardiac Death	0.8% (2)	0.0% (0)	1.00
- TV-MI	5.9% (15)	4.7% (6)	0.64
- ID-TLR	8.2% (21)	3.9% (5)	0.12
Cumulative ST	3.7% (9)	1.6% (2)	0.35
TLF 3-4 Years	2.1% (5)	1.6% (2)	1.00
- Cardiac Death*	0.3% (1)	0.0% (0)	1.00
- TV-MI*	0.4% (1)	1.6% (2)	0.27
- ID-TLR	1.7% (4)	0.0% (0)	0.30
- Primary ID-TLR**	1.2% (3)	0.0% (0)	0.55
- Secondary ID-TLR	0.3% (1)	0.0% (0)	1.00
VLST 3-4 years	0.0% (0)	0.0% (0)	1.00

\* Cardiac death due to aortic rupture after AVR and CABG to the target vessel incorporated with peri-procedural TV-MI. Target lesion was patent.

\*\* One of ID-TLR patient in BVS arm was treated by EES due to delivery failure of BVS.

# ABSORB China 2-years

Prospective, randomized, active control, open-label, multicenter study in 480 subjects enrolled from 24 sites in China

**Inclusion:** Up to 2 *de novo* lesions in separate native coronary arteries  
Lesion length  $\leq 24$  mm, RVD  $\geq 2.5$  mm -  $\leq 3.75$  mm, %DS  $\geq 50\%$  -  $< 100\%$

**Exclusion:** AMI, EF  $< 30\%$ , eGFR  $< 30$  mL/min/1.73m<sup>2</sup>,  
LMCA, ostial lesion, excessive vessel tortuosity, heavy calcification,  
myocardial bridge, bifurcation with side branch  $\geq 2$  mm

**1: 1 Randomization**

## Absorb BVS

Treat with single study device  
Diameters: 2.5, 3.0, 3.5 mm  
Lengths: 8, 12, 18, 28 mm

## XIENCE V


Treat with single study device  
Diameters: 2.5, 3.0, 3.5 mm  
Lengths: 8, 12, 18, 28 mm

**Primary Endpoint:** In-Segment Late Loss at 1 Year  
in the Per-Treatment-Evaluable (PTE) Population\*

# ABSORB China 2-years



## Target Lesion Failure (TLF)

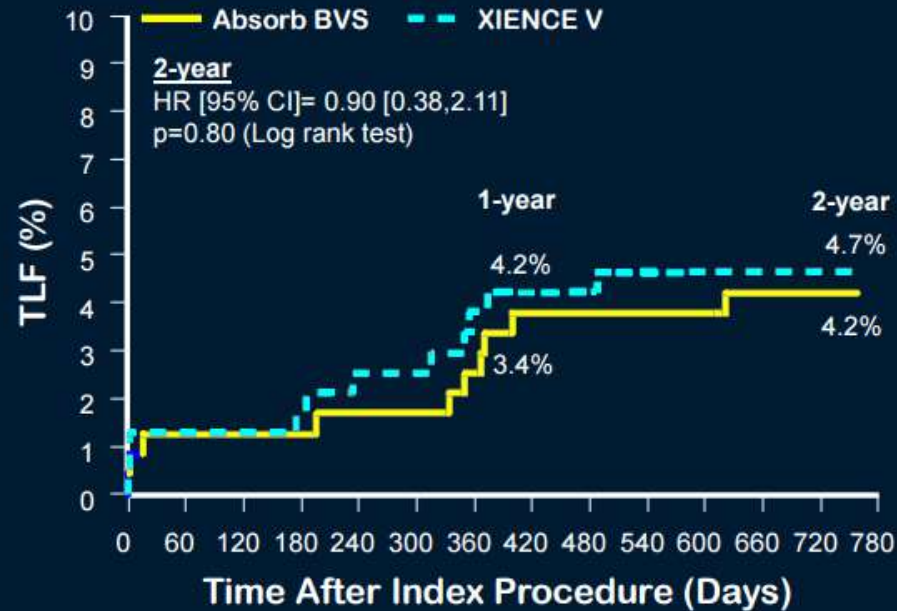

Time (days)	0	37	208	298	393	758
Absorb BVS (# At Risk)	238	235	234	234	230	227
XIENCE V (# At Risk )	237	234	230	229	225	223



# ABSORB China 2-years



## Scaffold/Stent Thrombosis

	Absorb BVS (N=241)	XIENCE V (N=239)	P-Value
All (0 - 730 days)	0.8% (2/237)	0.0% (0/231)	0.50
Definite	0.4% (1/237)	0.0% (0/231)	1.00
Probable	0.4% (1/237)	0.0% (0/231)	1.00
Early (0 – 30 days)	0.4% (1/238)	0.0% (0/236)	1.00
Late (31- 365 days)	0.0% (0/238)	0.0% (0/232)	1.00
Very Late (366- 730 days)	0.4% (1/237)	0.0% (0/231)	1.00

*There were 1 probable, subacute (1-30d) ST and 1 definite, very late ST in the Absorb BVS arm.*

# ABSORB China 2-years



## PSP Analysis for TLF & ST

		PSP*	Non-PSP
TLF	0-1 Year	0% (0/32)	3.9% (8/205)
	1-2 Year	0% (0/32)	1.5% (3/204)
ST	0-1 Year	0% (0/32)	0.5% (1/205)
	1-2 Year	0% (0/32)	0.5% (1/204)


*This is a post-hoc analysis for hypothesis-generating only.*

\*PSP analysis (all lesions must satisfy all the criteria below) based on as-treated population:

- Pre-dilatation
- Sizing (vessel):  $2.25\text{mm} \leq \text{QCA RVD} \leq 3.5\text{ mm}$
- Post-dilatation:
  - Pressure > 16 atm
  - Balloon diameter: scaffold diameter > 1:1 and balloon diameter  $\leq$  scaffold diameter + 0.5mm

# ABSORB China 4-years


Target Lesion Failure Through 4 Years

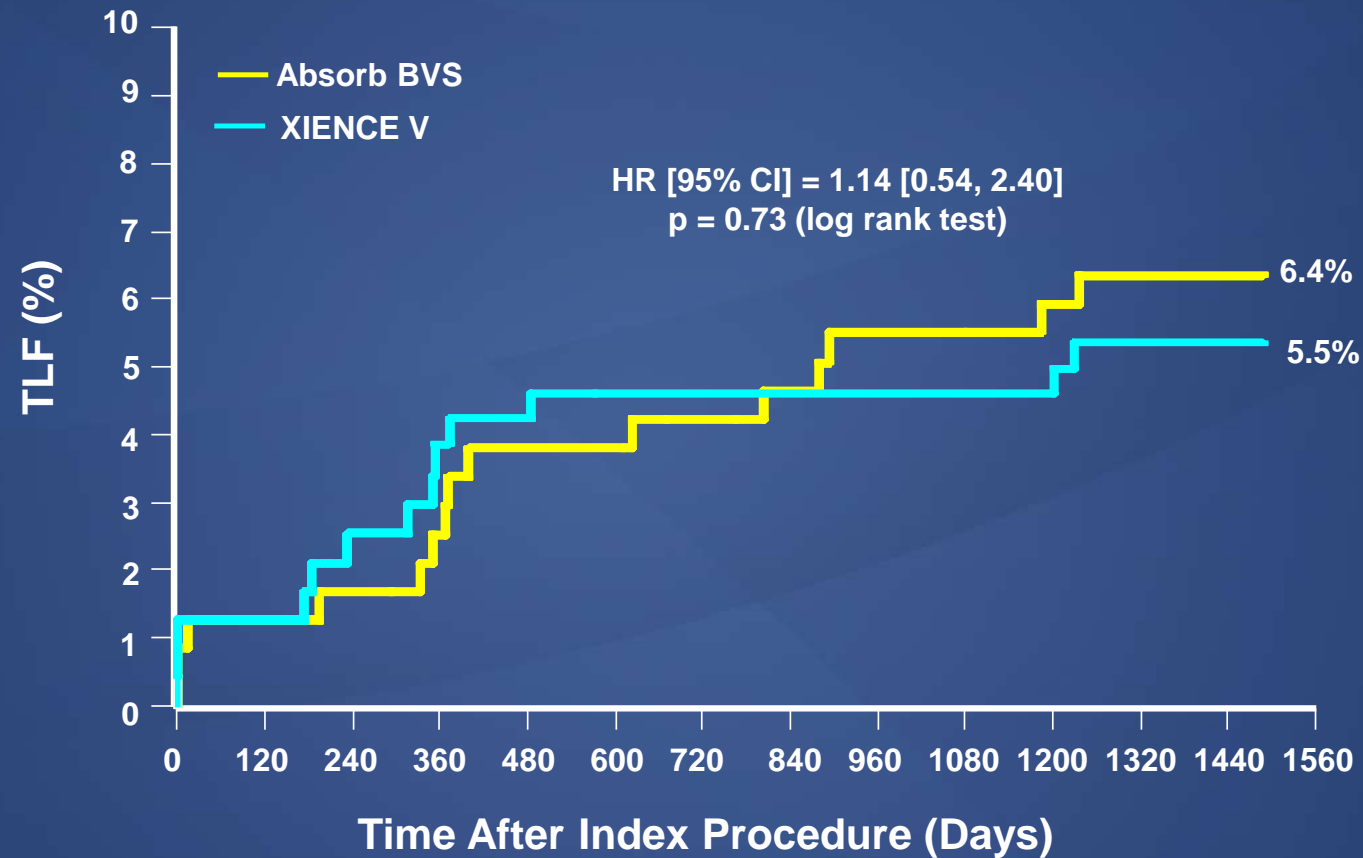

Time (days)	0	37	208	298	393	758	1123	1488
Absorb BVS (# At Risk)	238	235	234	233	229	225	220	217
XIENCE (# At Risk)	237	234	230	229	223	221	221	219

# ABSORB China 4-years


## Cardiac Death Through 4 Years

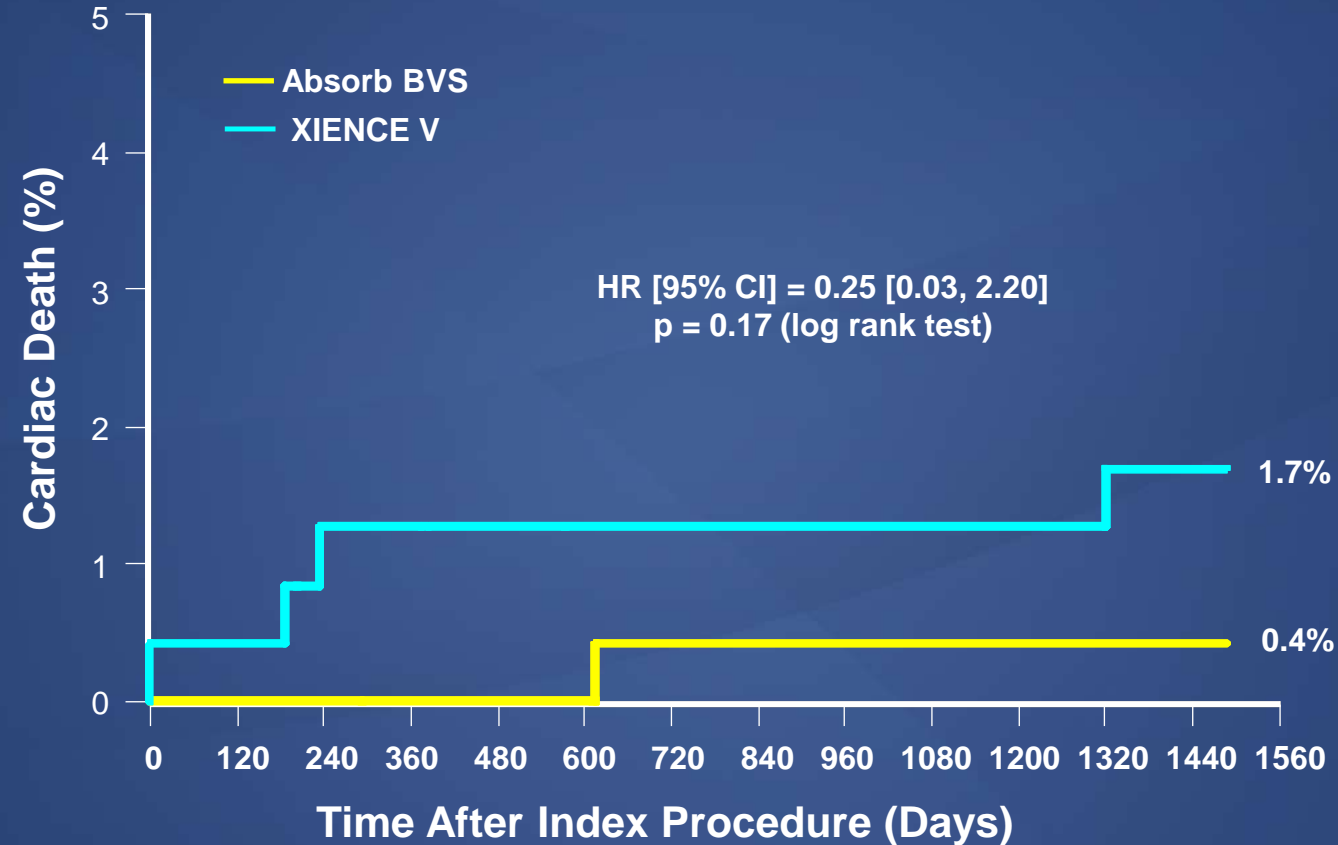

Time (days)	0	37	208	298	393	758	1123	1488
Absorb BVS (# At Risk)	238	238	238	237	237	234	232	231
XIENCE (# At Risk)	237	236	233	232	230	229	229	228


# ABSORB China 4-years

## Target-Vessel Myocardial Infarction Through 4 Years

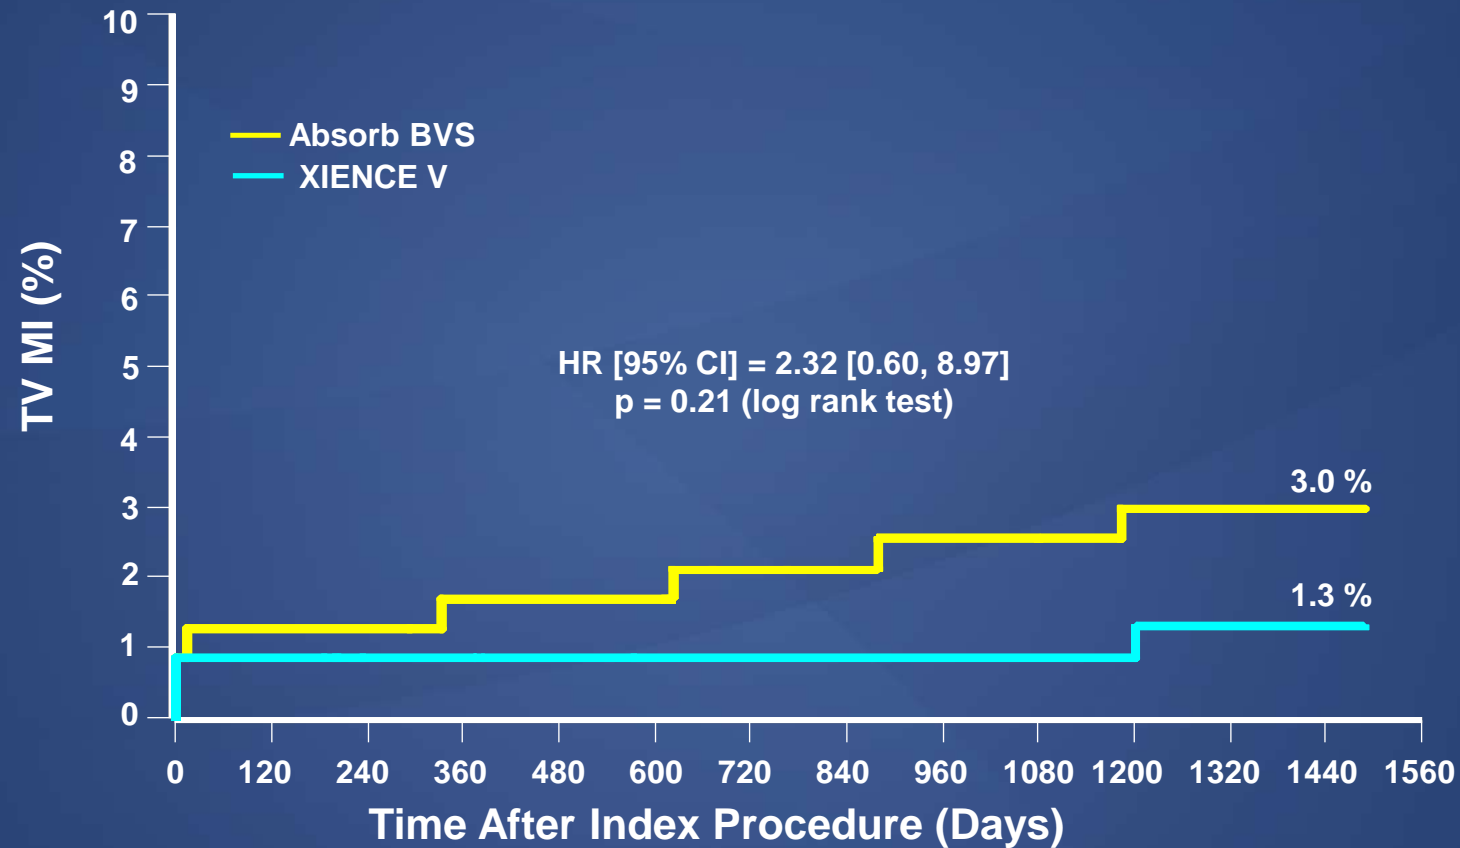

# ABSORB China 4-years

## Ischemia-Driven Target Lesion Revascularization Through 4 Years

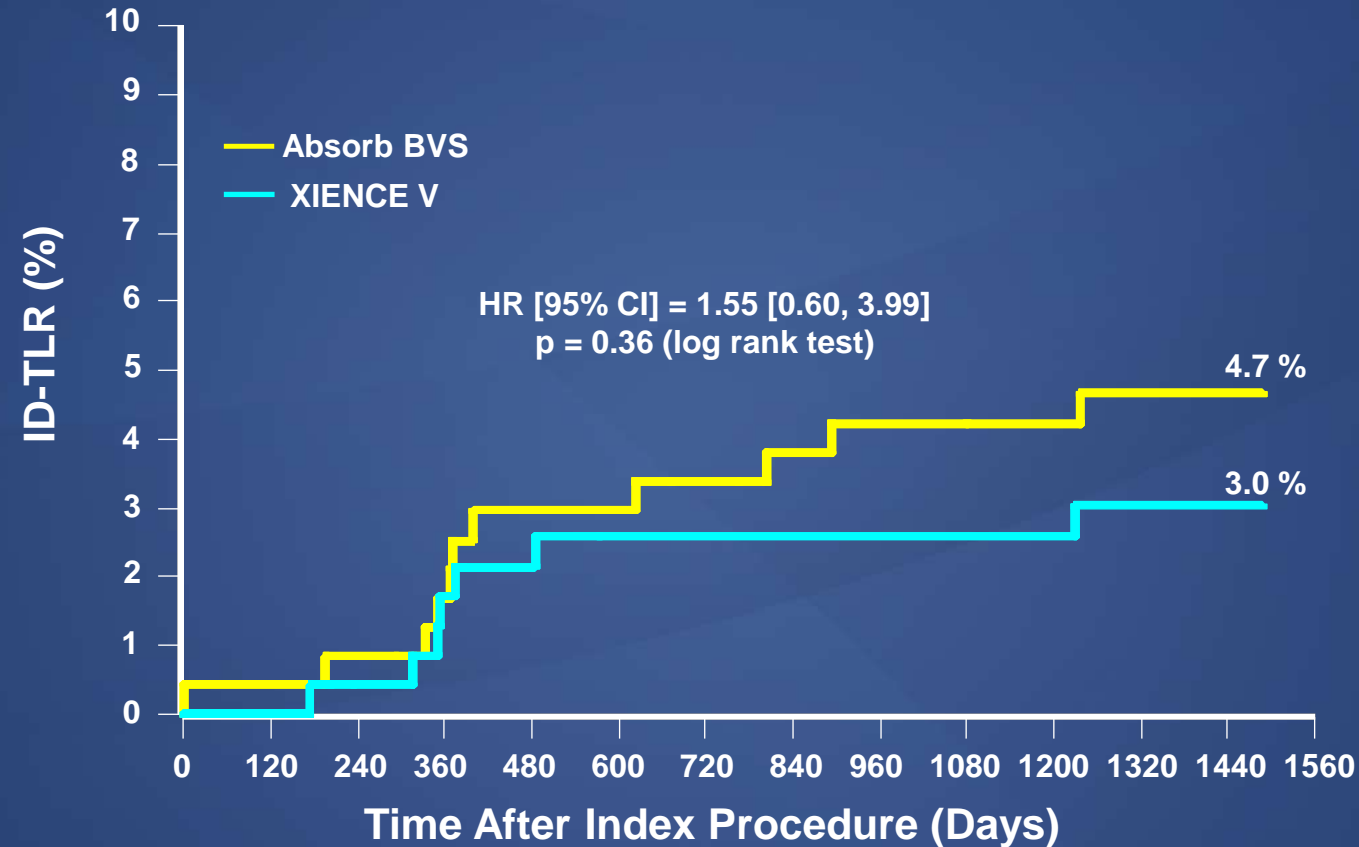


Time (days)	0	37	208	298	393	758	1123	1488
Absorb BVS (# At Risk)	238	237	236	235	231	227	223	221
XIENCE (# At Risk)	237	236	232	231	225	223	223	221



# ABSORB China 4-years

Definite/Probable Scaffold/Stent Thrombosis Through 4 Years

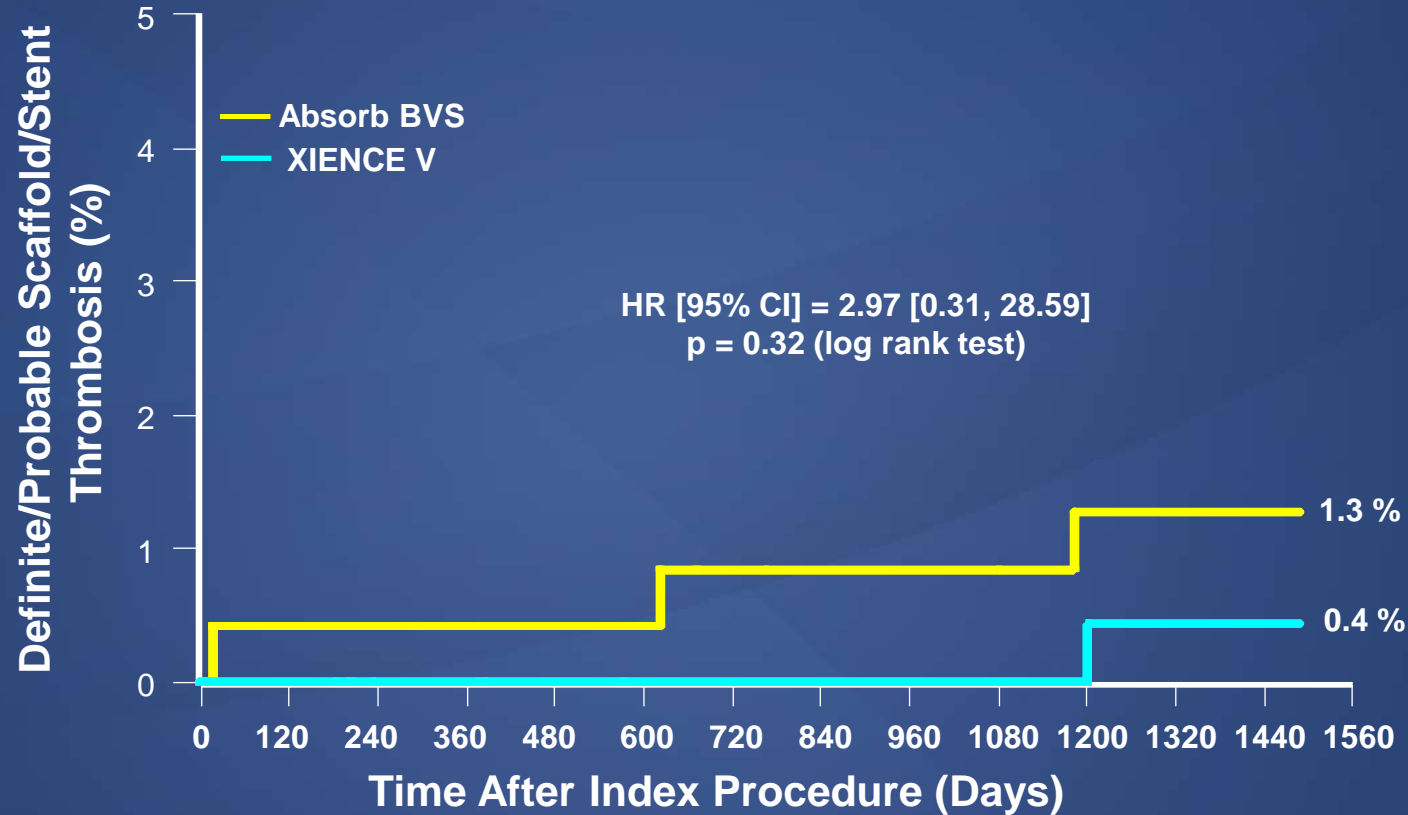


Time (days)	0	37	208	298	393	758	1123	1488
Absorb BVS (# At Risk)	238	237	237	236	236	232	230	228
XIENCE (# At Risk)	237	236	233	232	230	229	229	228

# ASSURE (D. Mathey)

Objective: Measure Absorb safety, efficacy and performance in all-comers over 3 years

Design: Prospective, observational multi-center registry, 183 patients, 6 sites in Germany

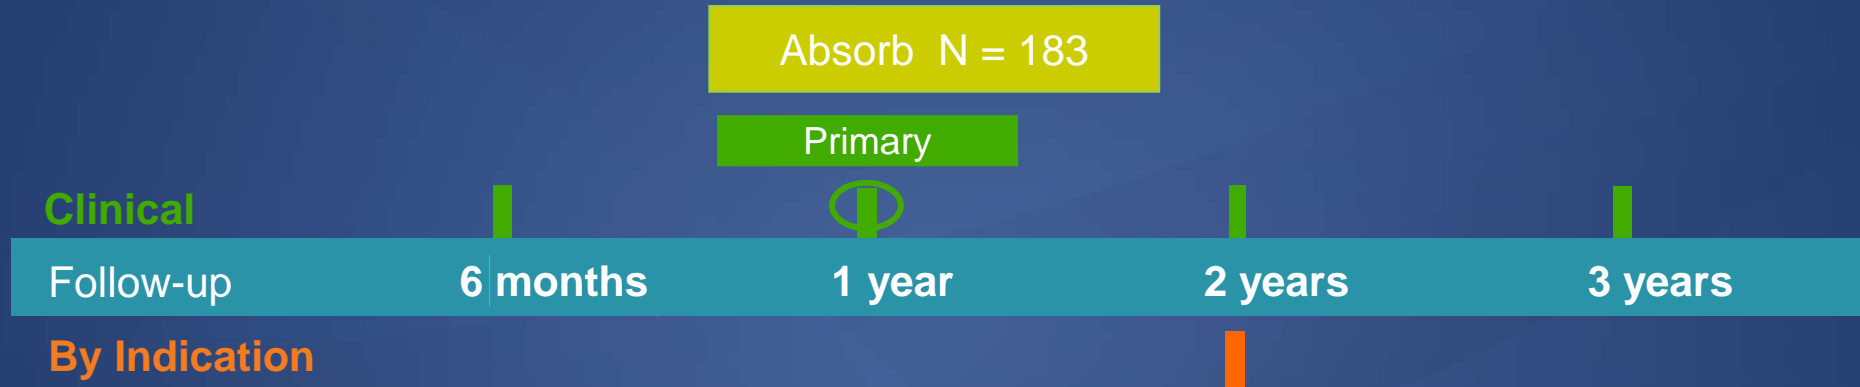

Primary Endpoints:

- Death (cardiovascular)
- MI
- TLR, TVR, TVF
- Angiographic parameter (QCA)

Twelve Months ASSURE, T. Schmitz, PCR 2014

# ASSURE (D. Mathey)

## Twelve Months Clinical Results

Baseline Characteristics	N = 183
Hypertension	82.0%
Diabetes	25.7%
Dyslipidemia	76.0%
Angina (not stable)	21.3%
ACC/AHA B2 or C lesions	64.6%
Moderately to heavy Ca-lesions	15.7%
Diameter stenosis	64.4%

12 Months Results	N = 183
Death*	0.5%
Target lesion revascularization**	2.8%
Myocardial infarction***	1.6%
MACE	5%
Stent Thrombosis	0%

\*Patient died due to major gastrointestinal bleeding

\*\* Restenosis in complex lesions

\*\*\* MI's were caused by non-TVF

**Dr. Schmitz' conclusion: One-year ASSURE results suggest that BVS for de novo coronary artery disease are associated with favorable clinical and functional outcomes in all day clinical practice without mandatory IVUS or OCT guidance.**

# ASSURE 2-years

## DESIGN

Prospective, observational,  
single-arm, multi-center


## OBJECTIVE

To investigate safety and  
effectiveness of the Absorb  
bioresorbable vascular  
scaffold for de novo coronary  
artery lesions in real-world  
practice

## COORDINATING CLINICAL INVESTIGATOR

Detlef Mathey, MD, University  
Cardiovascular Center  
Hamburg, Germany

**CORE LAB** University of Ulm

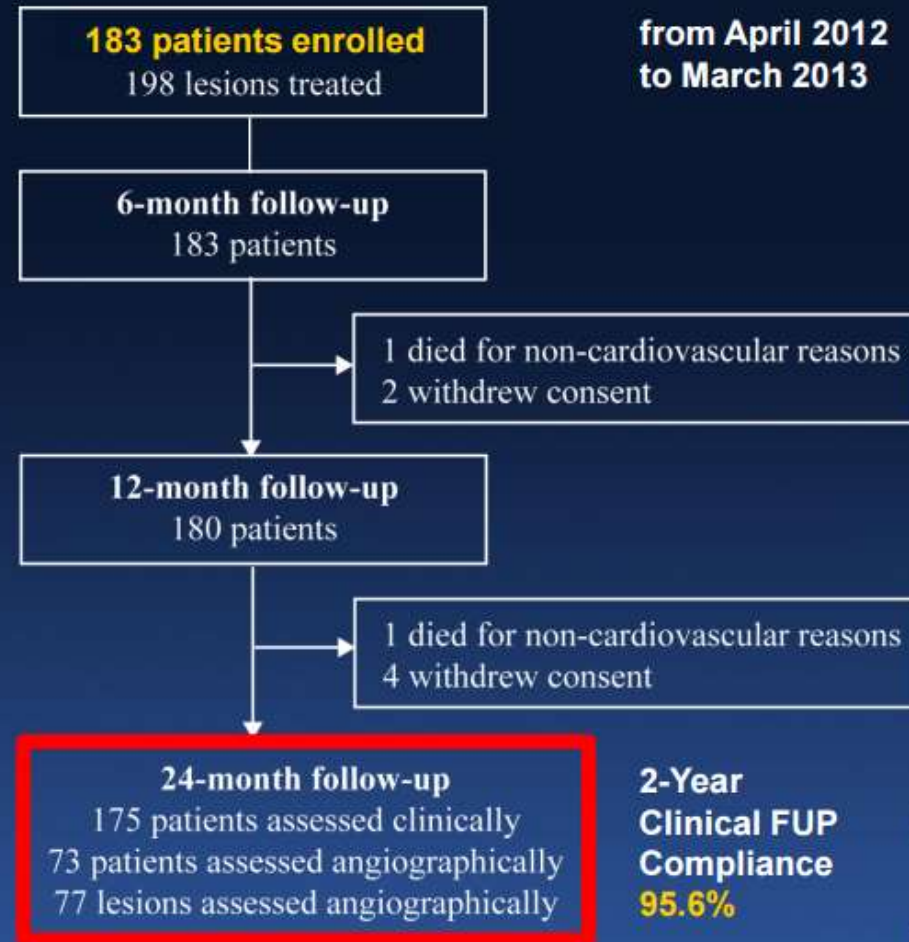

# ASSURE 2-years

## Freedom From MACE at 2 Years



# ASSURE 2-years

## Angiographic Findings

*2-Year FU (22.2 ± 6 Months)*

77 lesions

### Post Procedure (mean)

Acute gain, mm	1.7
% DS in-scaffold	14.6
Acute gain, %	61.8

### 2-Year FU (mean)

LLL in-scaffold, mm	0.24
% DS in-scaffold	20.8
Net gain, %	47.2




# ASSURE 2-years

## Late Loss at 2 Years

*Restenoses excluded (N=67)*

*Restenoses (N=8\*)*

\* CTOs excluded

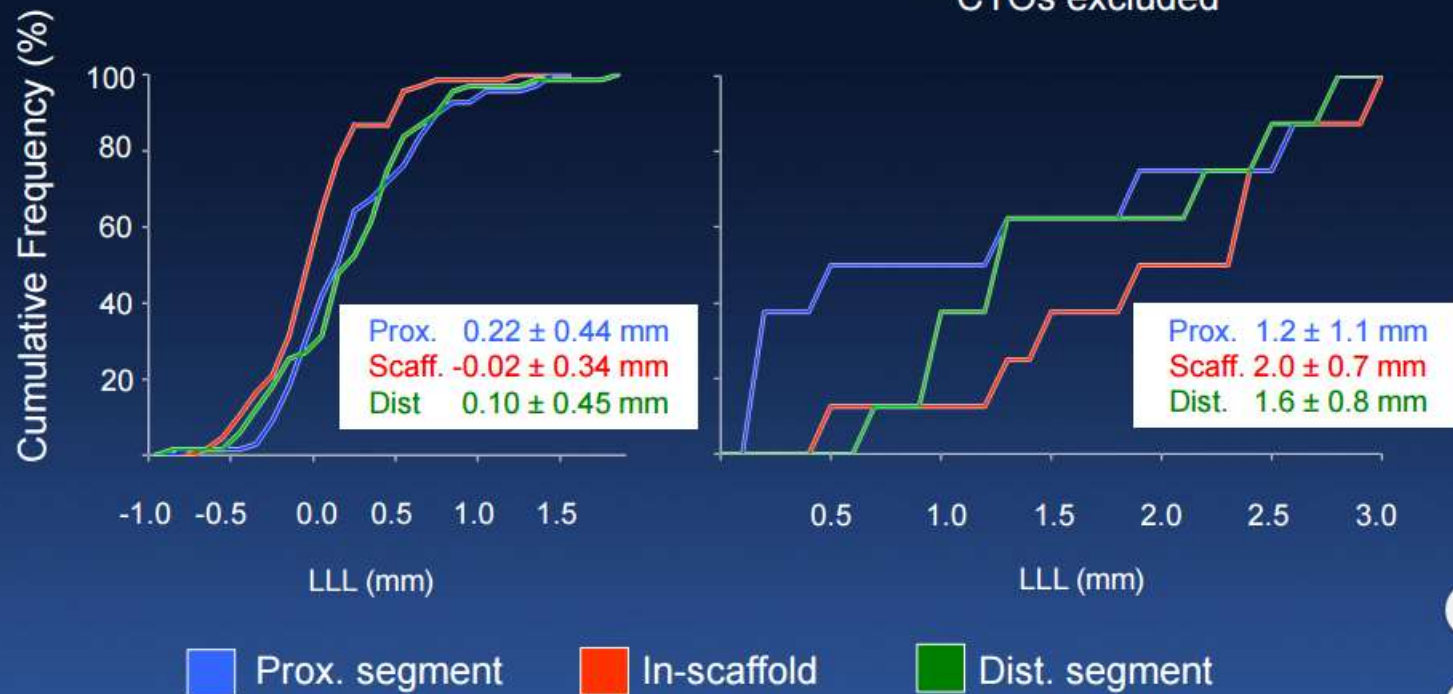

# ABSORB IV

## ABSORB III + IV Clinical Trial Program

### ABSORB IV

~3,000 pts randomized 1:1 ABSORB v XIENCE

RVD: 2.50 - 3.75 mm; Lesion length:  $\leq 24$  mm

Scaffold diameters: 2.5, 3.0 and 3.5 mm


Scaffold lengths: 12, 18, and 28 mm

~5,000 total pts (ABSORB III + IV) with up to 2 de novo lesions in different epicardial vessels randomized, with FU for at least 5 years, at up to 160 US and non-US sites

#### Primary endpoints:

1. Angina at 1 year (ABSORB IV)
2. TLF between 1 and 5 years (landmark analysis)

# ABSORB IV

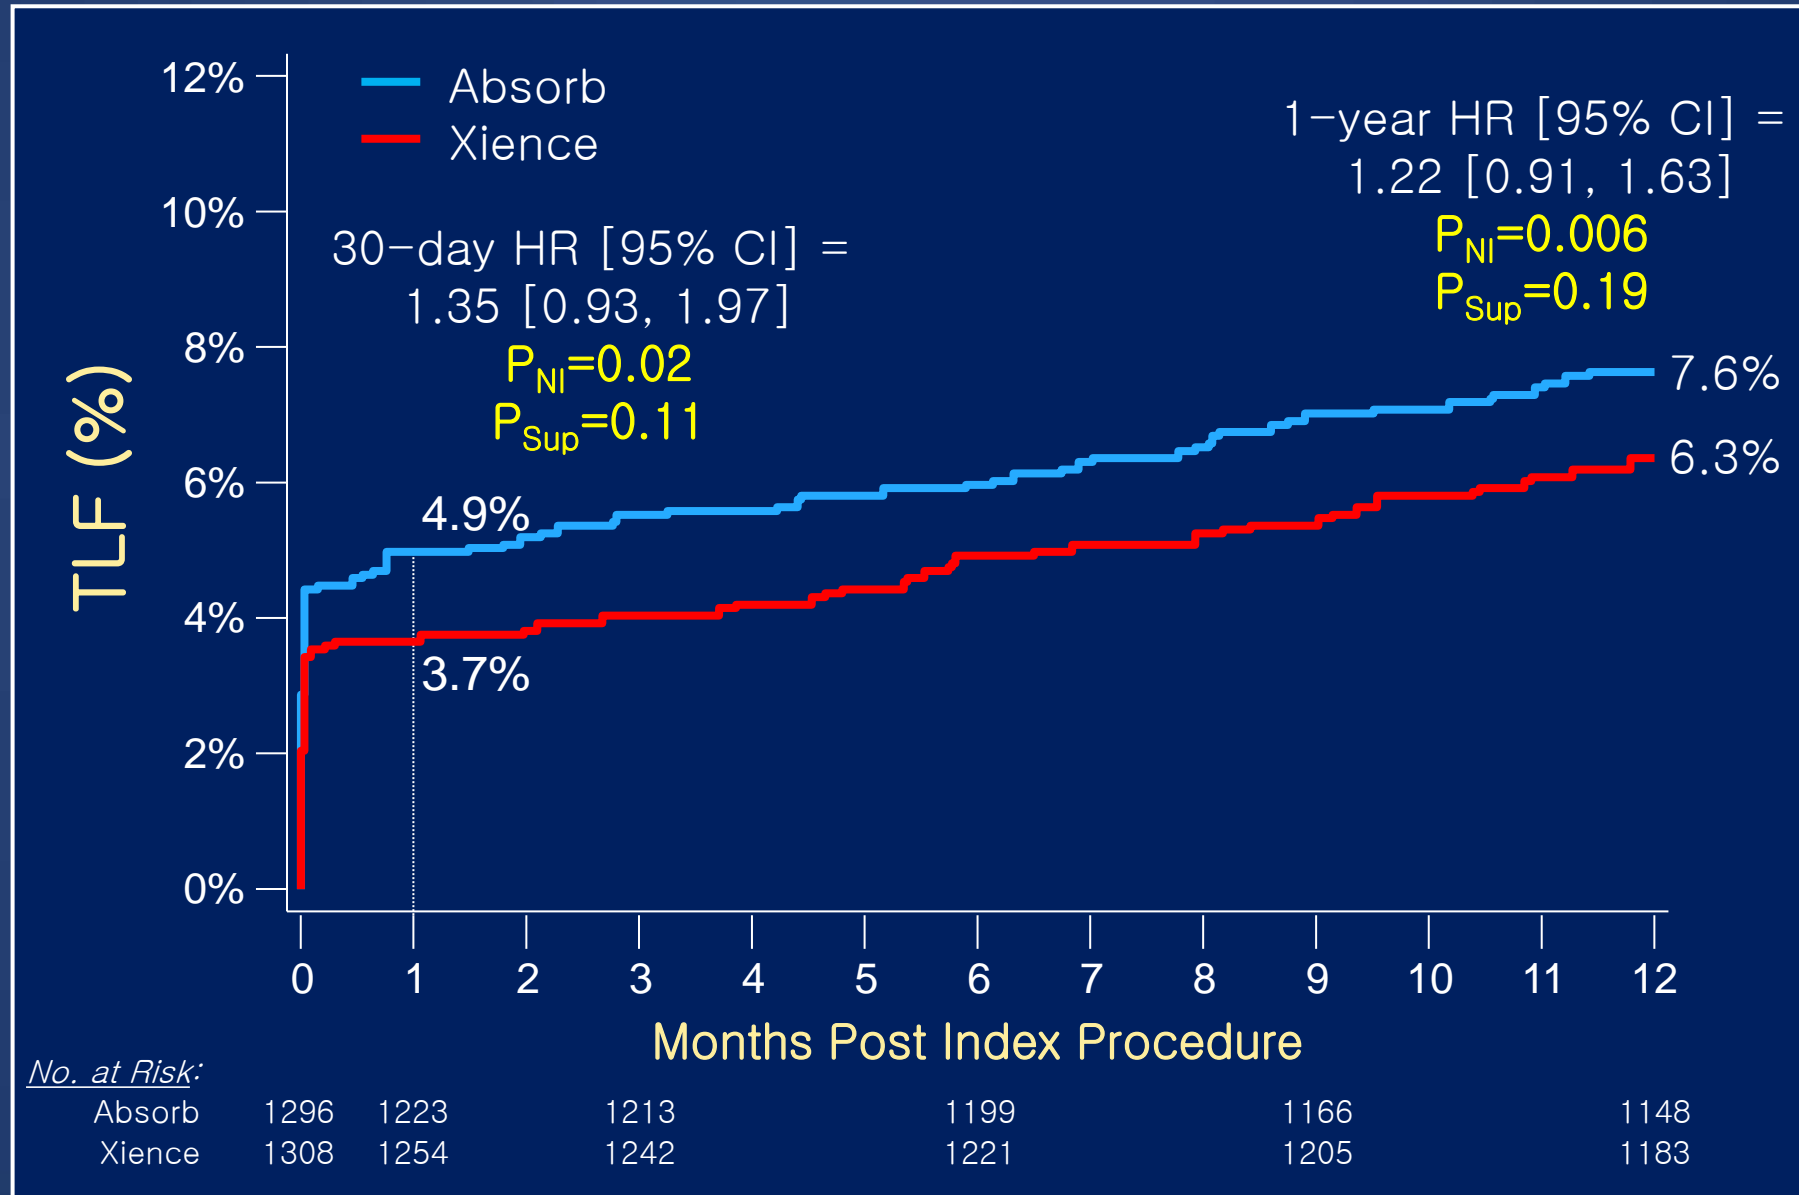


# ABSORB IV 1-Year Endpoints

	Absorb (N=1296)	Xience (N=1308)	p-value
TLF	7.6% (98)	6.3% (82)	0.19
- Cardiac death	0.8% (10)	0.6% (8)	0.62
- TV-MI	5.8% (75)	4.5% (58)	0.12
- ID-TLR	2.9% (37)	1.9% (24)	0.08
TVF (CD, MI, ID-TVR)	8.7% (111)	7.6% (99)	0.33
PoCE (death, MI, revasc)	9.7% (124)	8.6% (112)	0.35
- All-cause death	1.3% (16)	1.1% (14)	0.69
- MI	6.2% (80)	5.0% (65)	0.18
- Peri-procedural MI	3.8% (49)	3.4% (44)	0.56
- Spontaneous	2.6% (33)	1.7% (22)	0.12
- All revascularization	4.9% (63)	3.9% (50)	0.19
- ID-TVR	4.0% (51)	2.9% (37)	0.11

# ABSORB IV 30-Day Endpoints


	Absorb (N=1296)	Xience (N=1308)	p-value
TLF	4.9% (64)	3.7% (48)	0.11
- Cardiac death	0.1% (1)	0% (0)	0.32
- TV-MI	4.4% (57)	3.6% (47)	0.29
- ID-TLR	1.0% (13)	0.2% (3)	0.02
TVF (CD, MI, ID-TVR)	5.1% (66)	3.7% (48)	0.08
PoCE (death, MI, revasc)	5.2% (67)	4.1% (53)	0.17
- All-cause death	0.1% (1)	0.1% (1)	0.99
- MI	4.5% (58)	3.6% (47)	0.25
- Peri-procedural MI	3.8% (49)	3.4% (44)	0.56
- Spontaneous	0.8% (10)	0.2% (3)	0.05
- All revascularization	1.5% (19)	0.6% (8)	0.03
- ID-TVR	1.2% (16)	0.2% (3)	0.003

# ABSORB IV

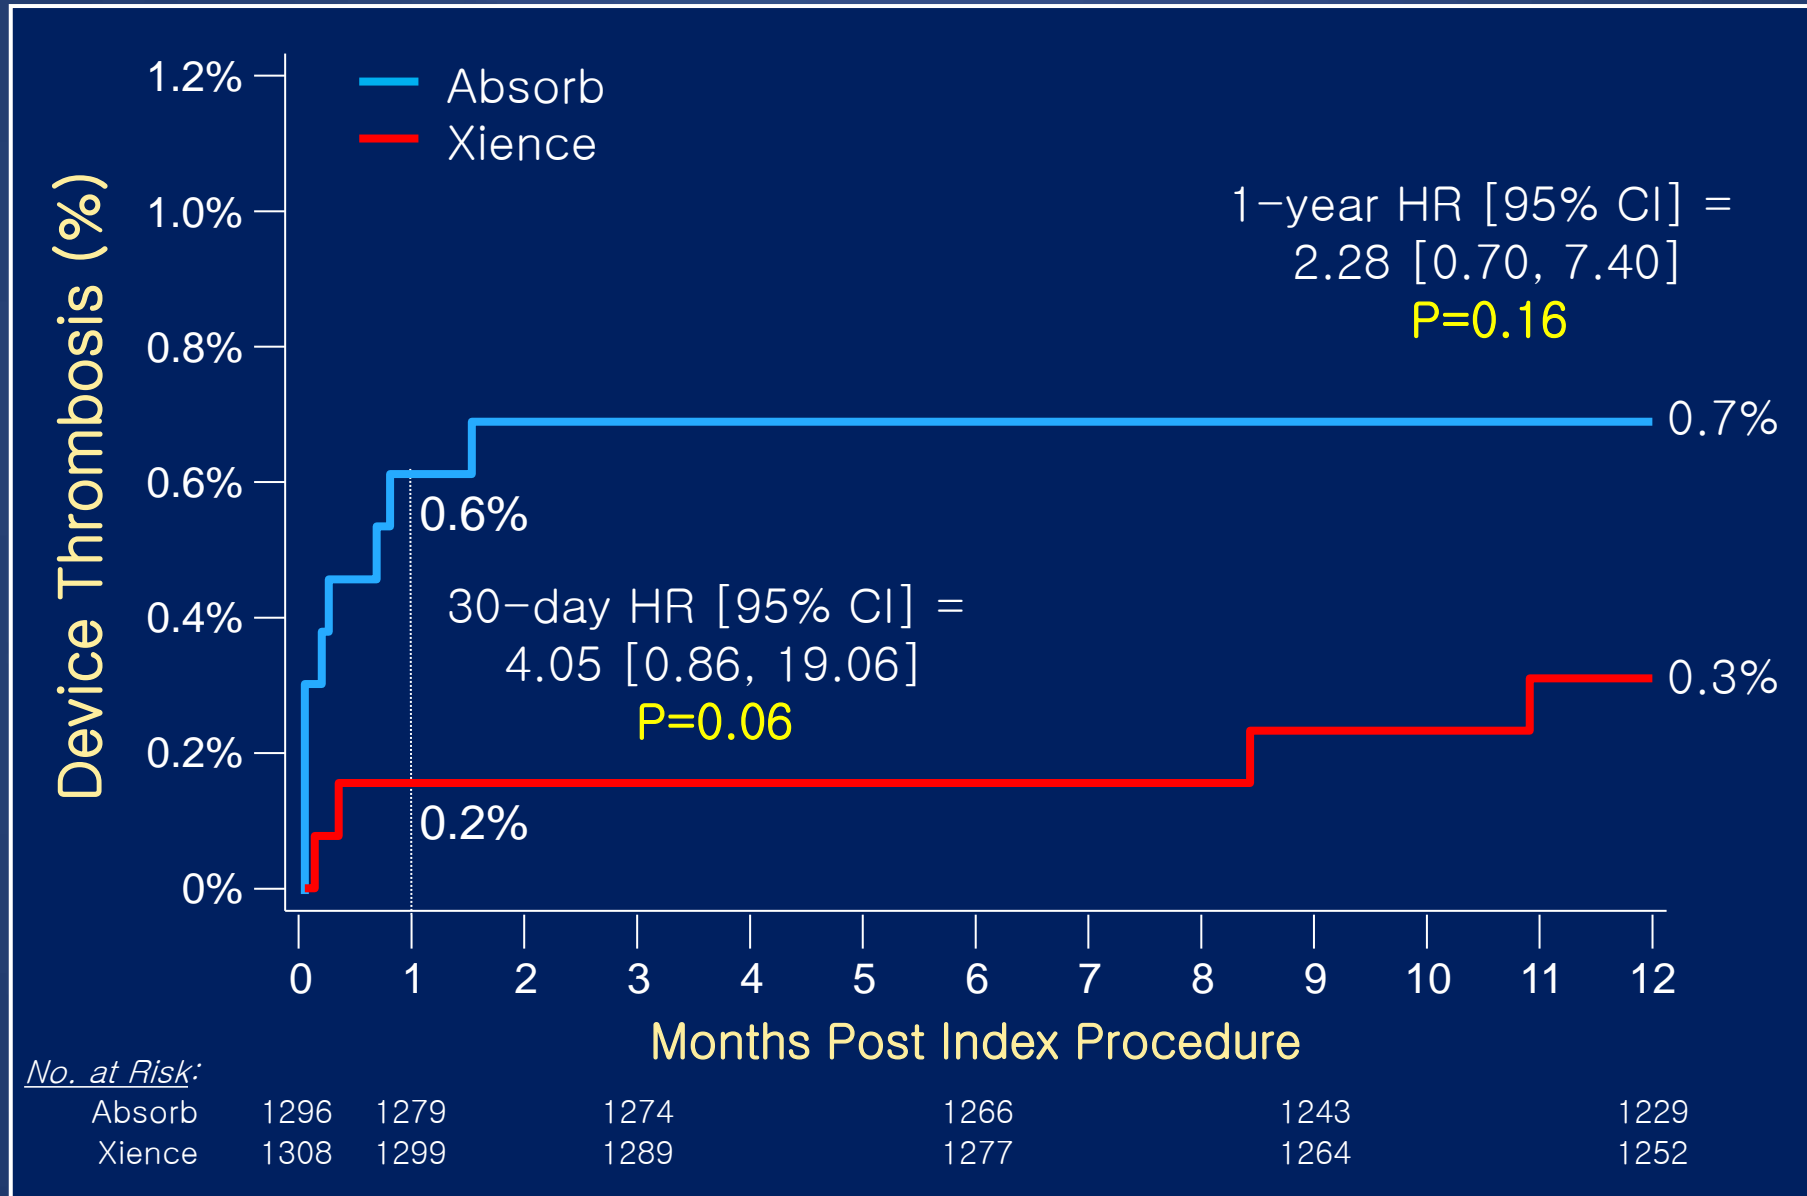




# ABSORB IV

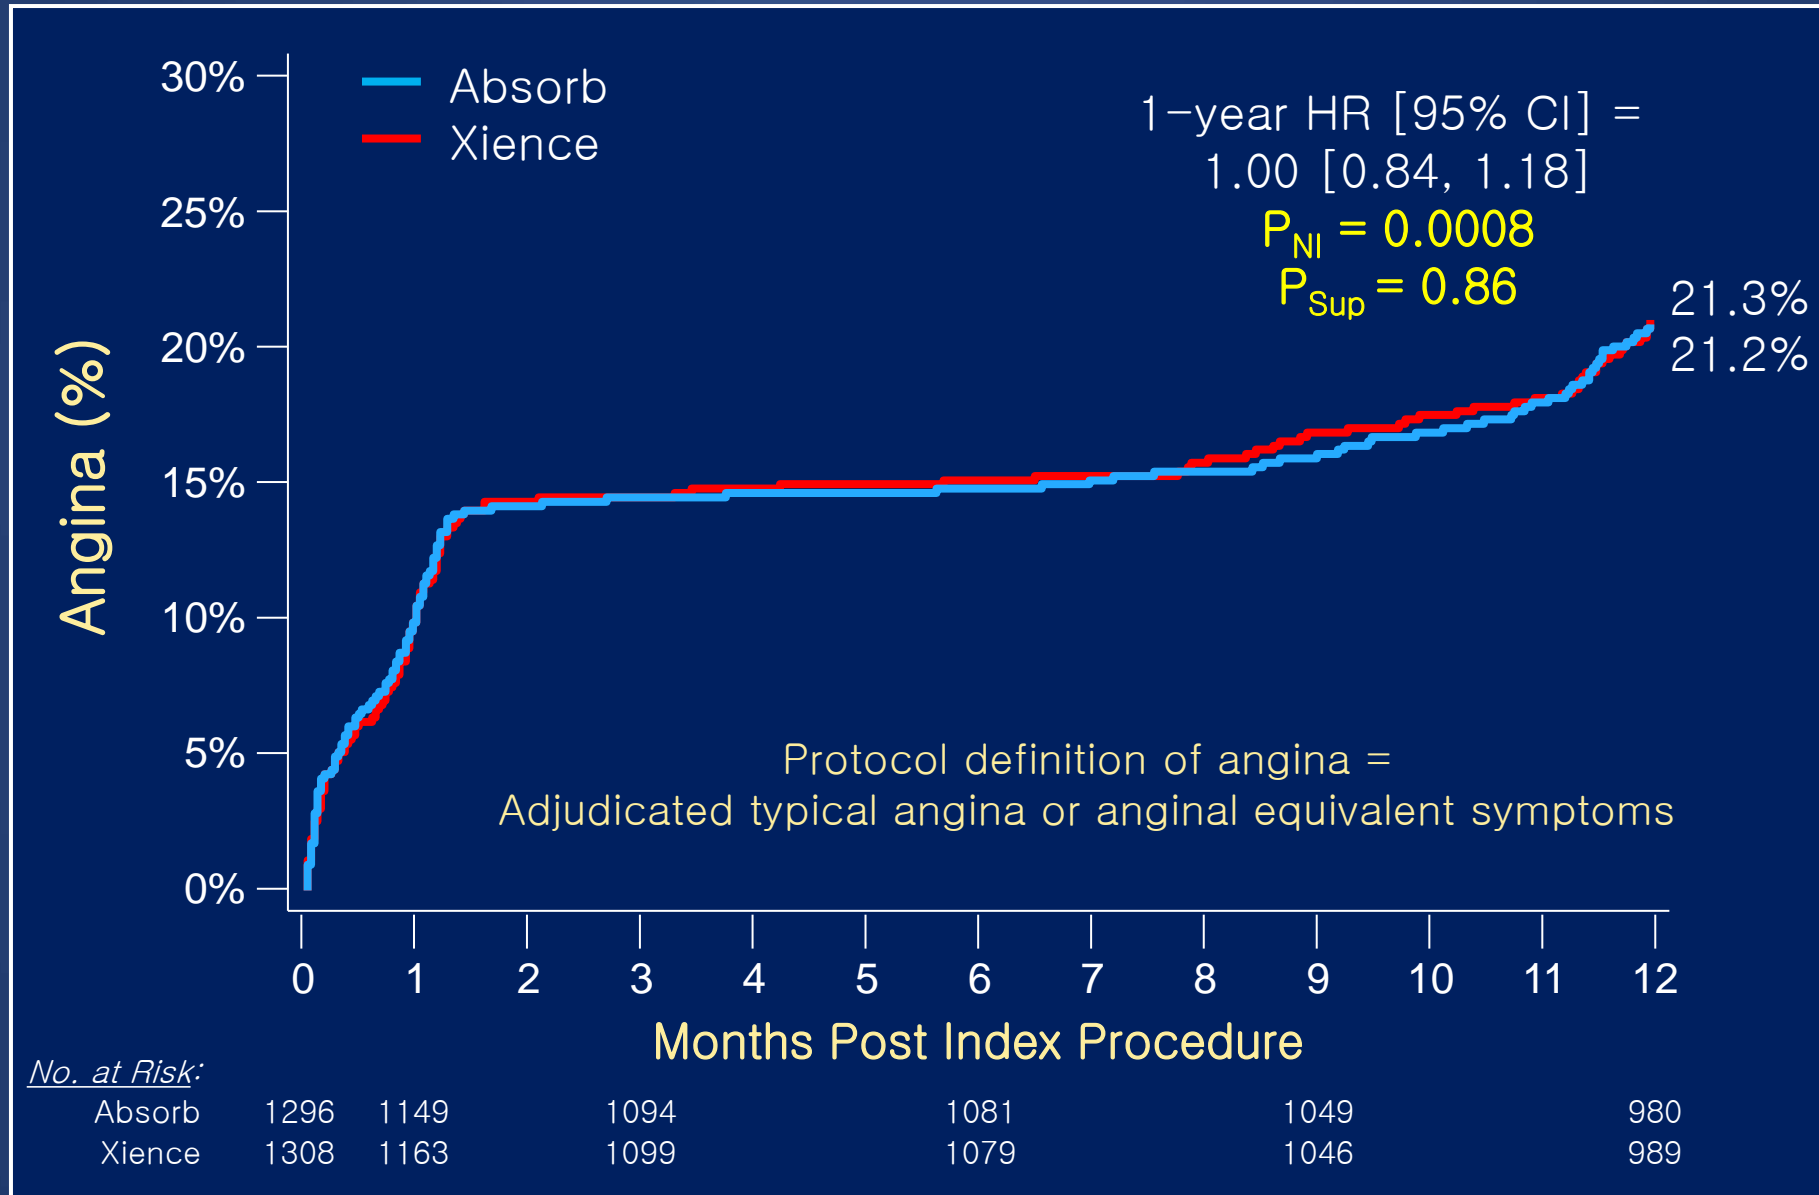


# AIDA 2-years

## Target-vessel Failure

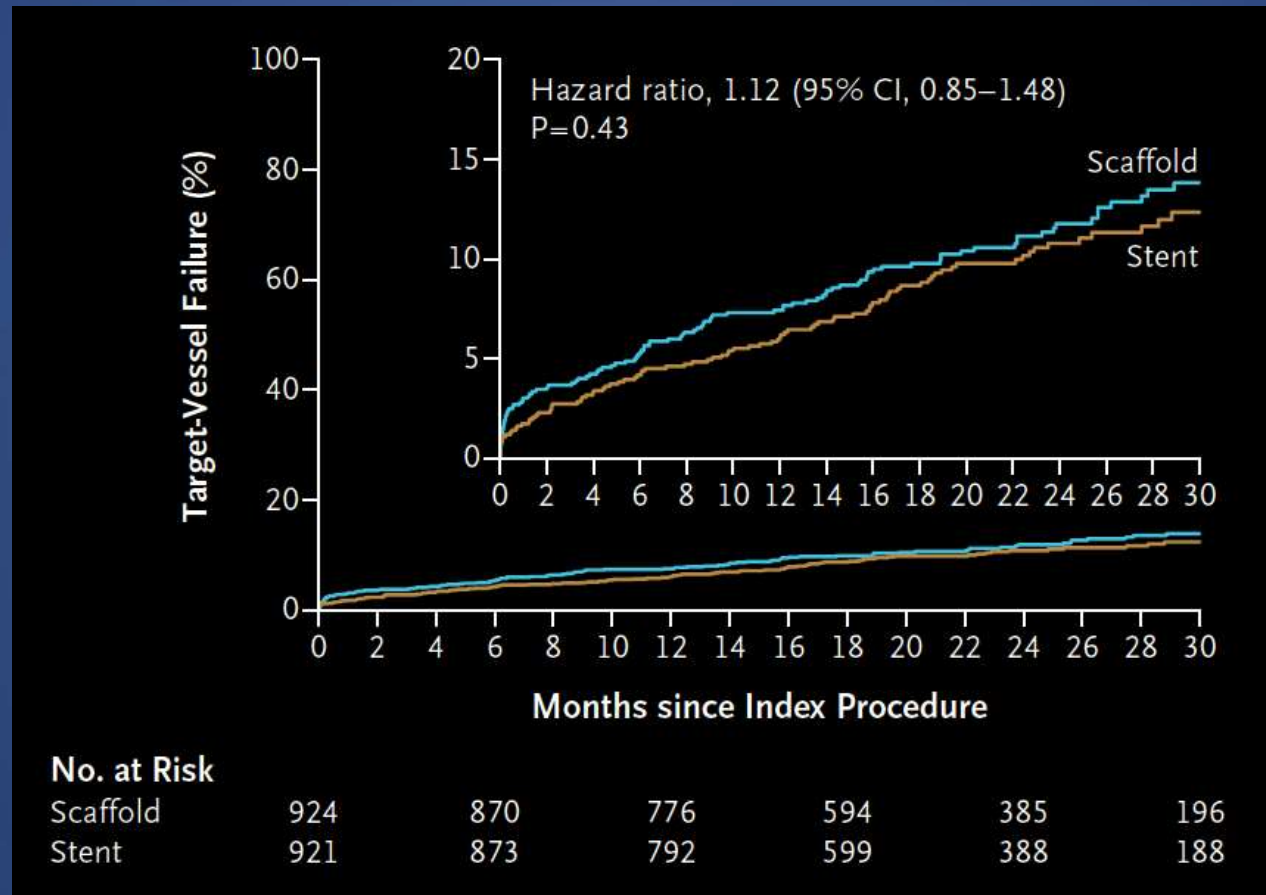


# AIDA 2-years

## Definite device thrombosis

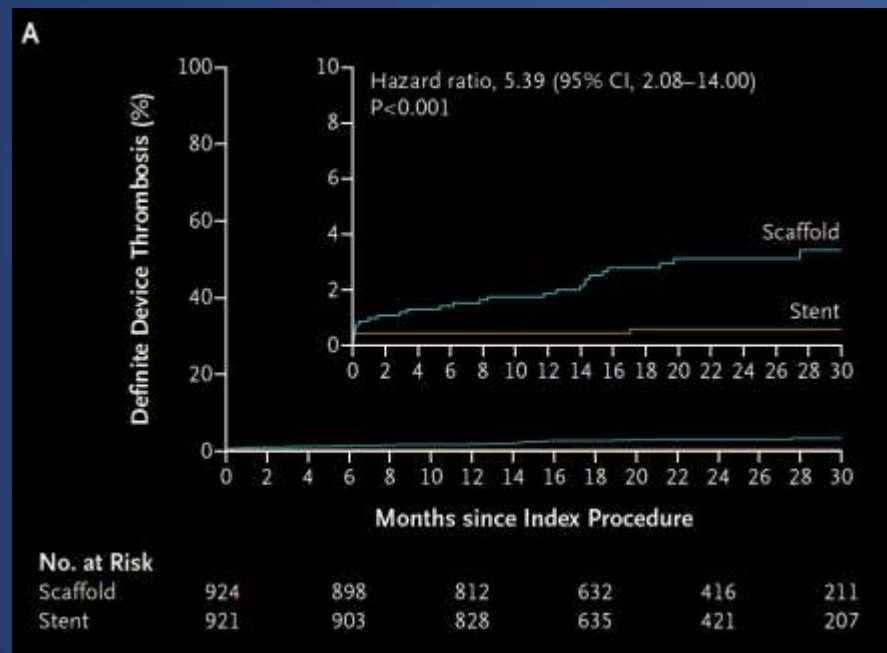

## Definite or probable device thrombosis

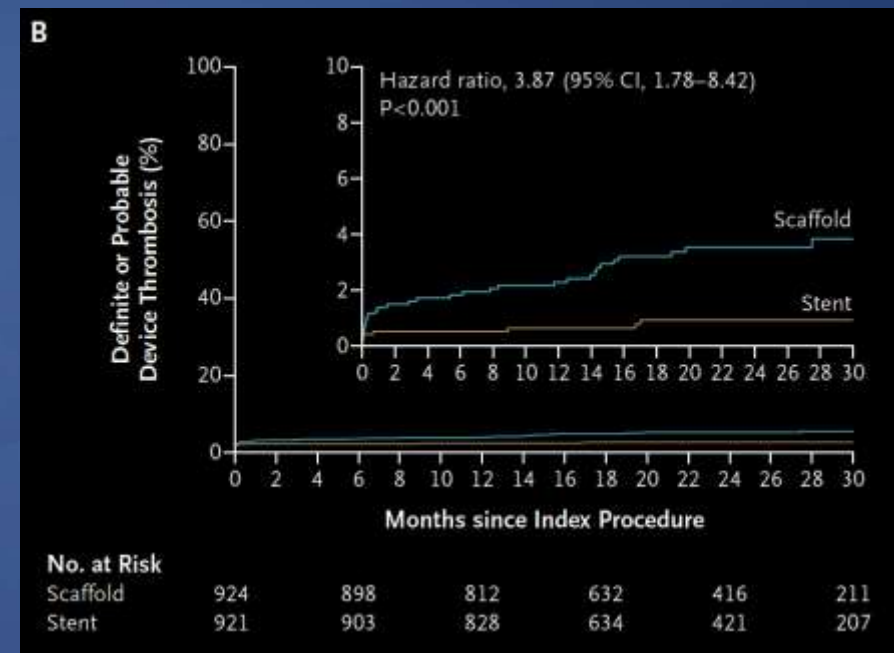

# COMPARE-ABSORB

## Primary endpoint 1 year TLF non-inferiority analysis

- Assumed difference between Xience and Absorb : 0 %
- Non inferiority margin : 4.5 %
- One sided 2.5% significance level
- TLF rate Xience 4.2%
- TLF rate Absorb 5.1%

$\Delta$  Prim. EP: Absorb - Xience = 0.9 % (95% CI: -1.2 – 3.0 %)




Absorb is non-inferior compared to Xience

$P < 0.001$

# COMPARE-ABSORB




## TLF at 1 year

Cardiac death, target vessel myocardial infarction,  
clinically-indicated target lesion revascularization

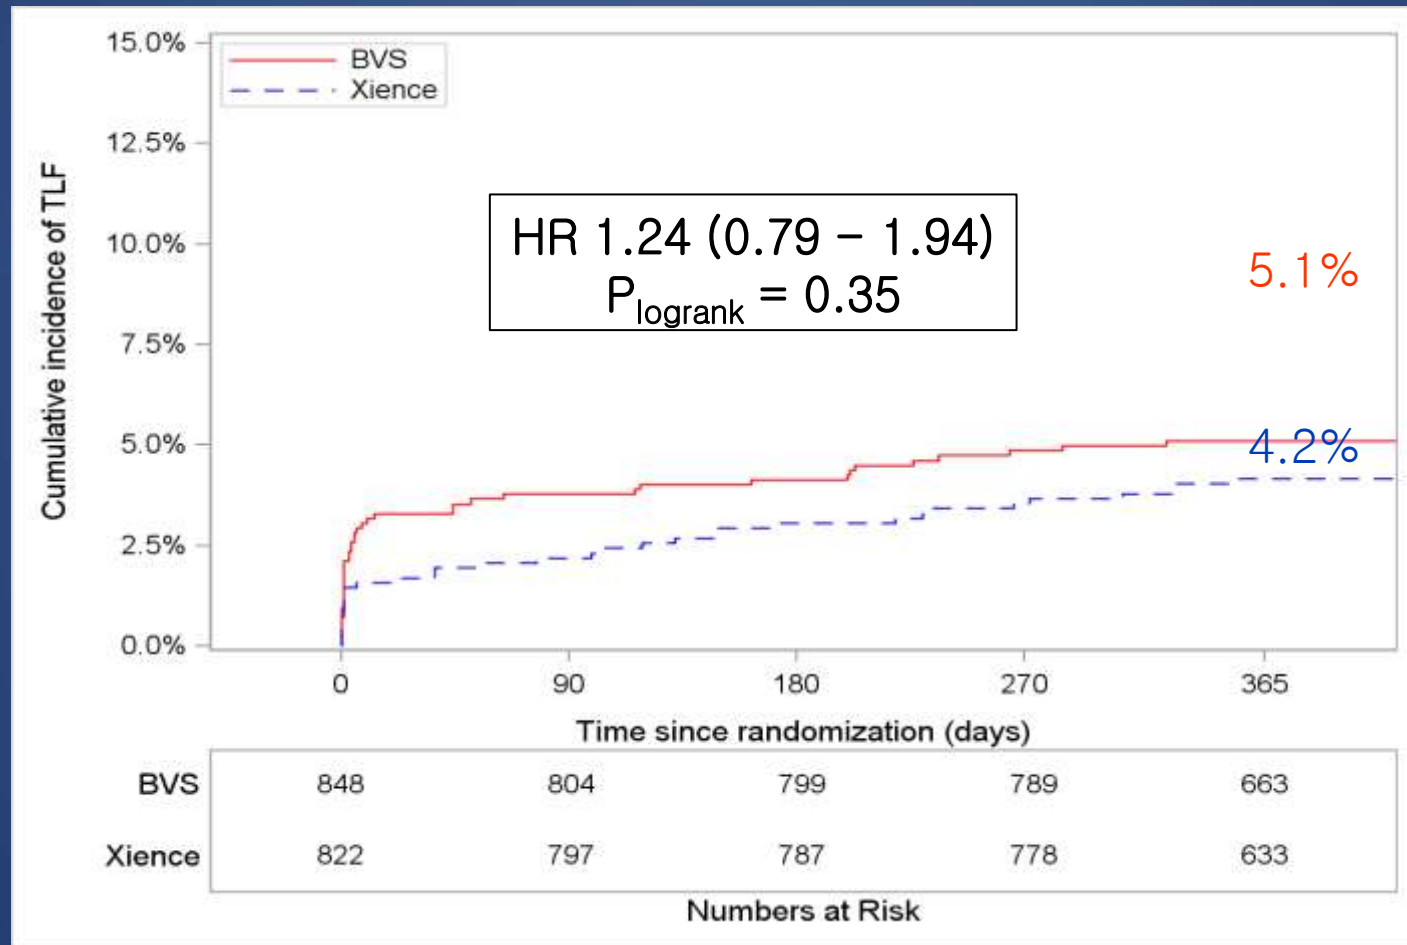

# COMPARE-ABSORB

## Components of TLF

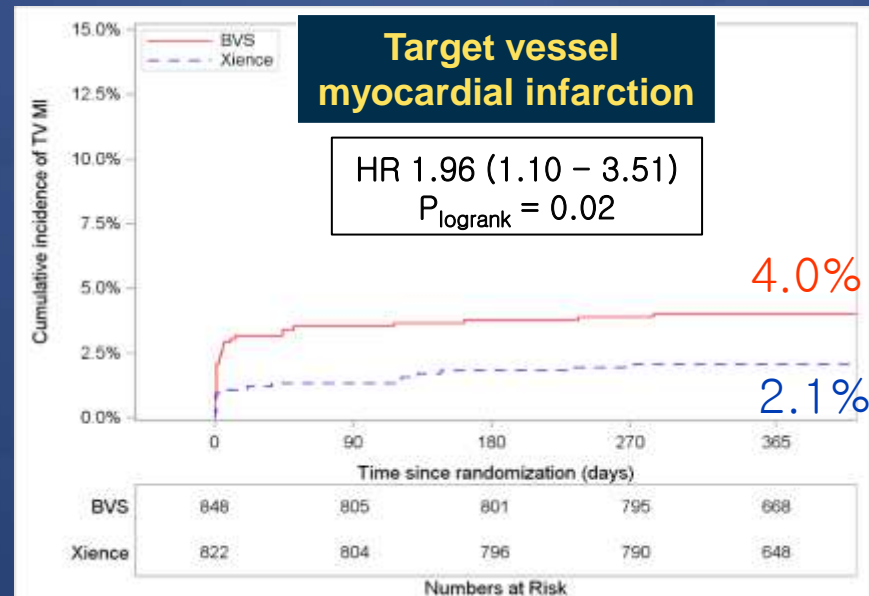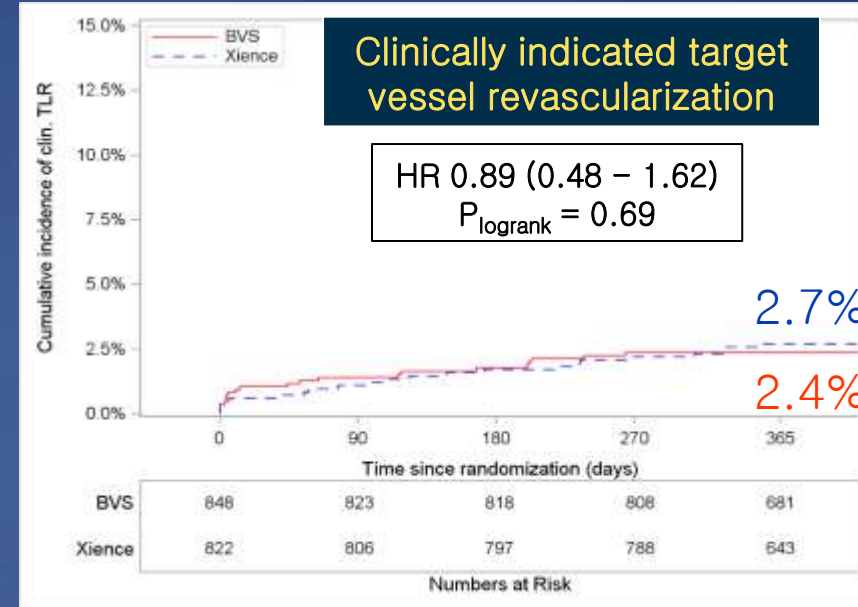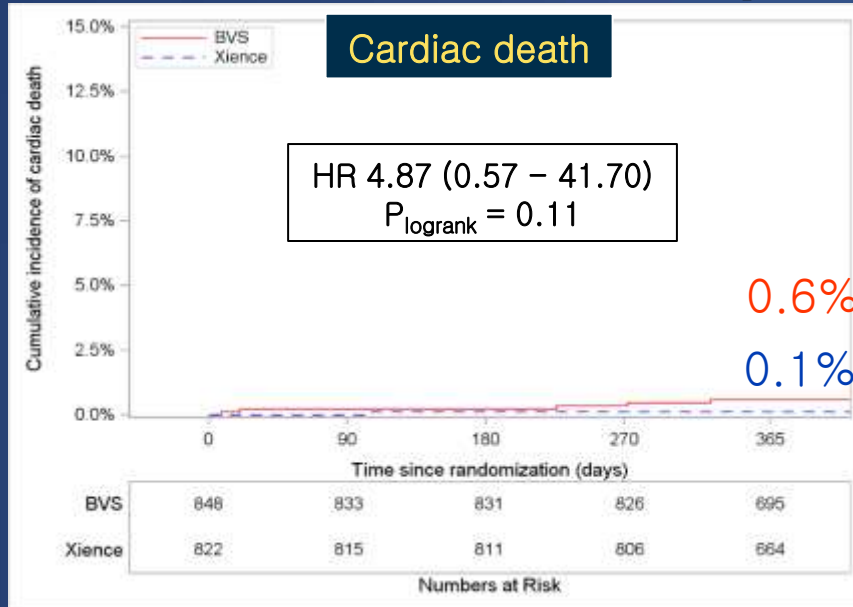

### MI definition:


- SCAI (peri-procedural)
- TUD (spontaneous)



# COMPARE-ABSORB

## Stent/Scaffold Thrombosis @ 1 year


Definite Stent/Scaffold Thrombosis (ARC definition)

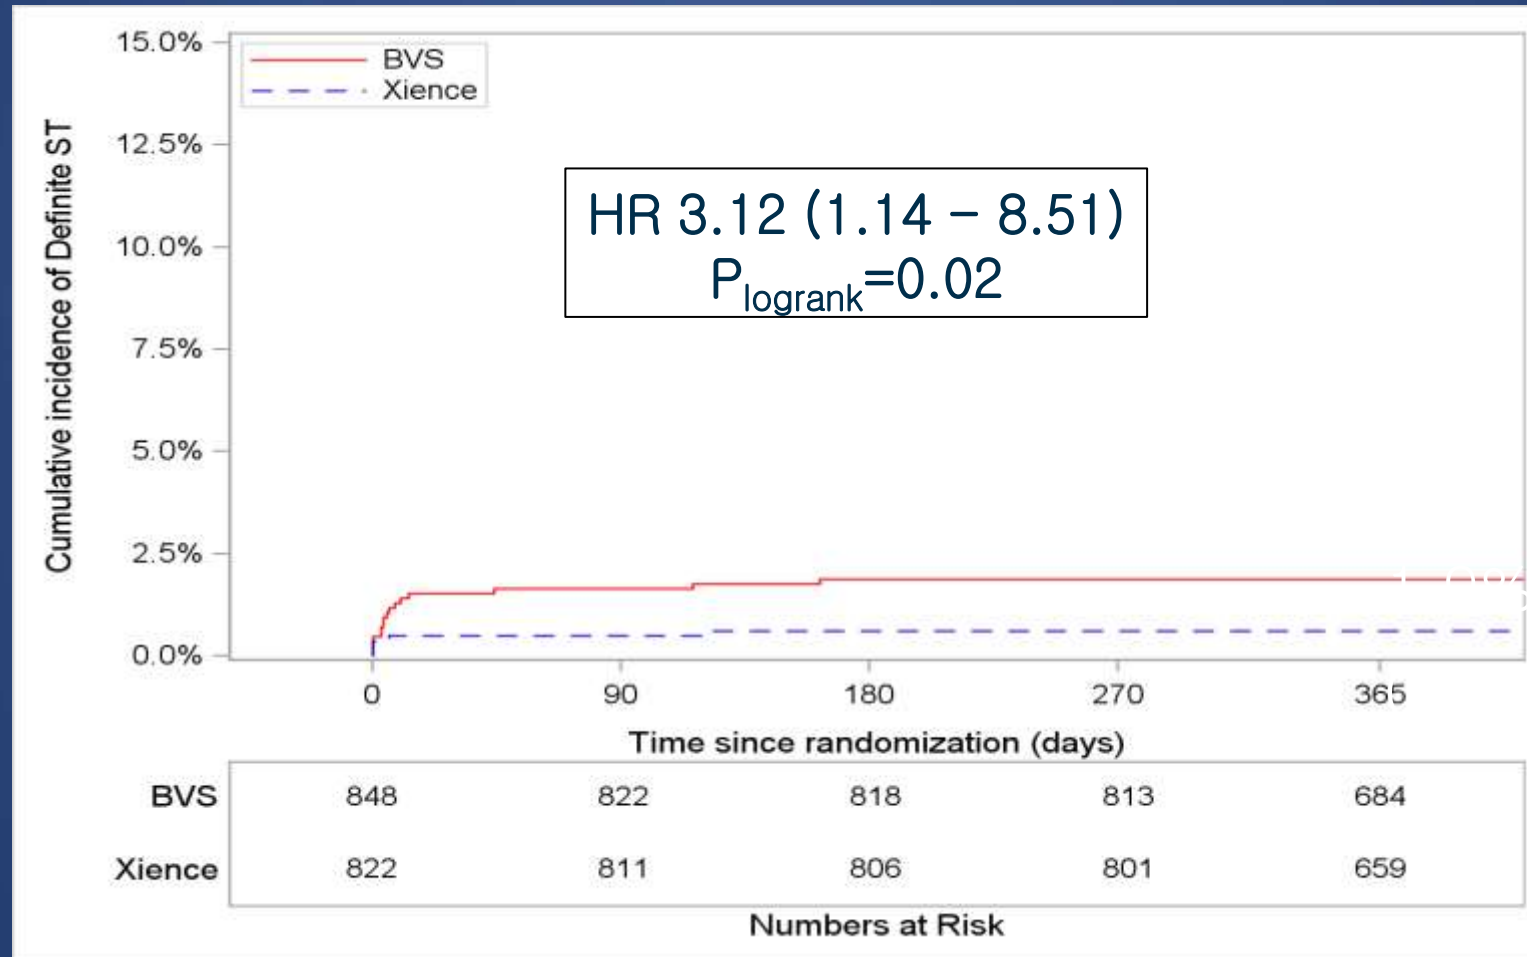

# COMPARE-ABSORB


Stent/Scaffold Thrombosis @ 1 year

Definite and Probable Stent/Scaffold Thrombosis  
(ARC definition)

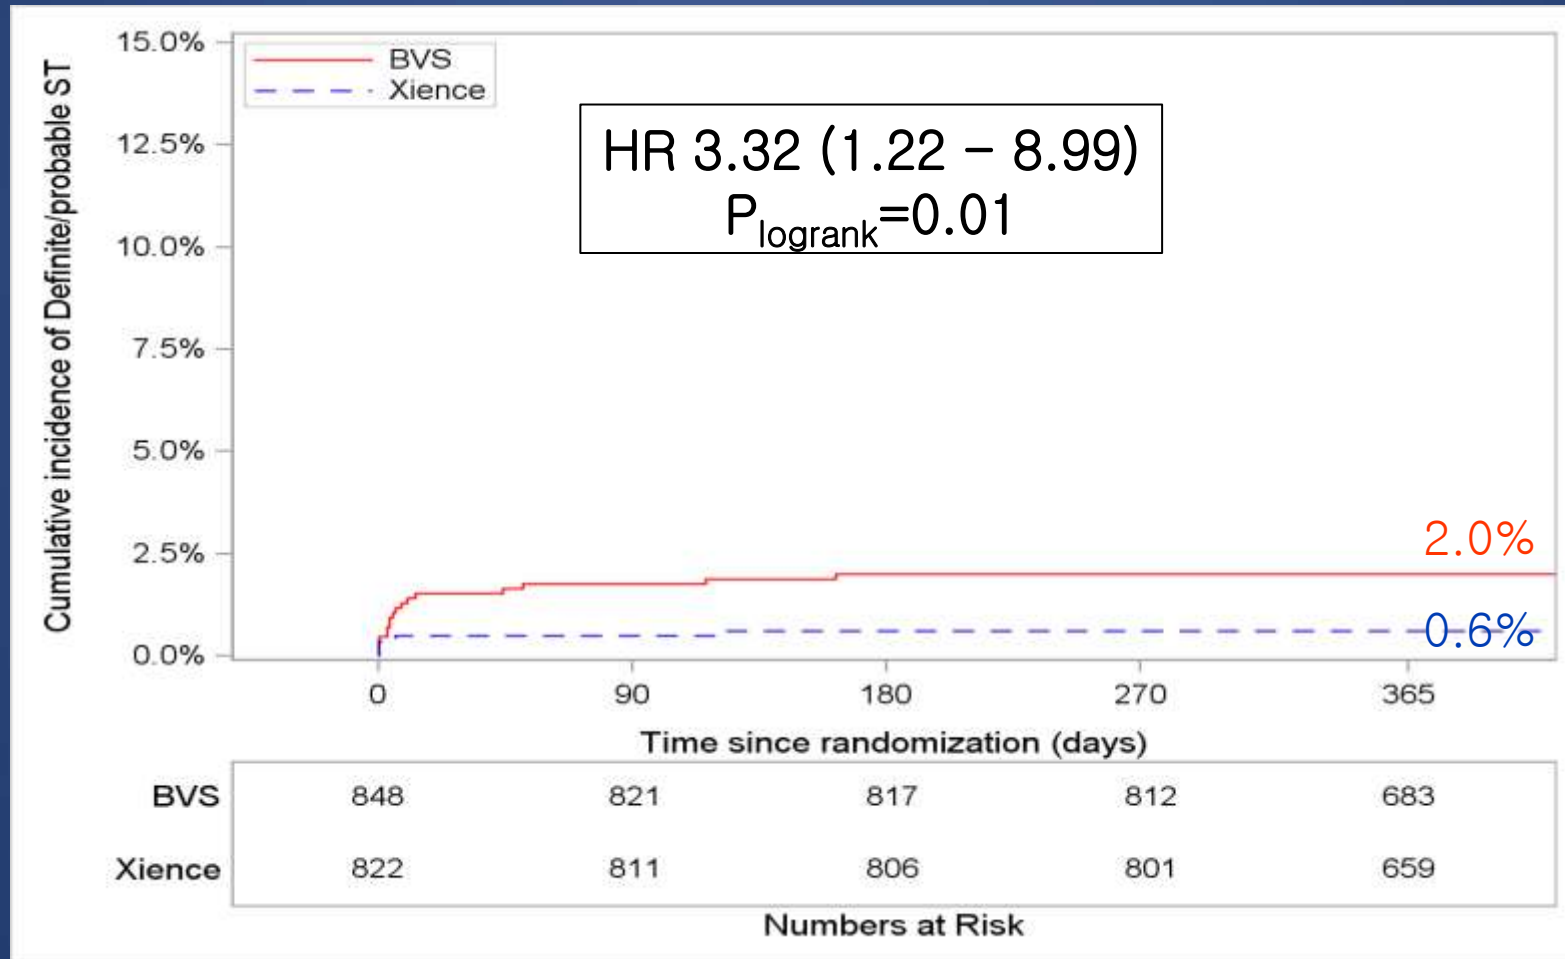



# COMPARE-ABSORB

## Clinical events

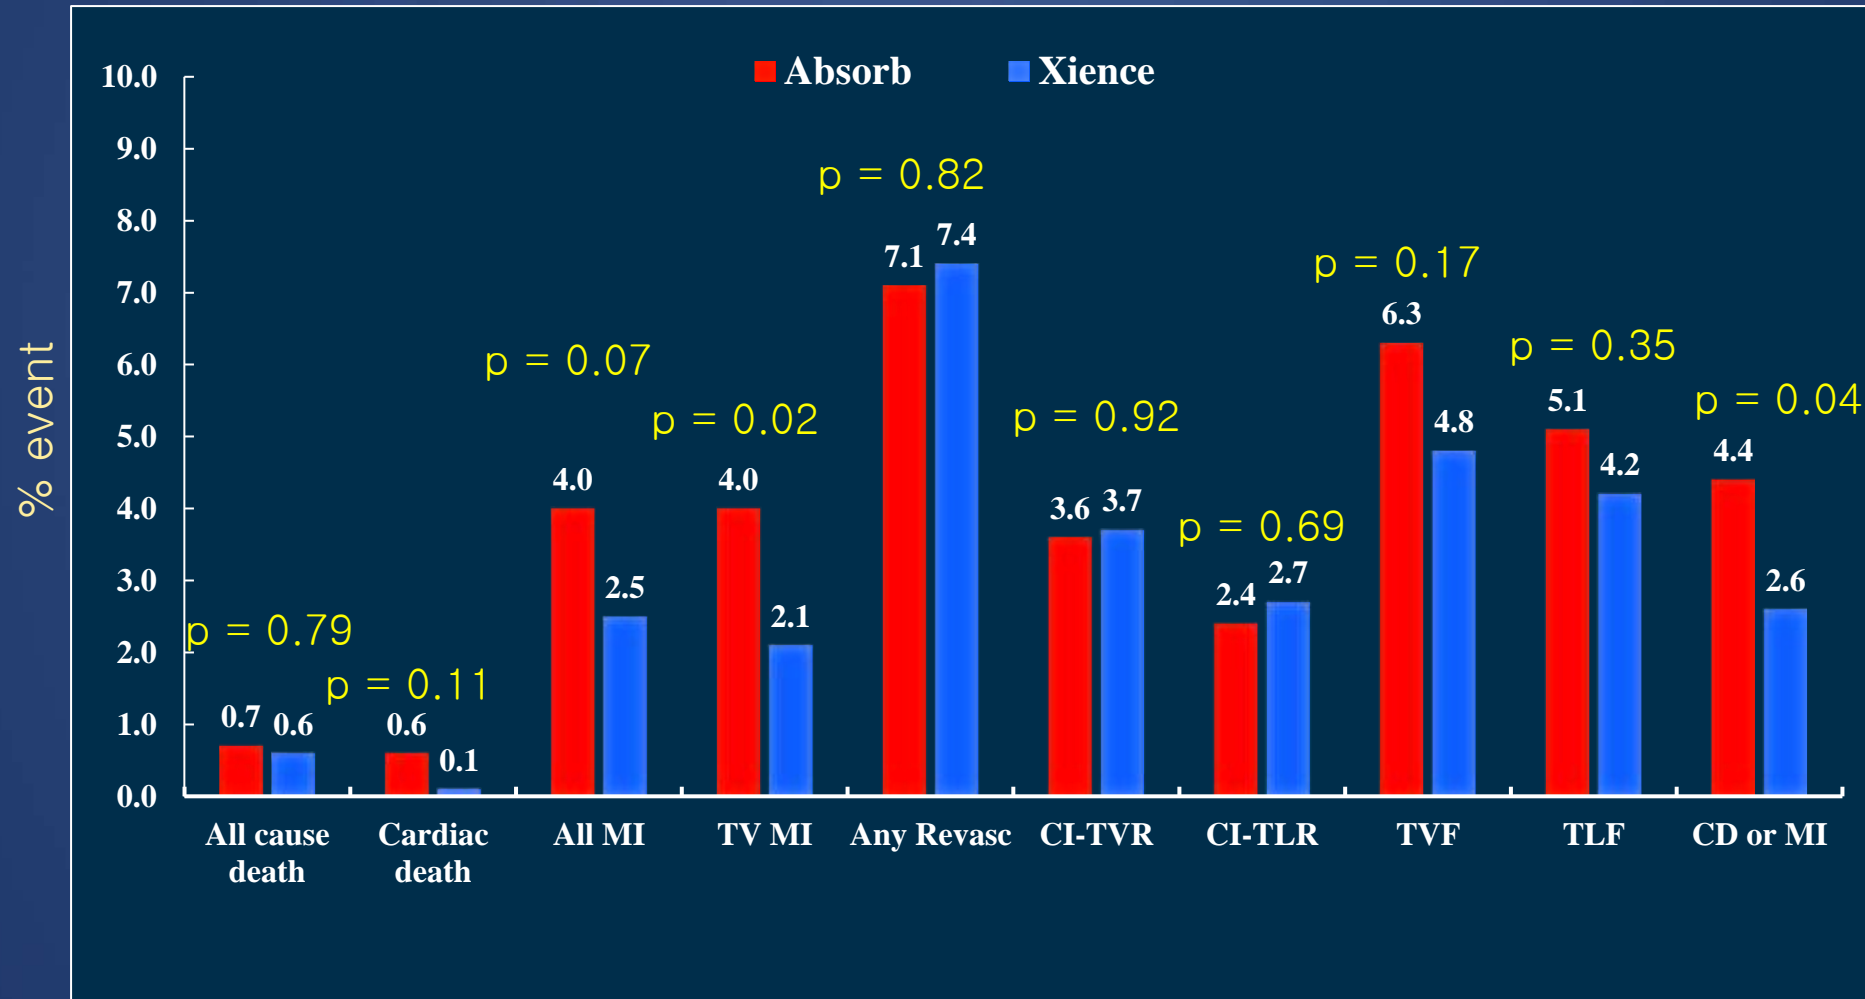

# COMPARE-ABSORB


## Device thrombosis

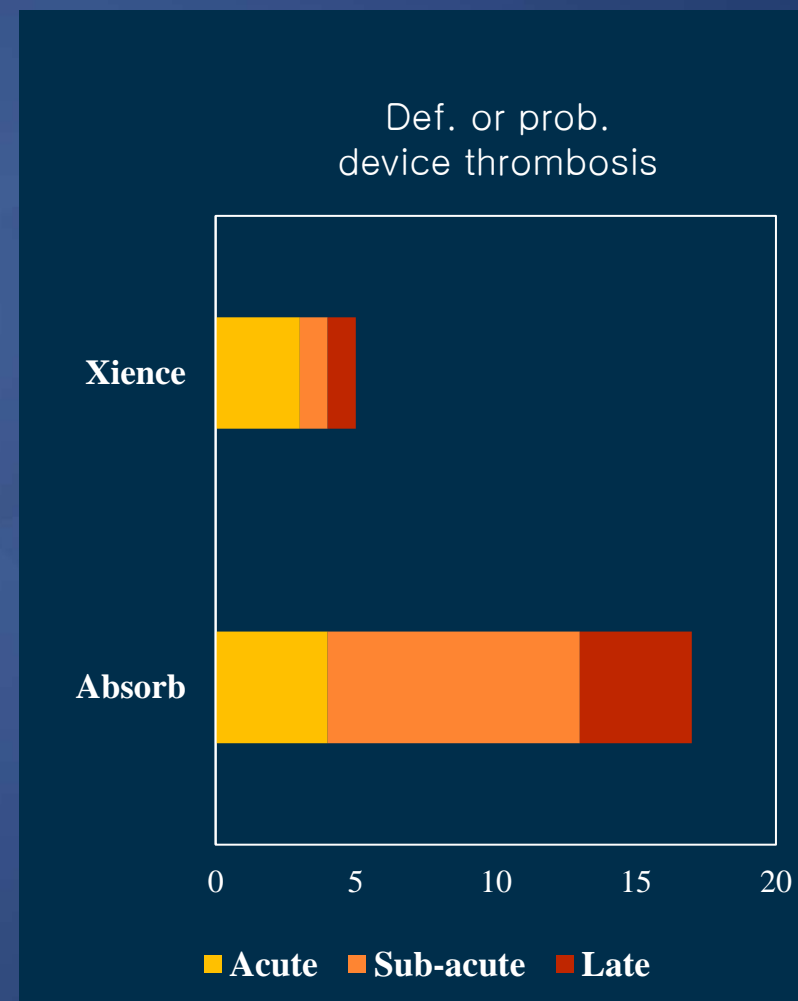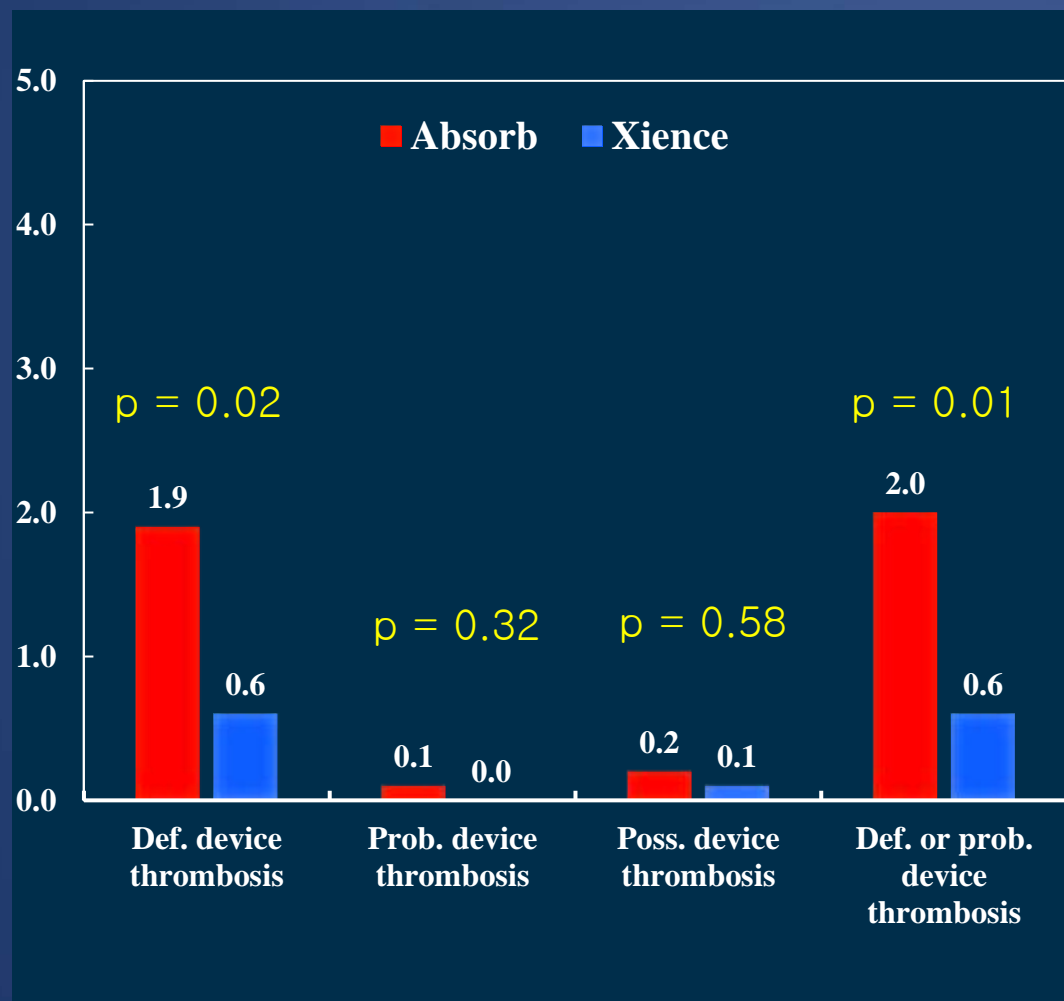

# Meta-analysis of ABSORB

Individual pt data pooled analysis of 4 randomized trials of BVS vs. EES (ABSORB II, III, Japan, China; N=3389 pts)


2-year target lesion failure

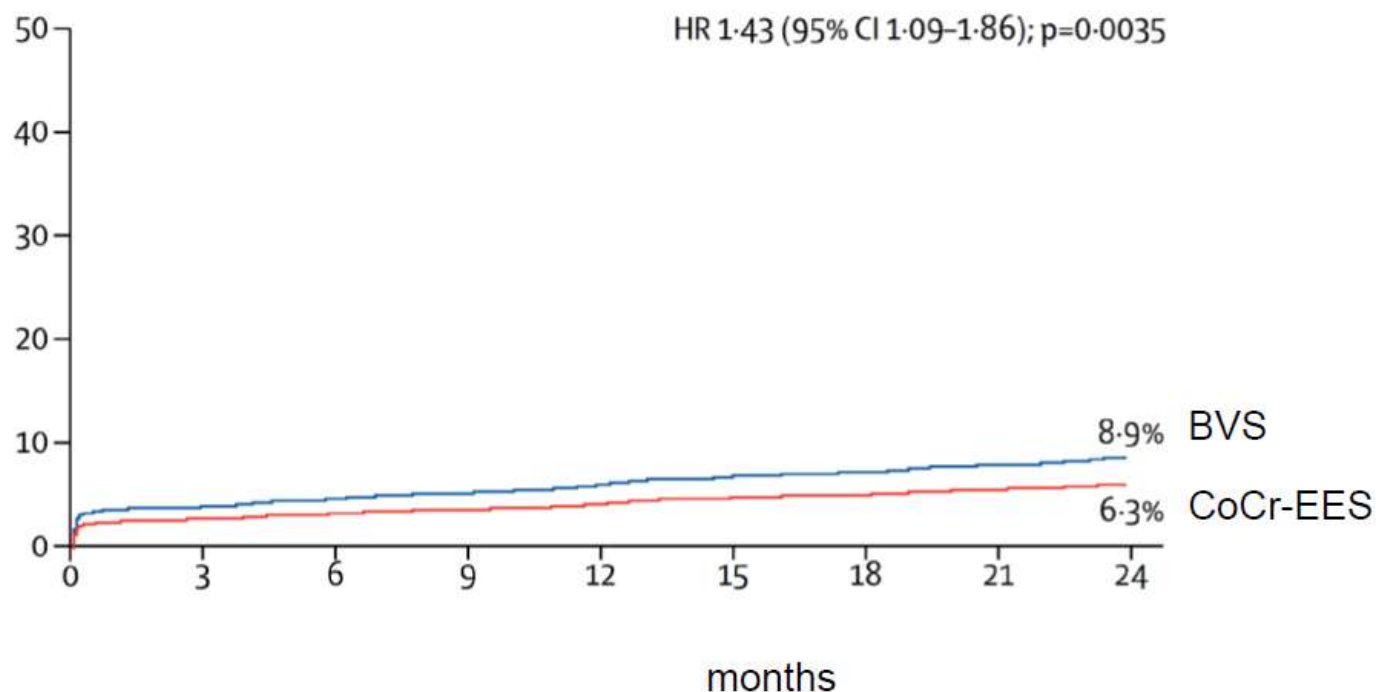

# ABSORB: 3-year Outcomes

Meta-analysis of 4 BVS vs. EES RCTs (n=3,389 pts)

## 3-Year TLF

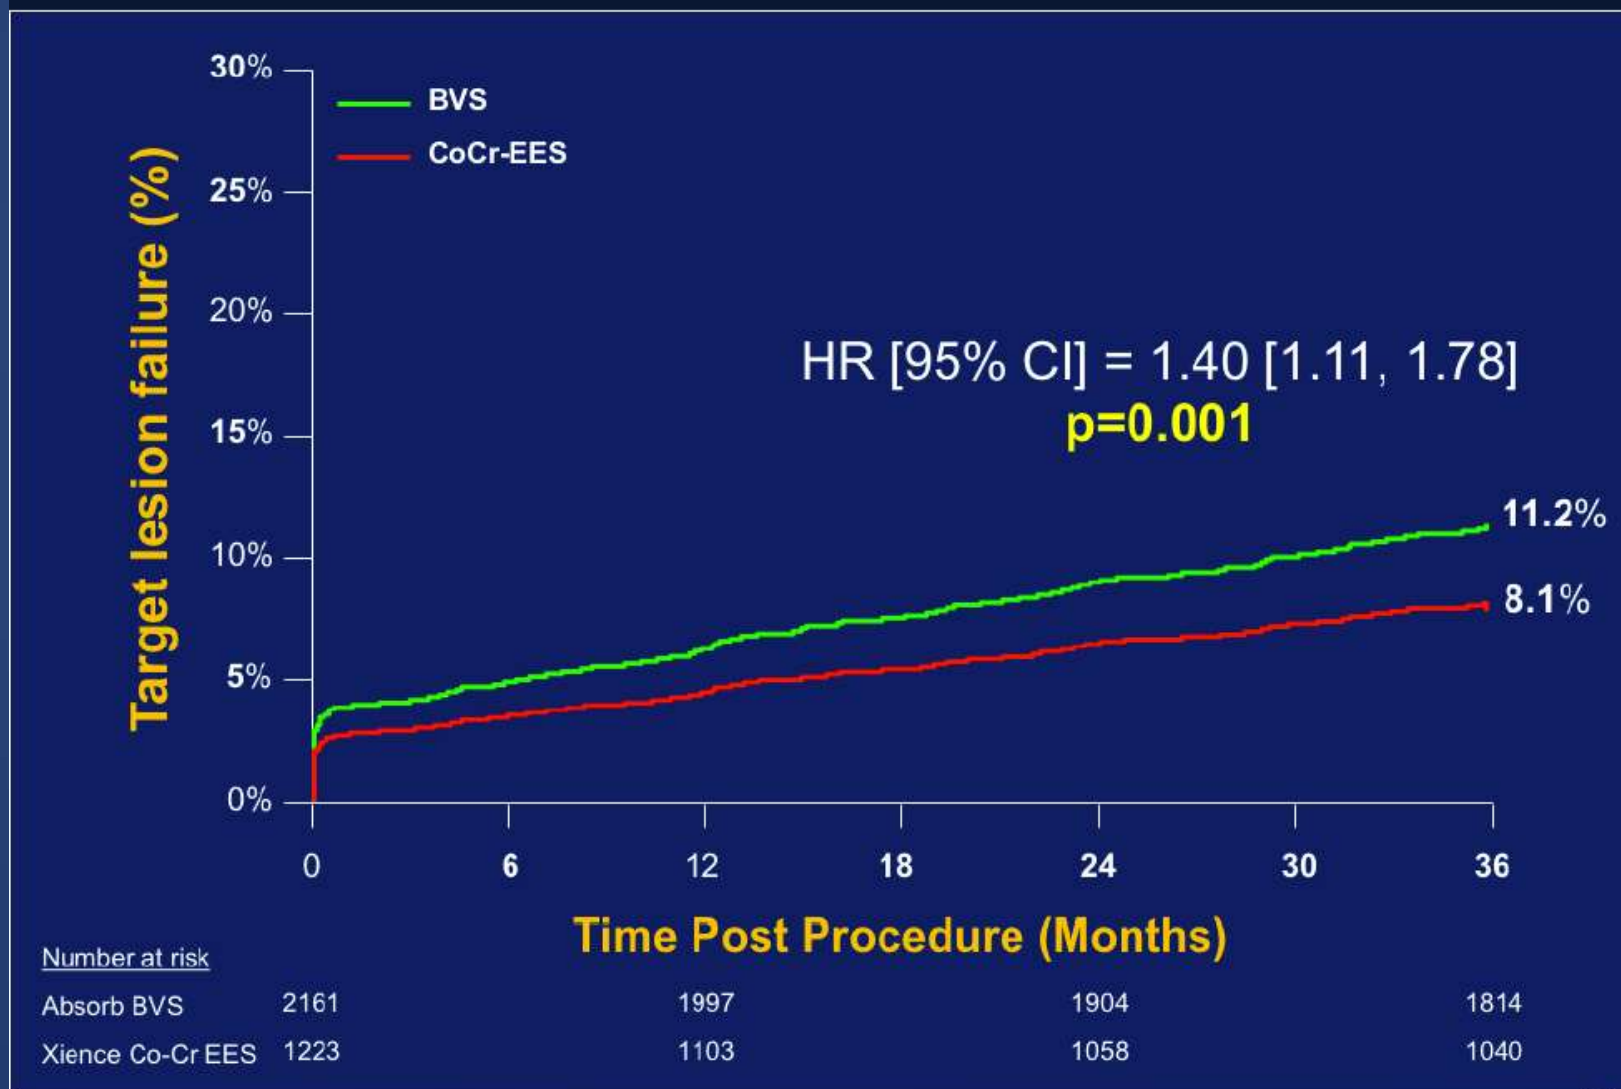




# ABSORB: 3-year Outcomes

Meta-analysis of 4 BVS vs. EES RCTs (n=3,389 pts)

## 3-Year Device Thrombosis

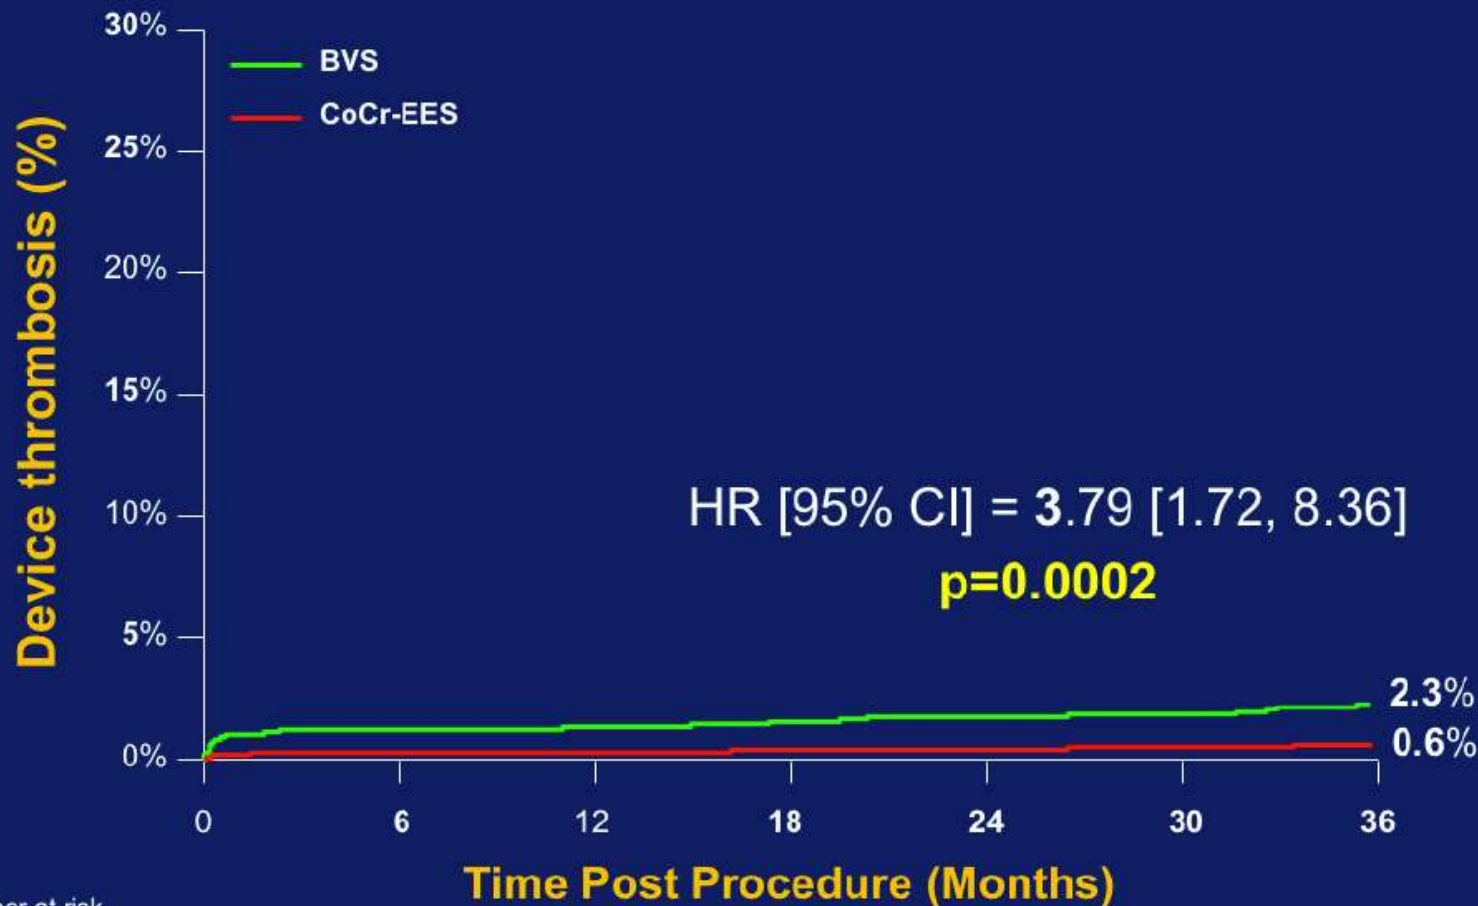

Number at risk

Absorb BVS	2161	2092	2042	1981
Xience Co-Cr EES	1223	1195	1169	1144



# ABSORB: 4-year Outcomes

Meta-analysis of 4 BVS vs. EES RCTs (n=3,389 pts)

## 4-Year TLF






# ABSORB: 4-year Outcomes

Meta-analysis of 4 BVS vs. EES RCTs (n=3,389 pts)

## 4-Year Device Thrombosis

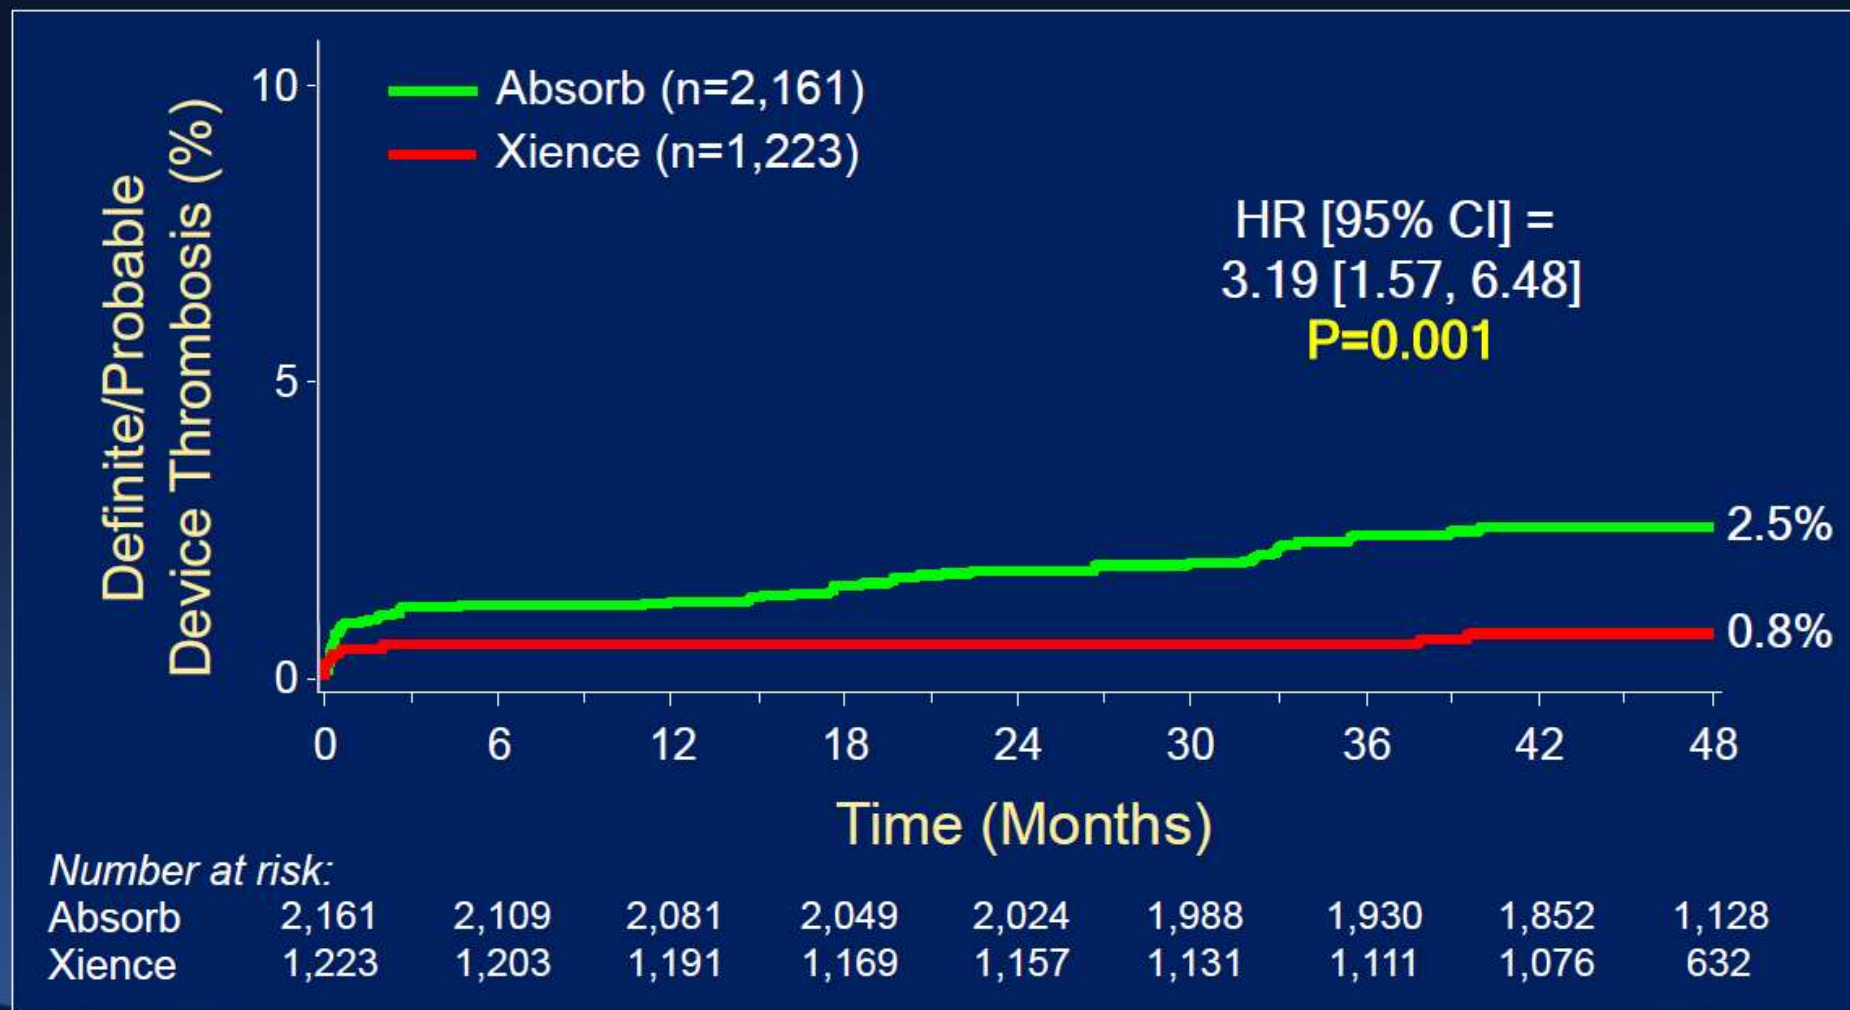





# **ABSORB** 4-Year Meta-analysis


Conclusions from 4 trials and 3,389 randomized patients

- Absorb BVS resulted in higher cumulative 4-year rates of TLF and device thrombosis compared with Xience CoCr-EES
- However, after 3 years, the point of complete polymer bioresorption, the excess risk from BVS has resolved, offering the potential for the long-term advantages of bioresorbable scaffold technology to emerge


# **BRS and imaging**

# ABSORB

Left main stem and ostial LAD disease

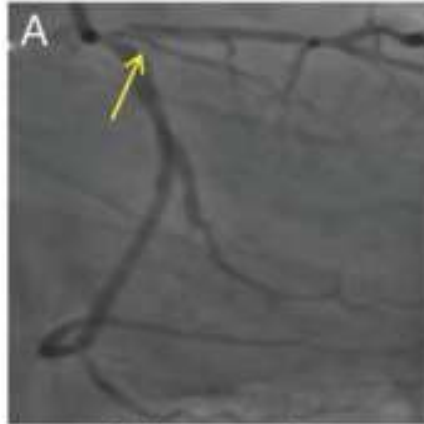


Before procedure

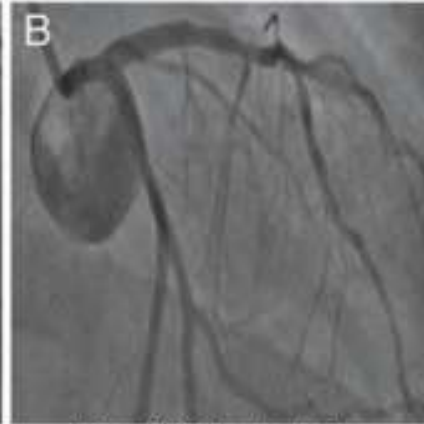


After BVS implantation

LAD stenosis distal to insertion of LIMA graft

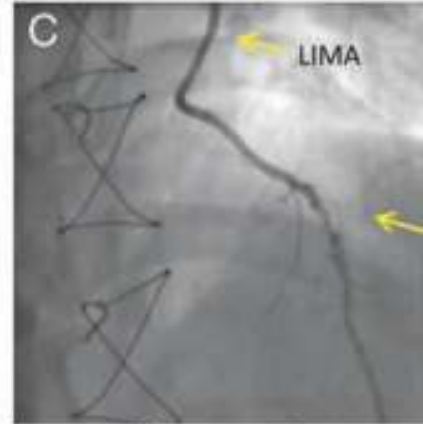

Before procedure

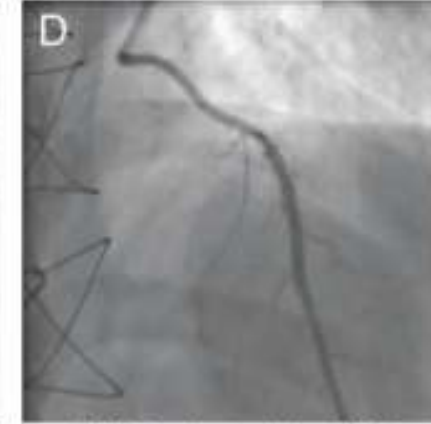


BVS implanted via LIMA

Long CTO of mid-RCA




Before procedure

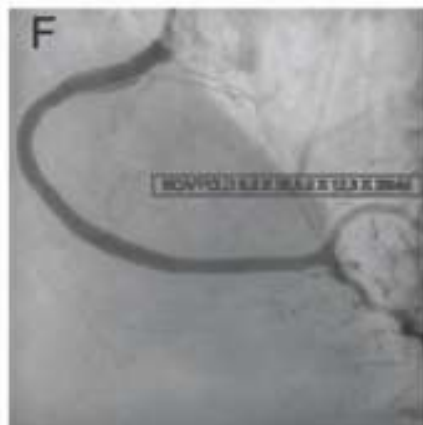


After BVS implantation

CTO of mid-LAD

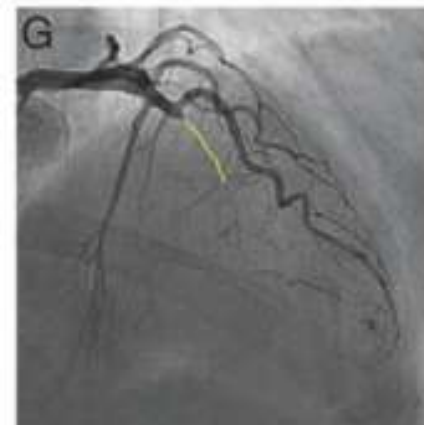

Before procedure

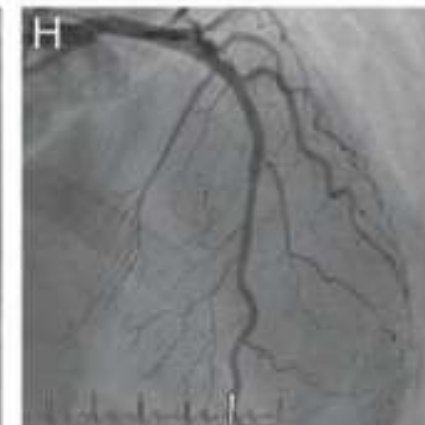


After BVS implantation




# ABSORB

LAD instent restenosis

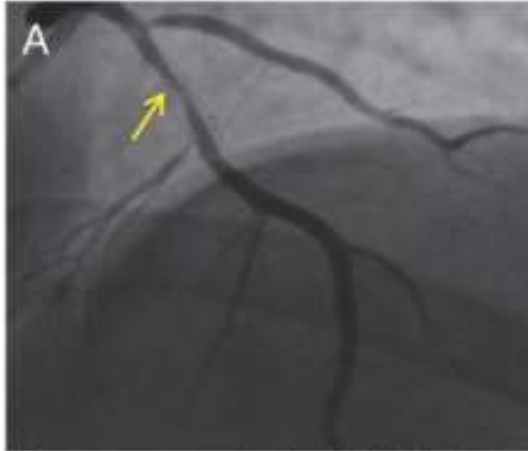

Instant restenosis in mid-LAD stent

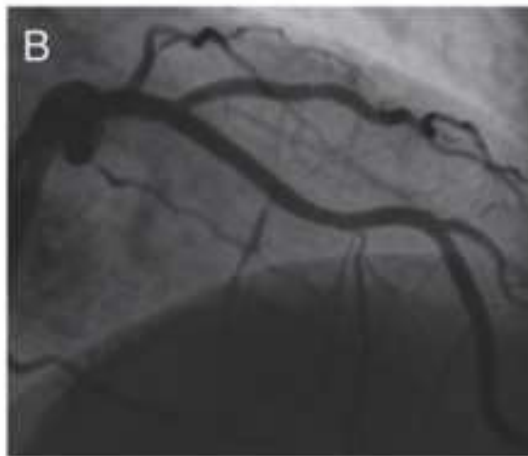


After BVS implantation

Non-ST elevation MI



Sub-total occlusion at presentation

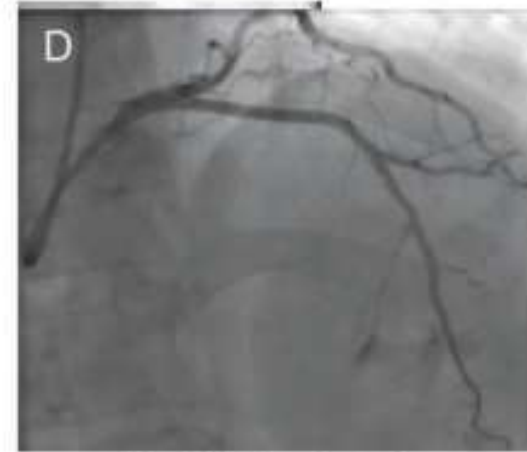

After BVS implantation

ST elevation MI



RCA occlusion at presentation




After BVS implantation

# IVUS - Good penetration


- Critical to guide BRS deployment
- Useful information on vessel morphology, the need for lesion preparation and site selection

# Poor resolution → Poor reproducibility

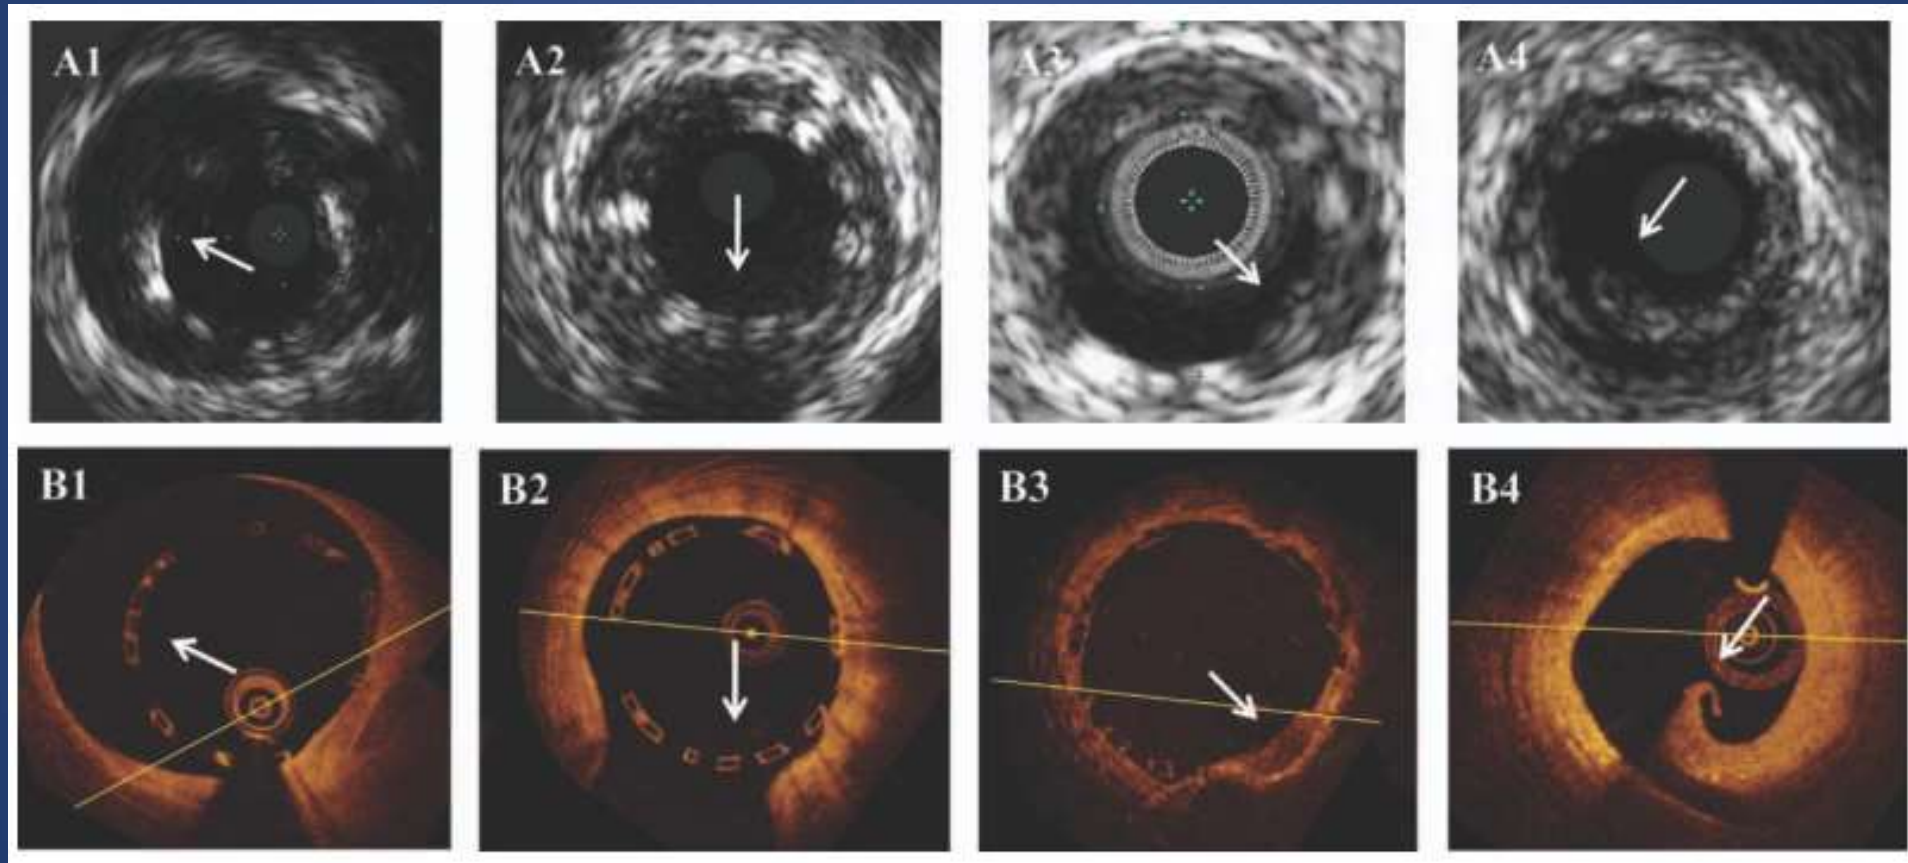

# OCT

## Morphologic changes in strut

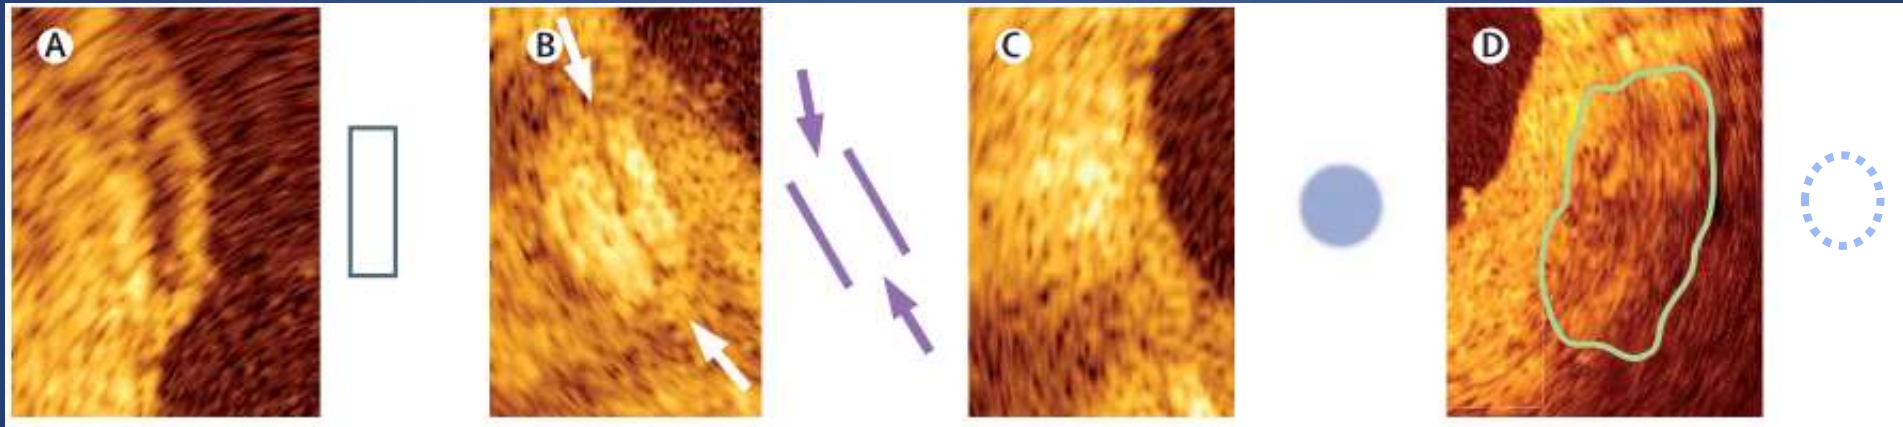


**Preserved  
Box**

**Open Box**

**Dissolved  
Bright Box**


**Dissolved  
Black Box**

# Resorption of malapposed

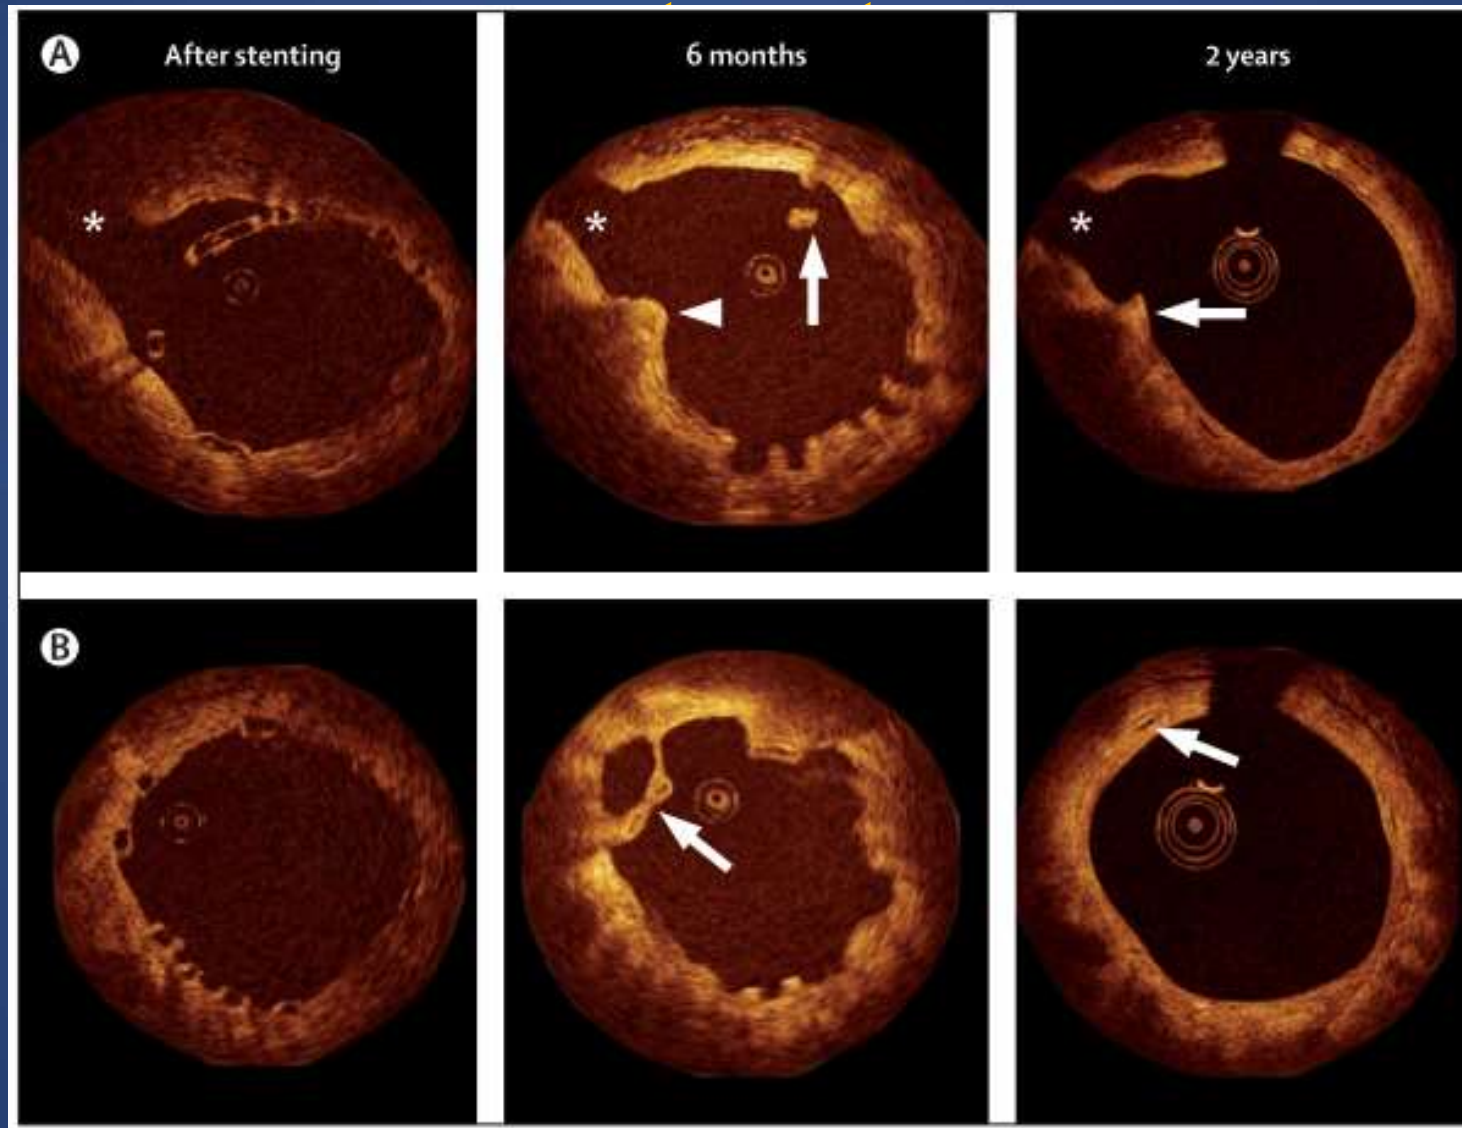



# BRS Resorption

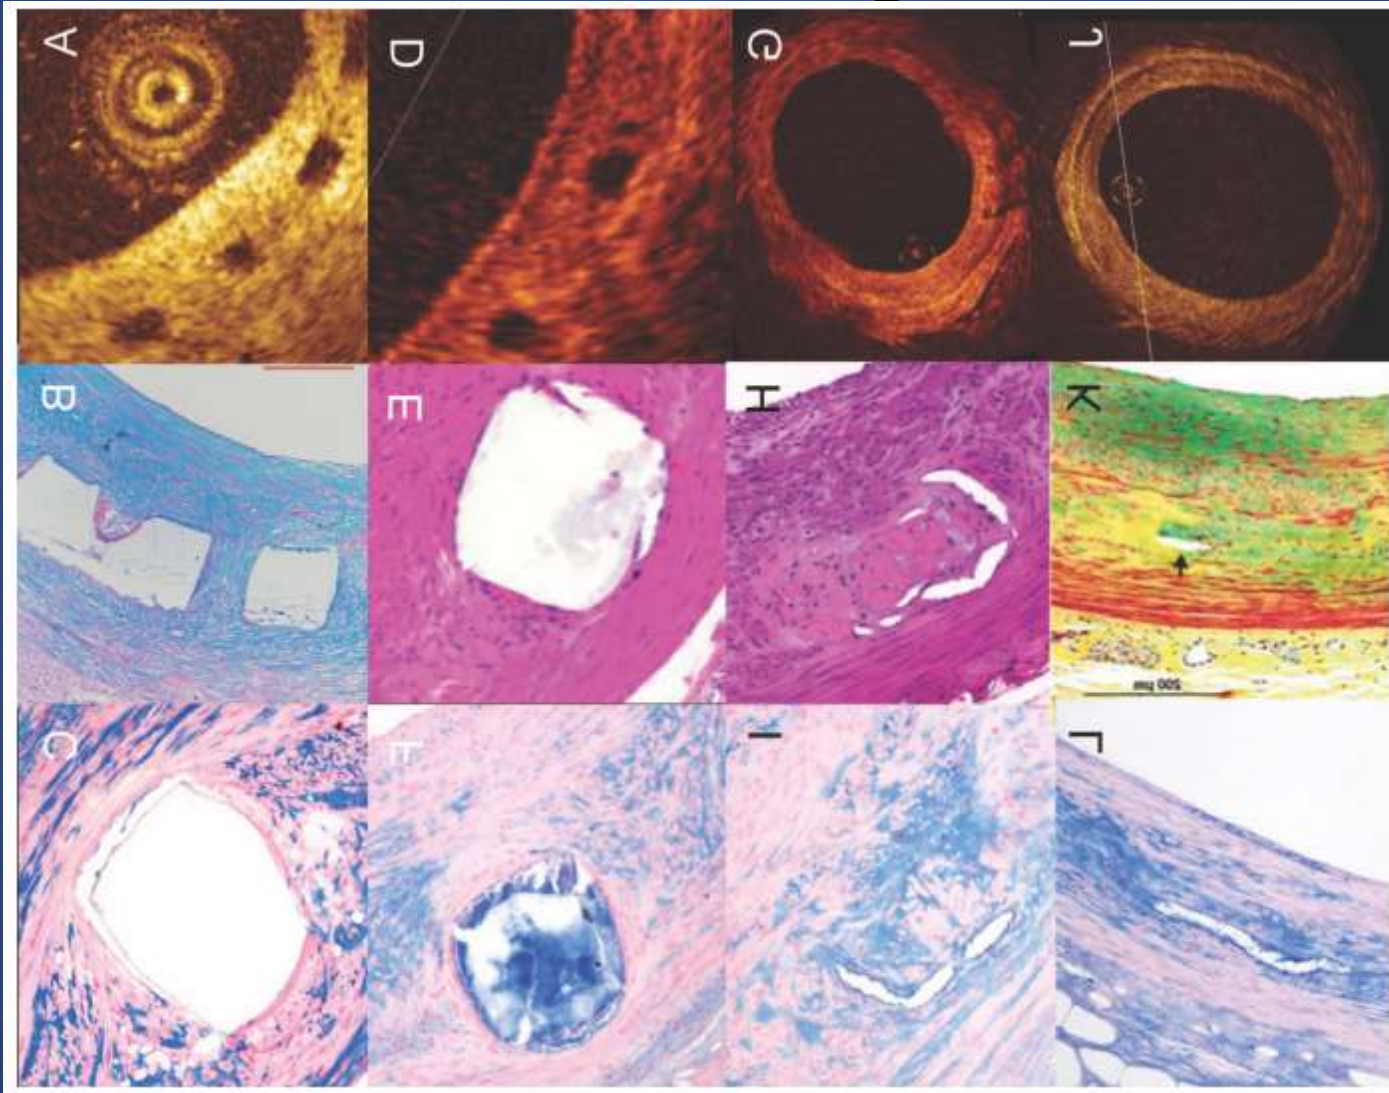





# Plaque Stabilization and Lumen Enlargement

6 month


60 month

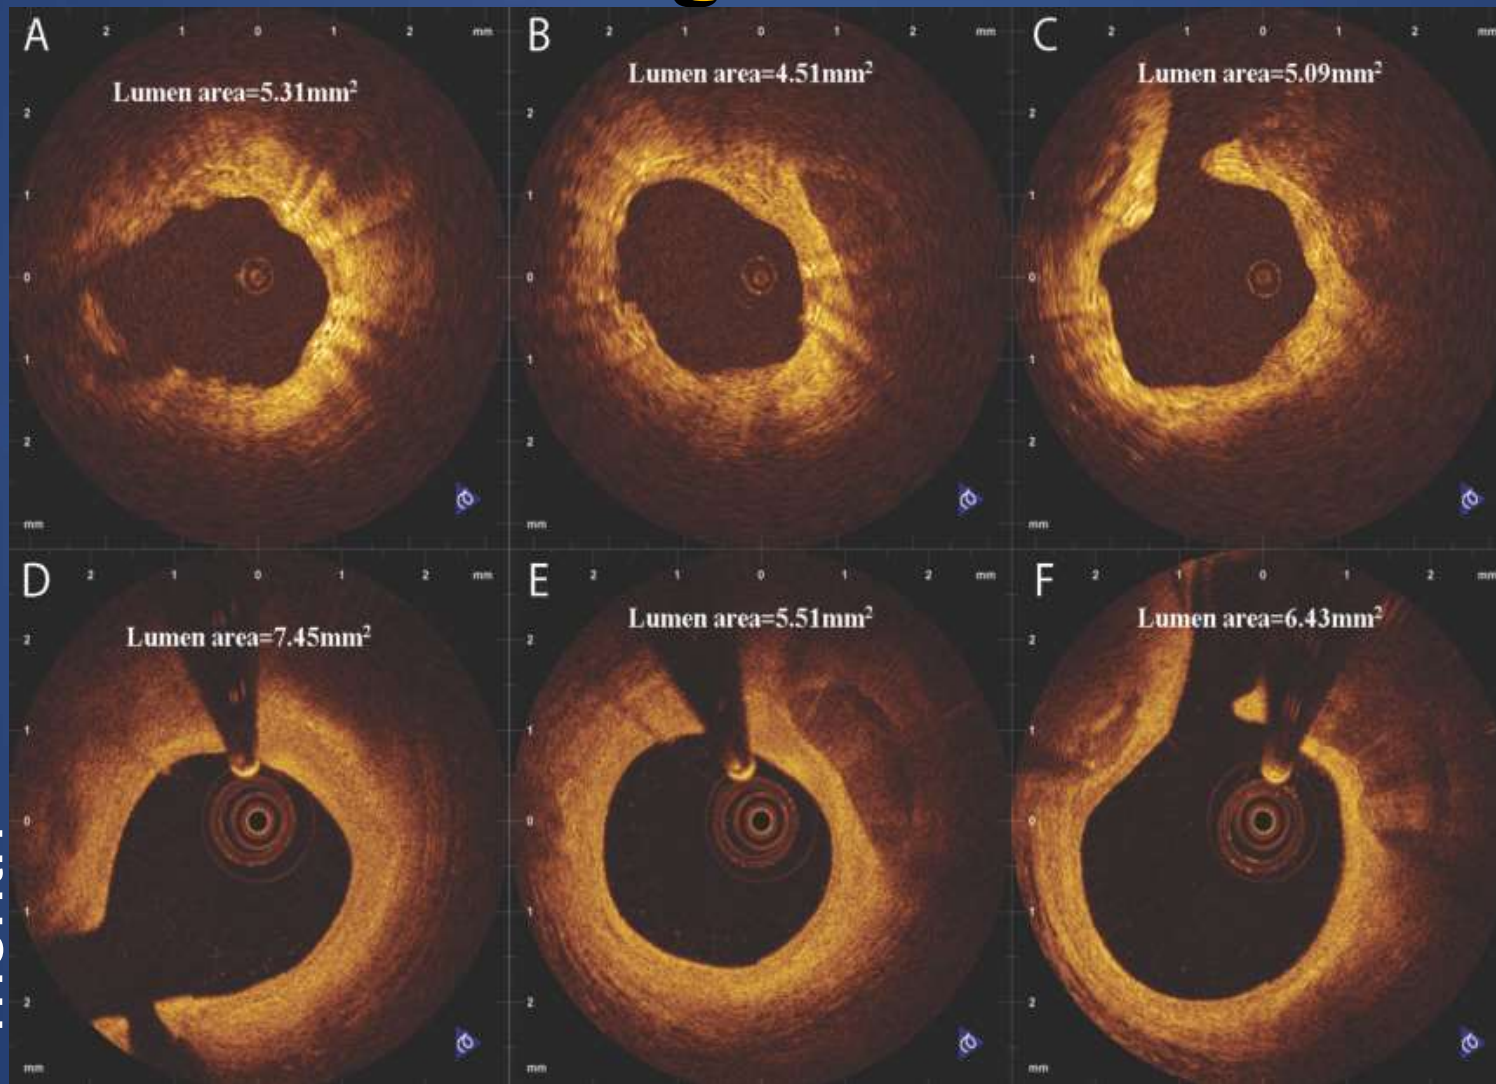

# OCT of acute scaffold disruption

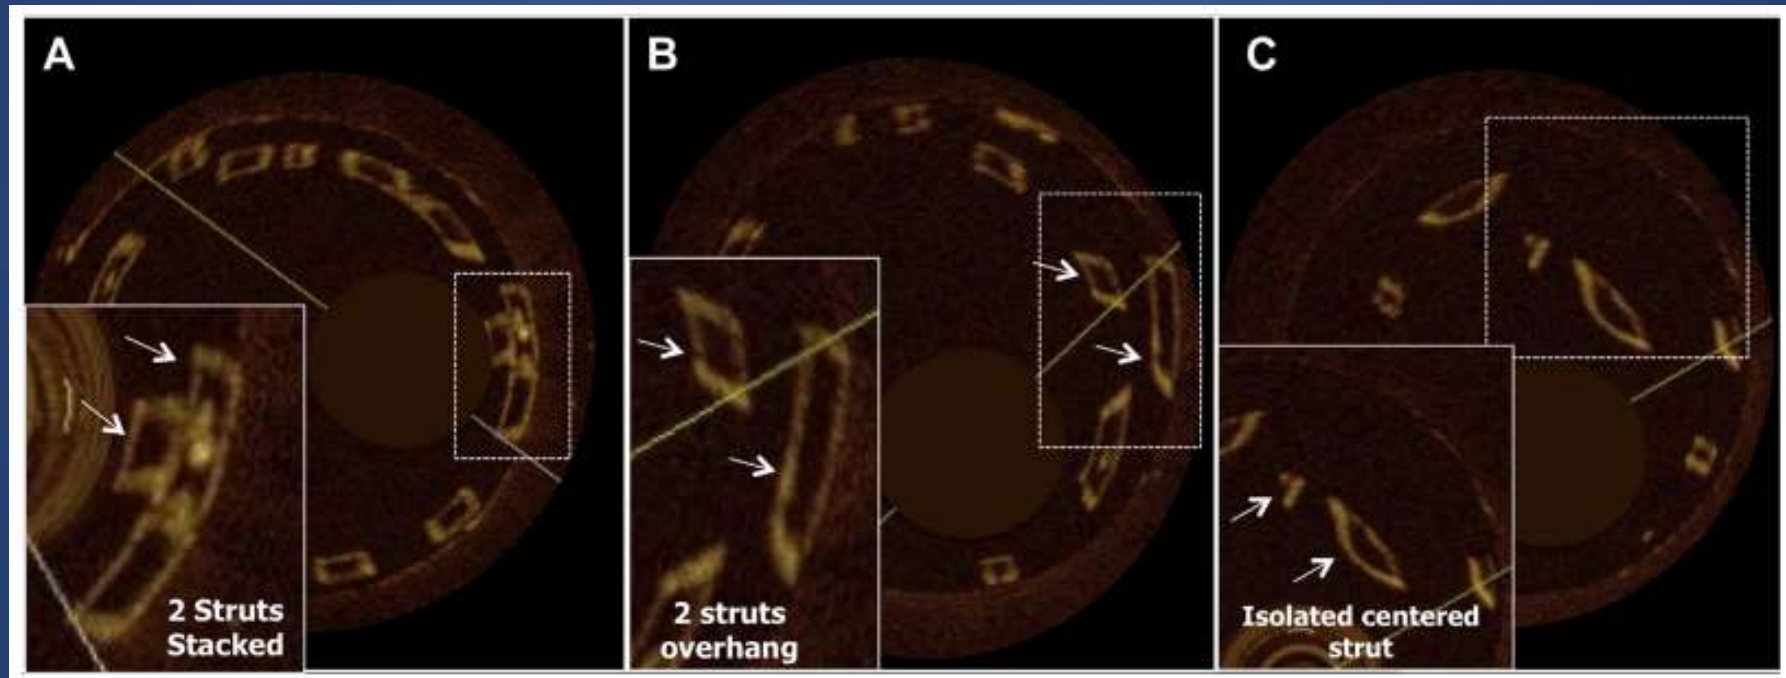


# Strut Fracture

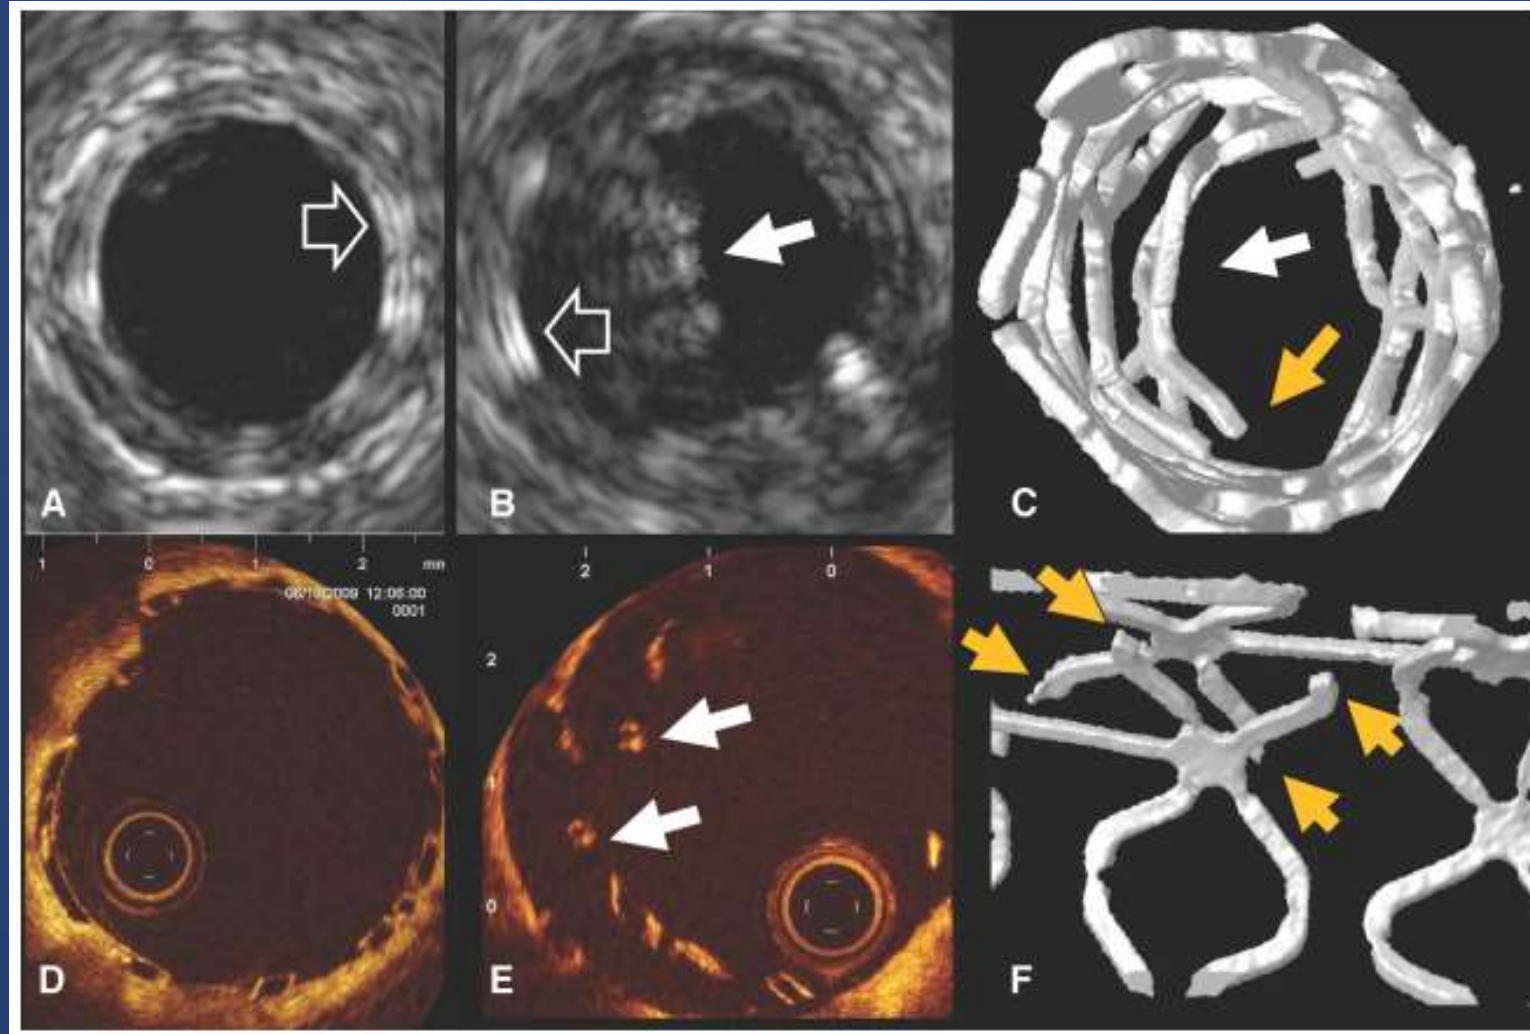




# Scaffold thrombosis

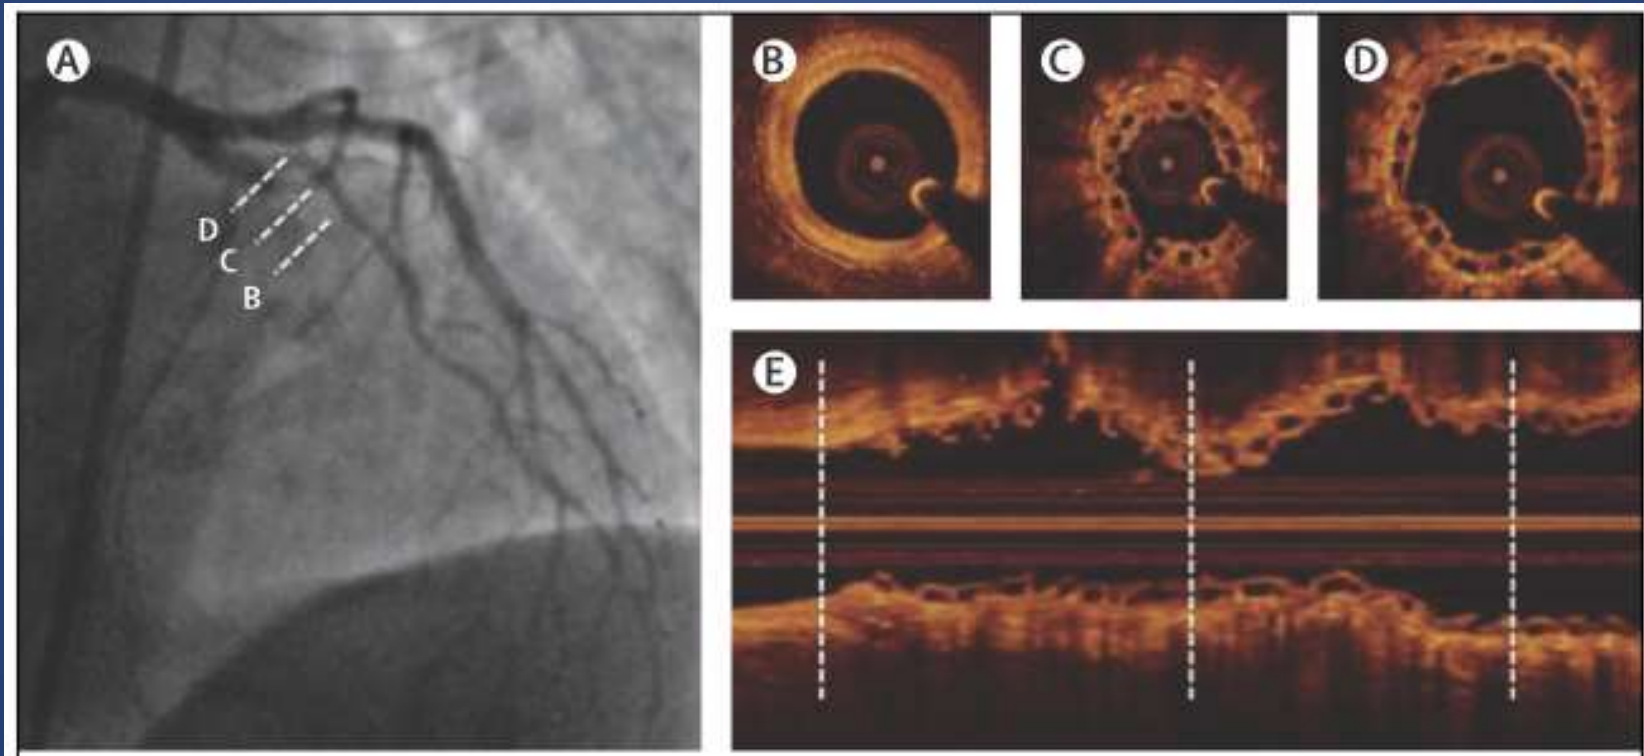

**Late Stent Thrombosis**

# Late Malapposition

- A 54 year-old man underwent PCI with Absorb 2.5 X 18mm

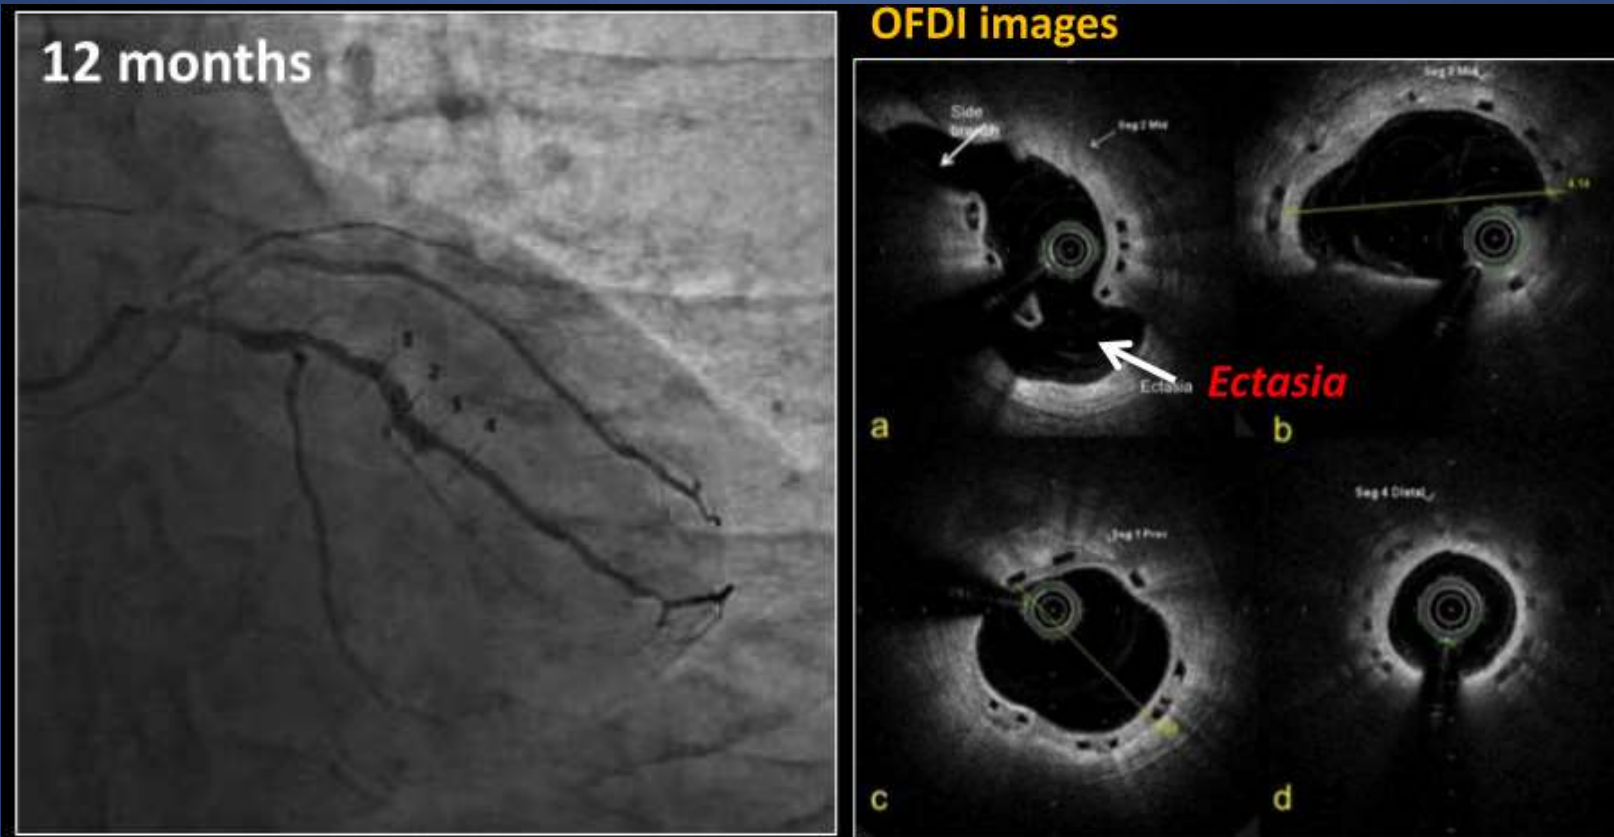

# Two modalities seem to be complementary


- While **IVUS** could be more helpful for the evaluation of the plaque morphology and in the preparation phase,
- **OCT** allows better qualitative scaffold analysis and follow-up evaluations.




# Coronary CT

Radiolucent, with radiopaque platinum markers



**No blooming artifact !**

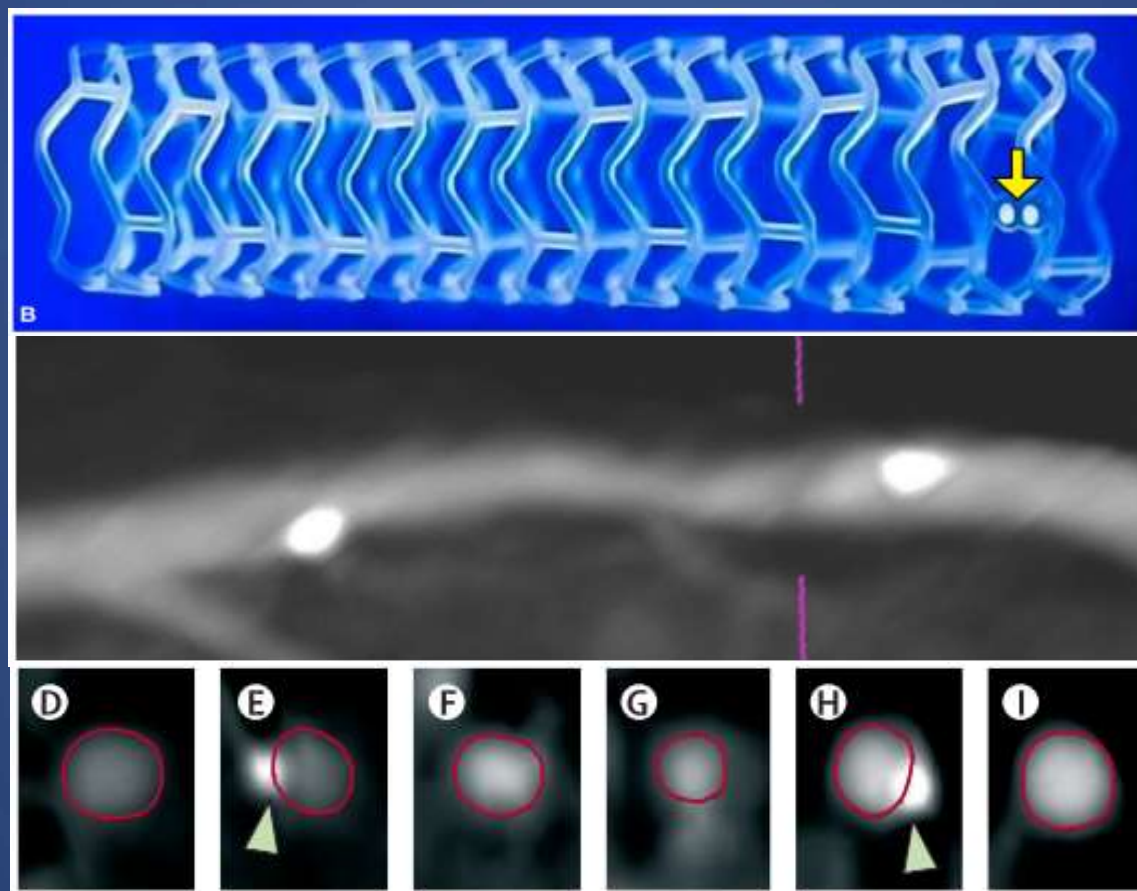

# Metal vs Bioresorbable scaffold by MSCT

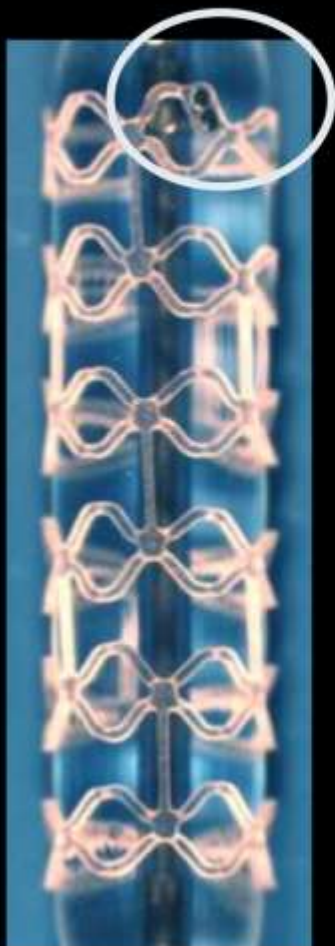

\*marker

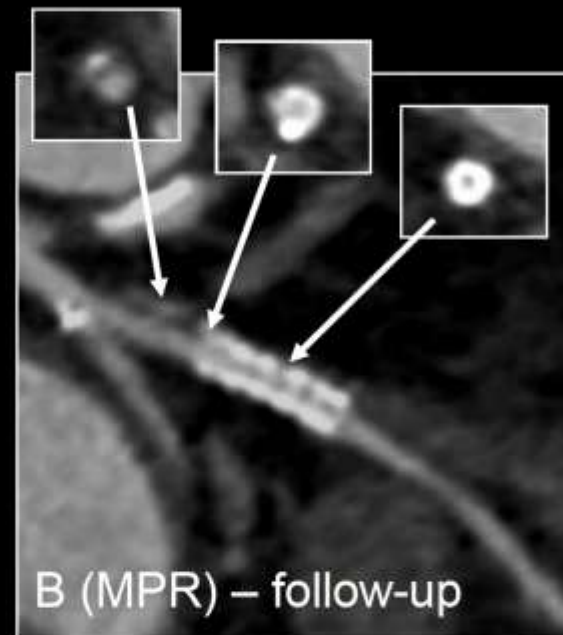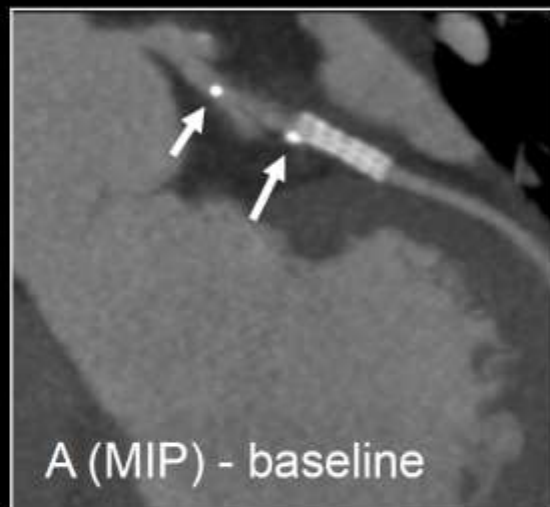

- Absorbable and metal stent implantation (bail-out)
- Highly attenuating distal metal stent well visible
- Only prox./dist. markers absorbable stent detectable
- In-stent plaque remains visible


# Cohort A

Serial imaging at 6m,24m and 60m

- MSCT – feasibility of functional assessment
- OCT –Plaque reduction and Vasomotion restoration



. Sealing and shielding of plaques as a result of scaffold implantation :  
can the scaffold cap the plaque? **60 Months Follow up**

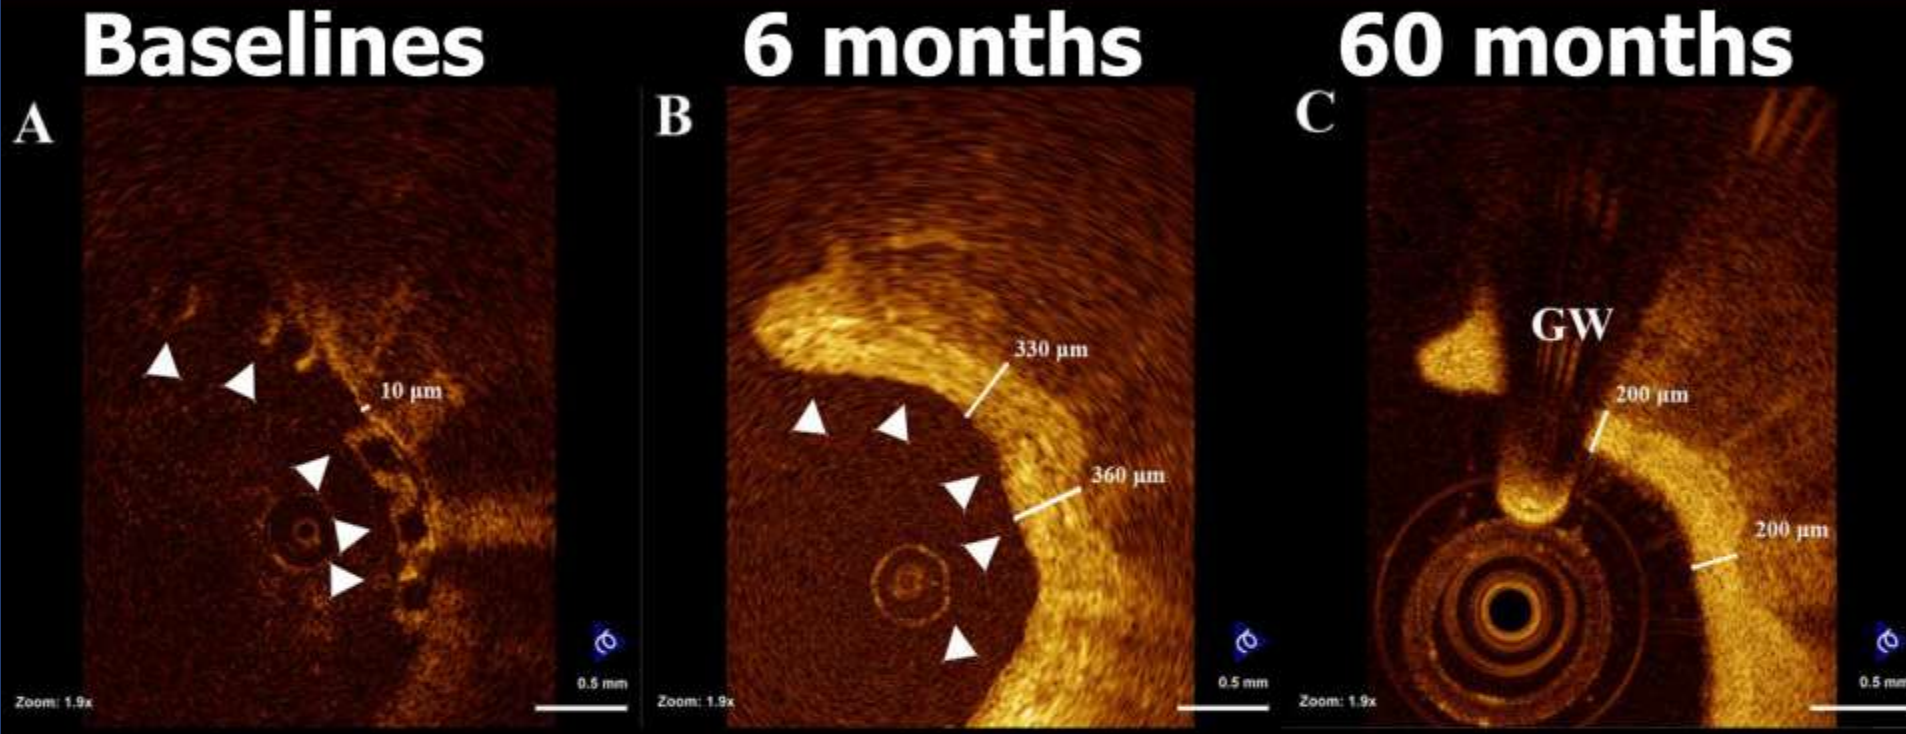

**ABSORB cohort A (n=30)**



## 5-Year Follow-up OCT of ABSORB A




# OCT optimization

	Not requiring OCT Optimization (n=21)	Requireing OCT optimization (n=8)	P-value
<b>Age</b>	50.8 ± 11.1	56.1 ± 17.8	0.34
<b>Female</b>	2 (9.5%)	1 (12.5%)	0.82
<b>Target vessel</b>			
<b>LAD</b>	9 (75%)	3 (25%)	0.80
<b>LCx</b>	6 (66%)	3 (33%)	0.66
<b>RCA</b>	5 (71%)	2 (29%)	0.95
<b>Lesion type, A</b>	10 (66%)	5 (33%)	0.49
<b>Lesion type, B or C</b>	11 (79%)	3 (21%)	0.49
<b>Mean n. POBA</b>	8.7 ± 3.3	16.5 ± 11.3	<0.01
<b>Length of procedure (min)</b>	83.7 ± 26.5	113.7 ± 39.0	<0.05




# ABSORB Cohort A

## IVUS and OCT

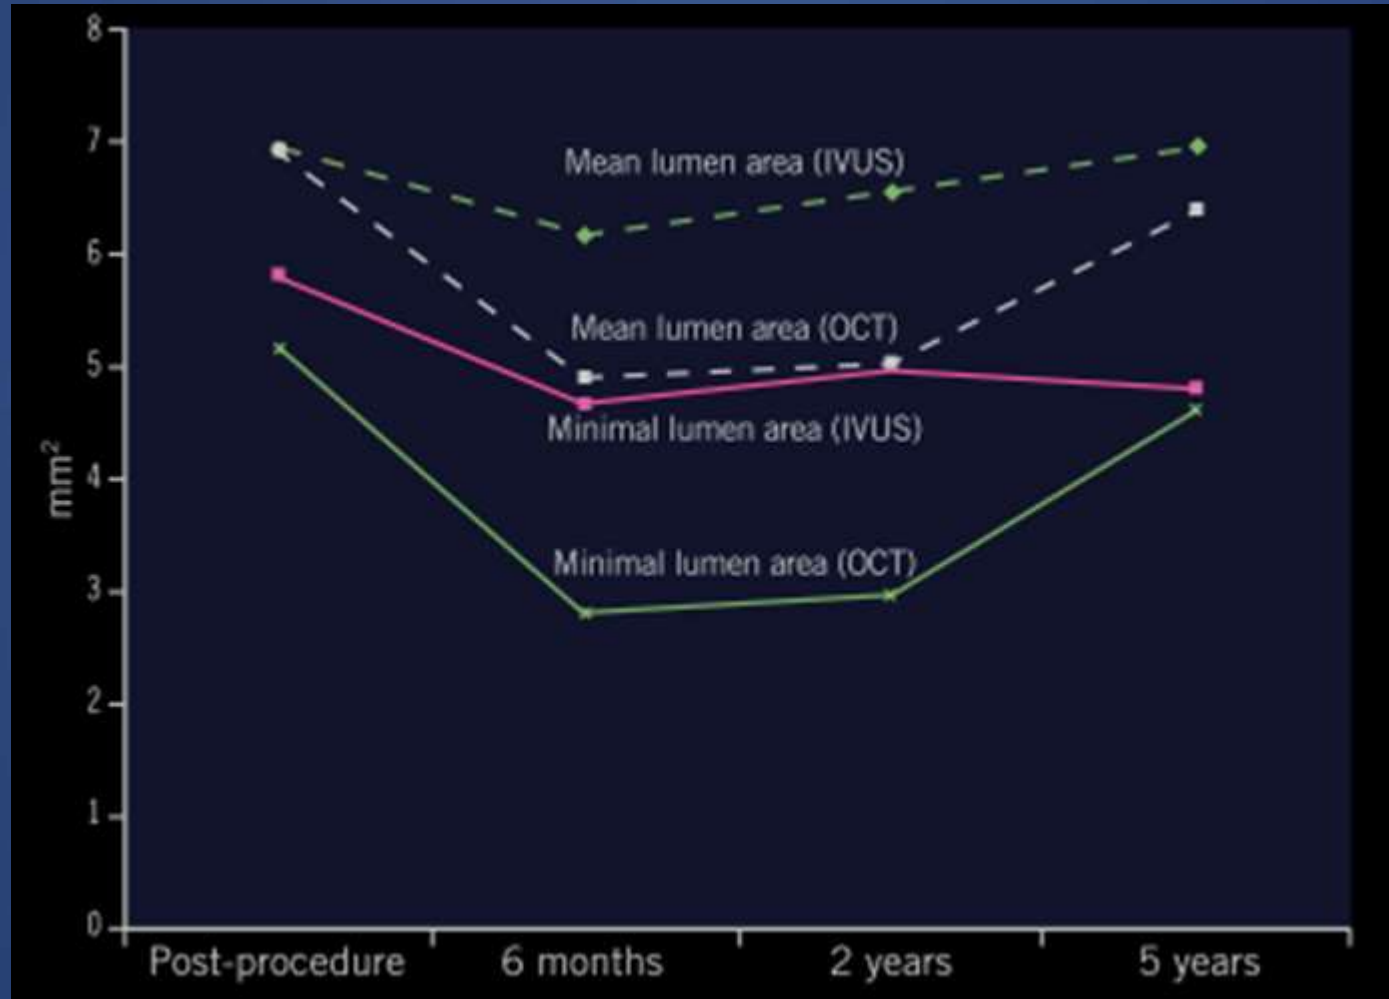


# ABSORB Cohort A

## Serial Luminal Measurement

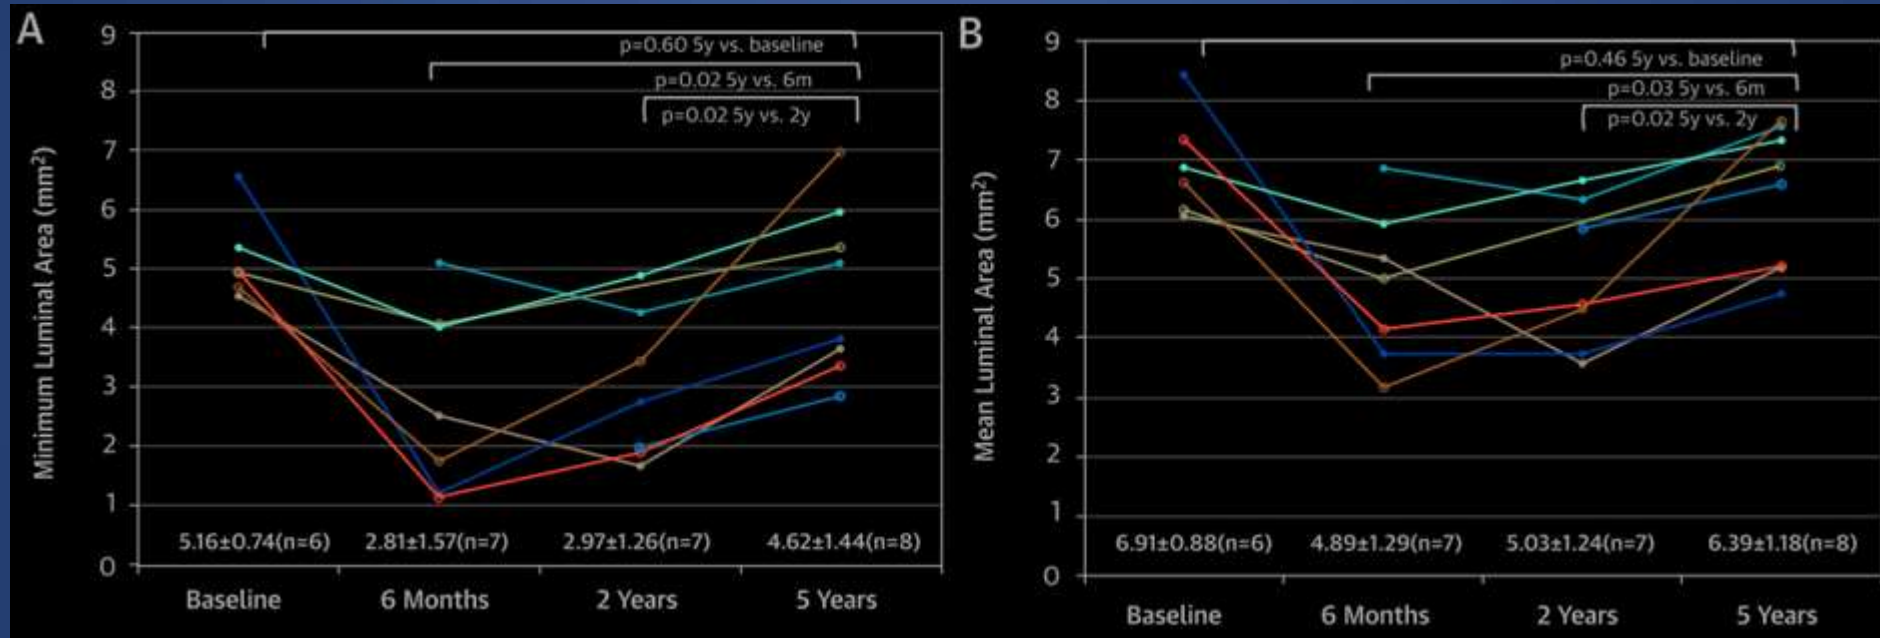


# Vasomotion Restoration

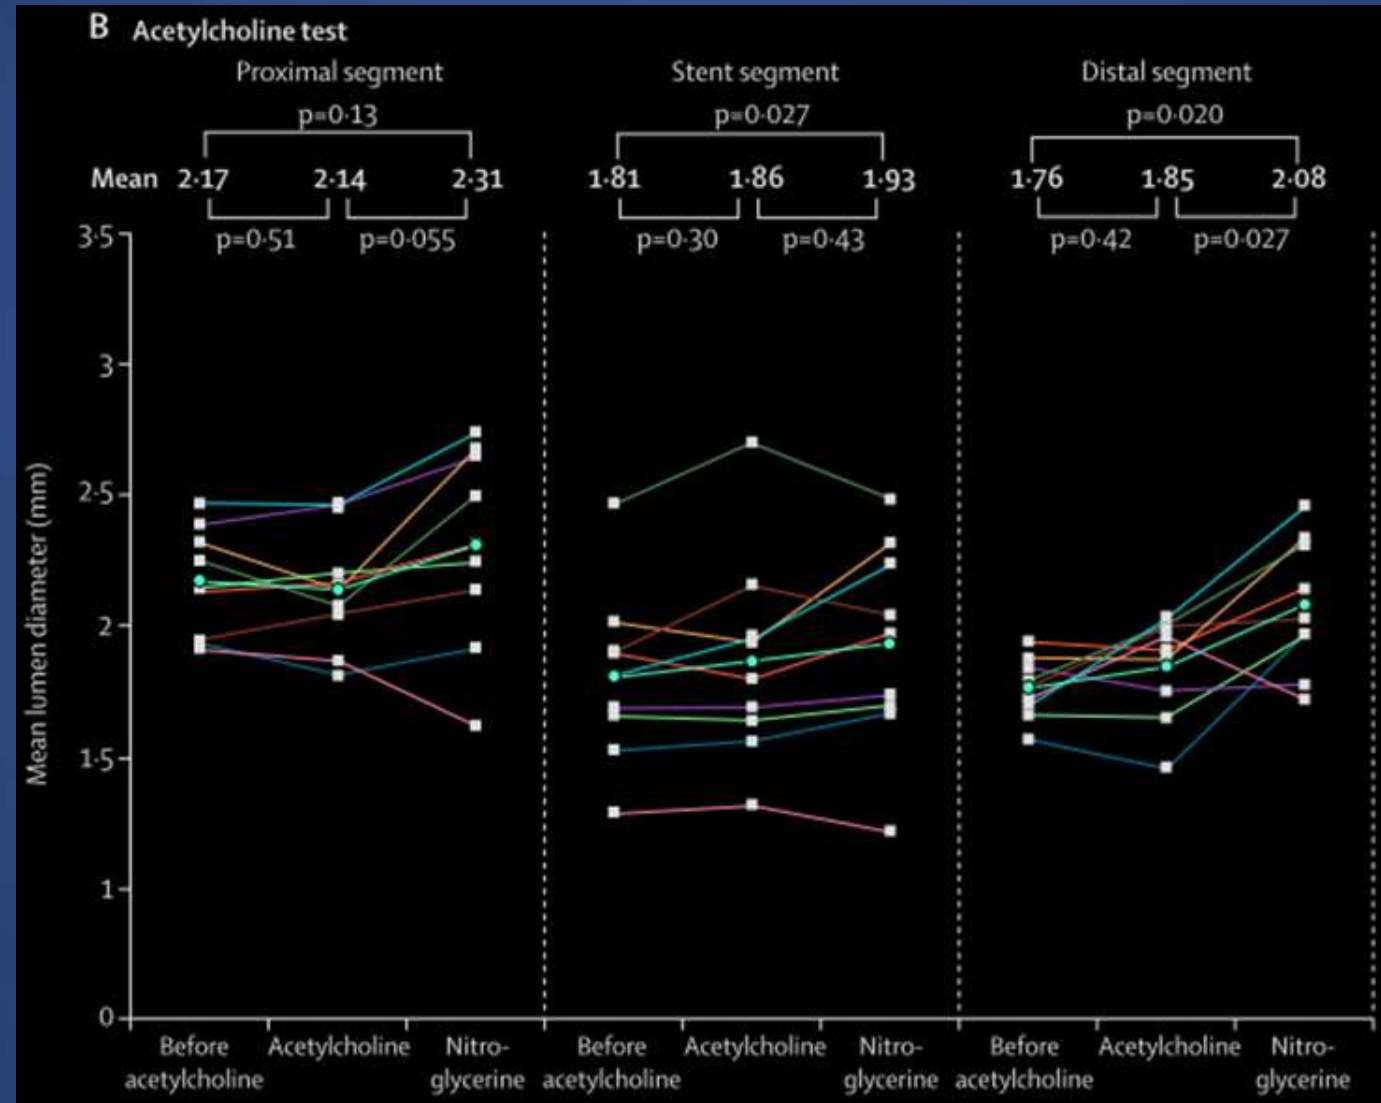


# ABSORB Cohort A

## MLA, Plaque area, Vessel area

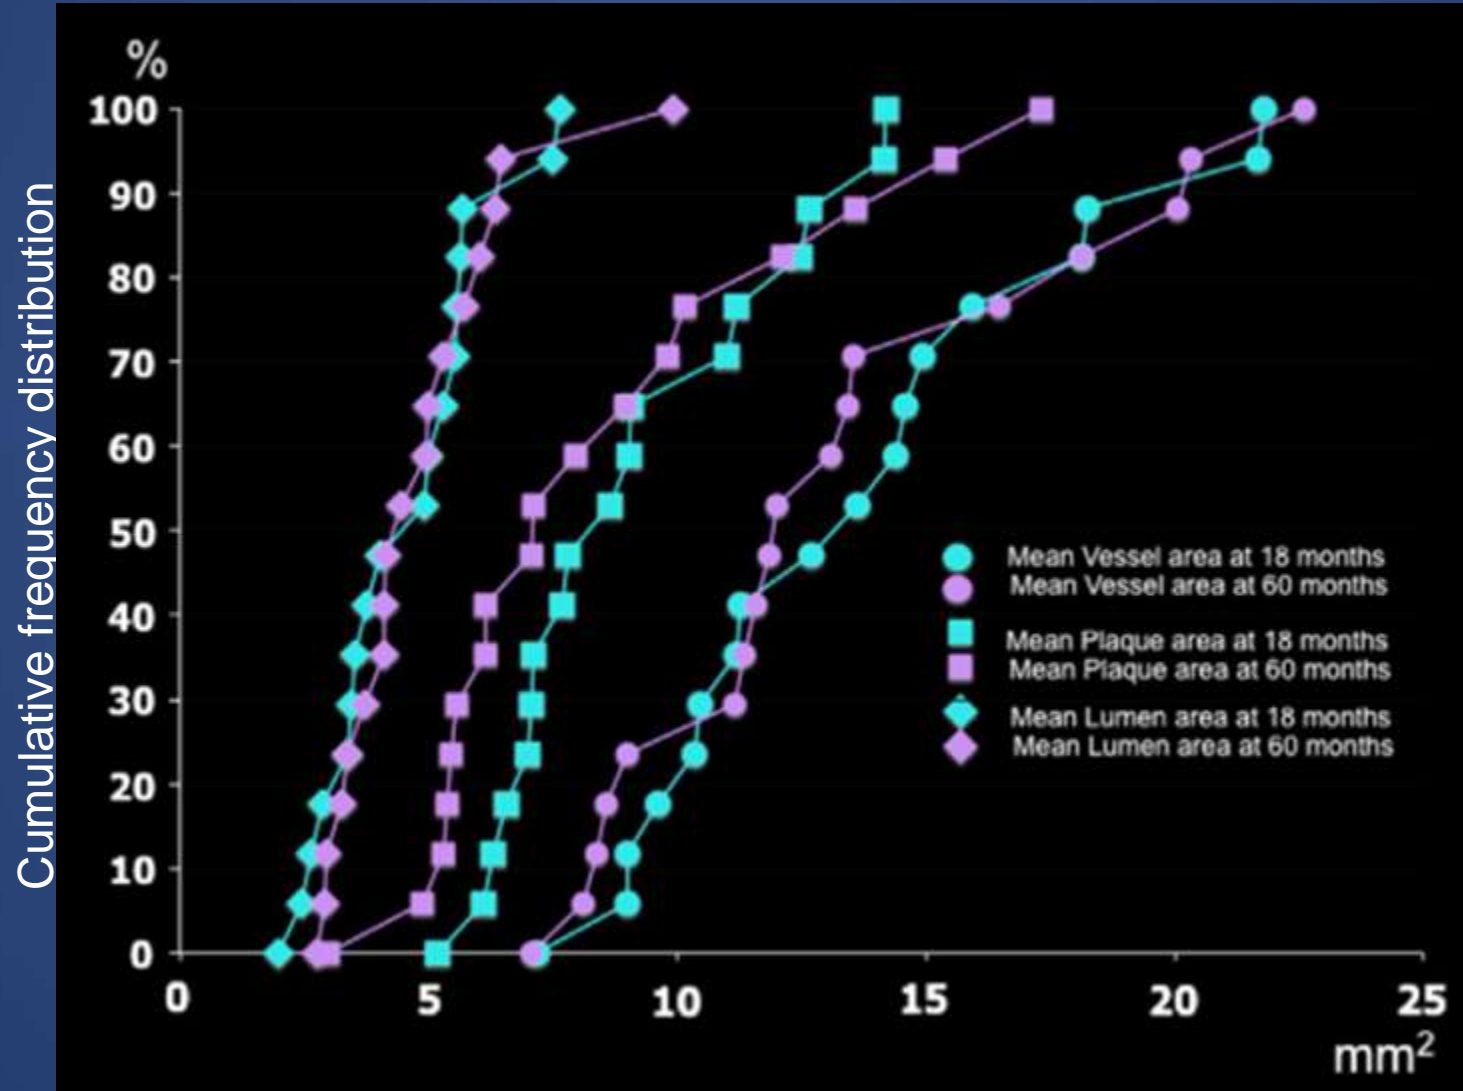

# ABSORB Cohort A

## MLA vs FFR<sub>CT</sub>

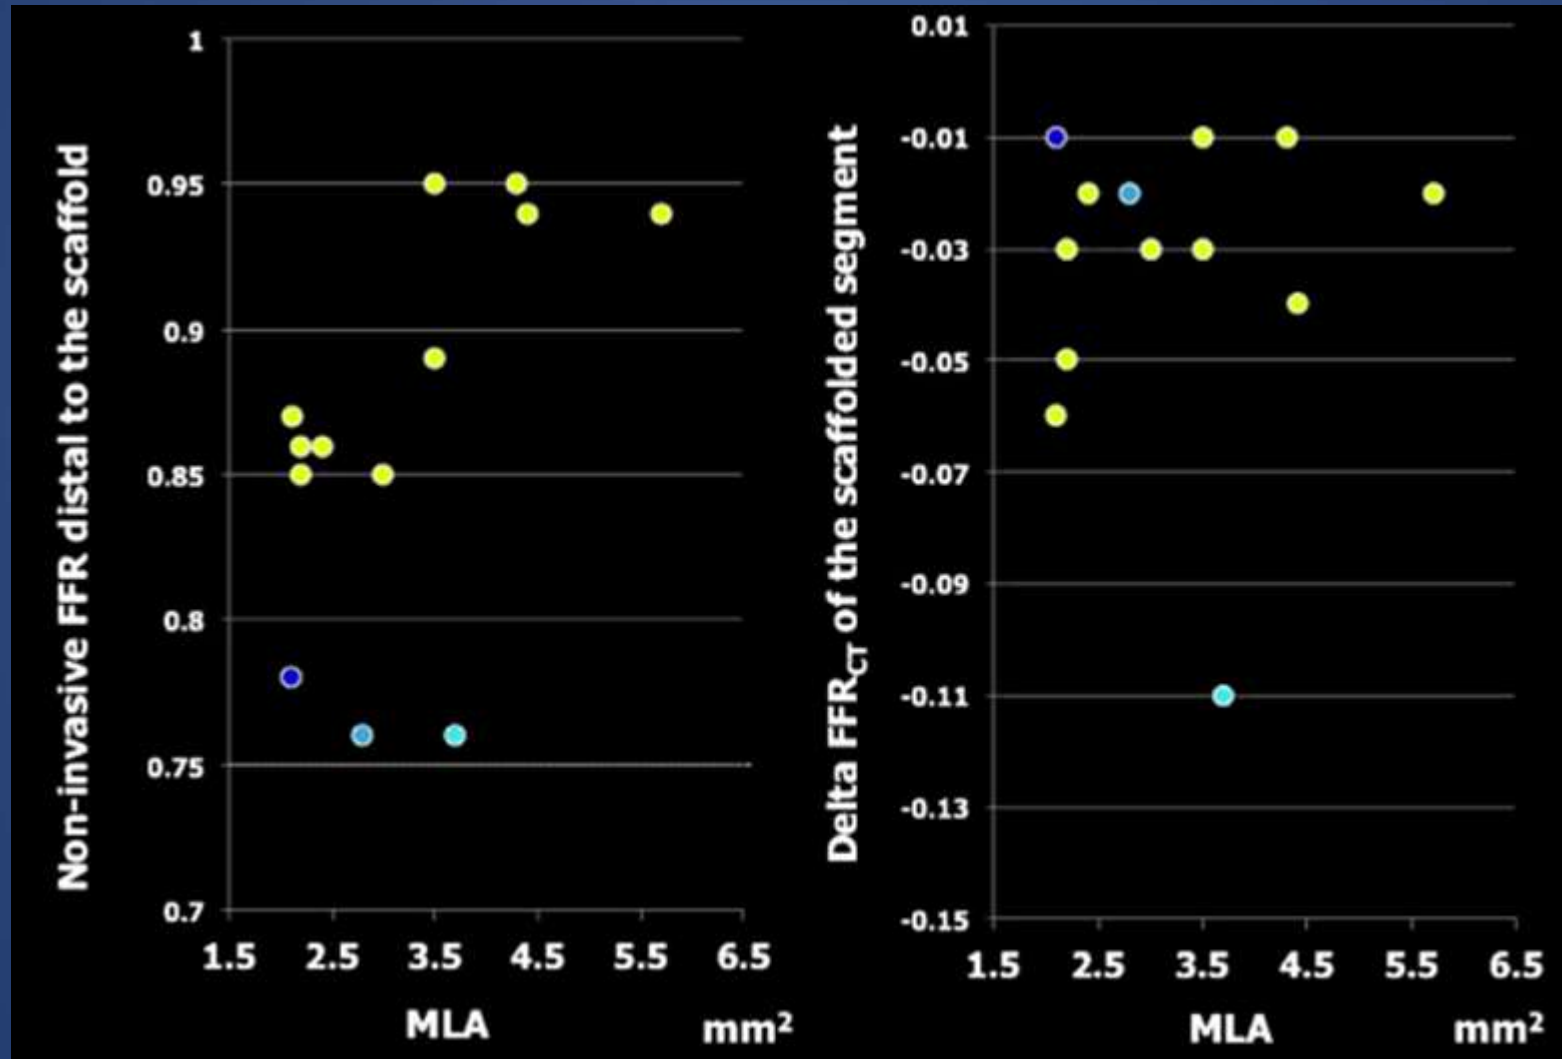

# Cohort B


## Imaging at 3 year

- Advanced bioresorption of BVS (VH / IVUS echogenicity)
- Acceptable angiographic late luminal loss between 1 and 3 yr (binary 6%)
- Increased MLA (IVUS and OCT)
- Biphasic change of total plaque area
  - ↑ between 1 and 2 yr but ↓ between 2 and 3 yr




# True-serial changes in percentage hyper-echogenic area

(%) \*P<0.05 vs post-procedure, † P<0.05 vs. 6M(B1)/12M(B2)



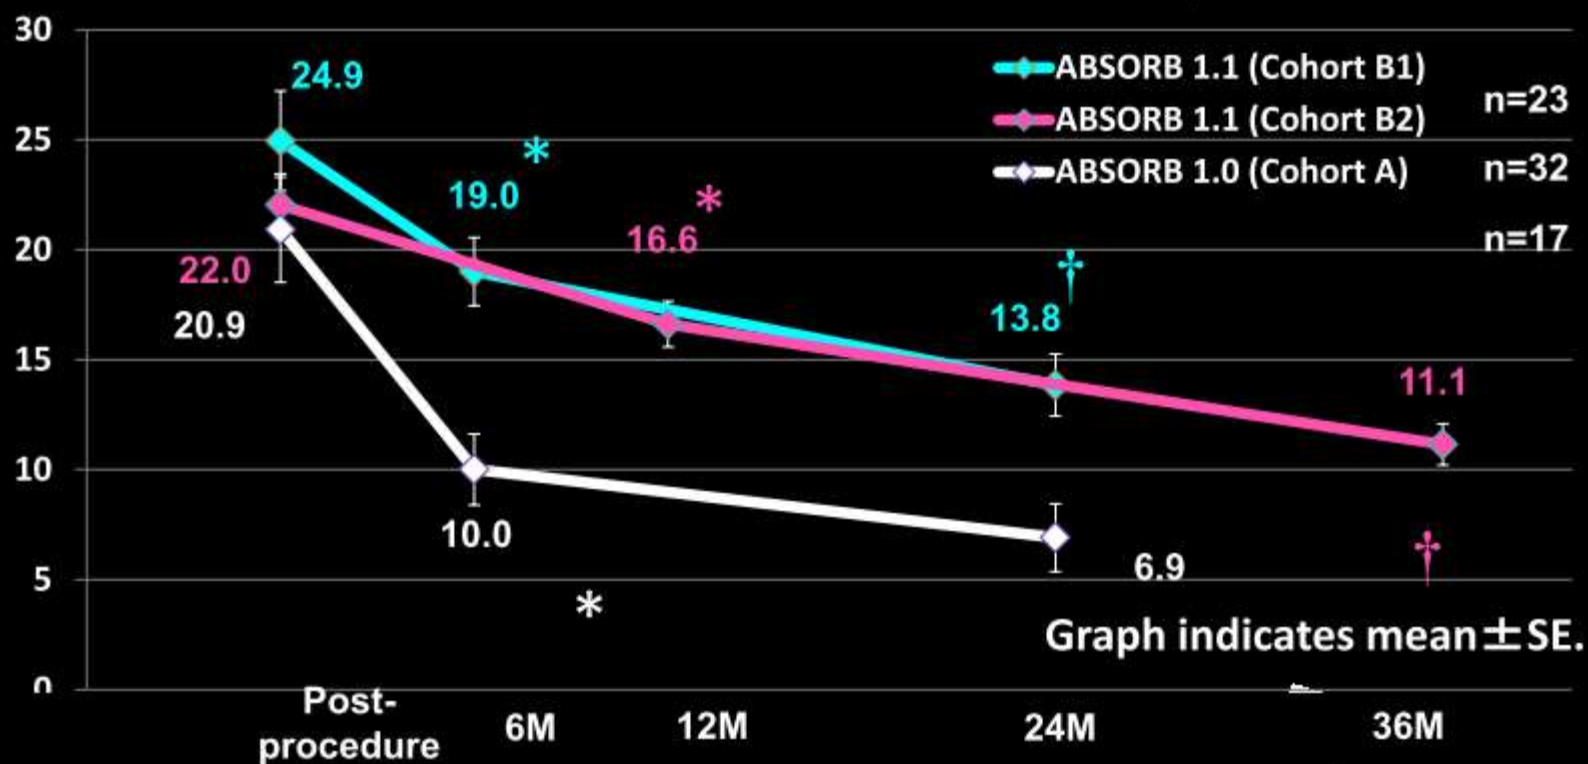


The actual duration of resorption of the second generation is in vivo approximately **18 months longer** than the first generation, and the mass loss of 2<sup>nd</sup> generation ABSORB scaffold takes approximately 36 months

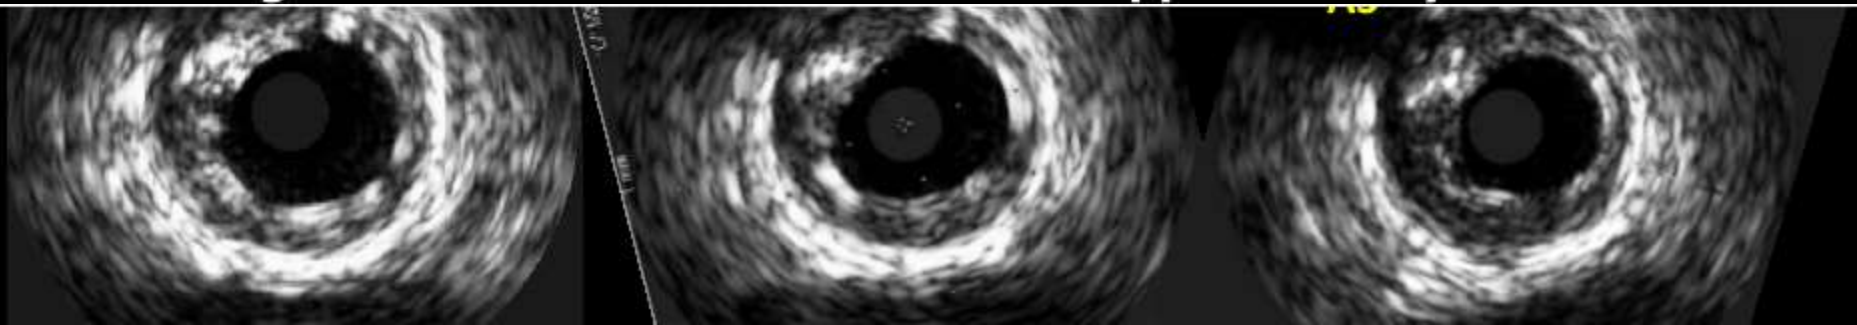

A



## Serial QCA without TLR cases

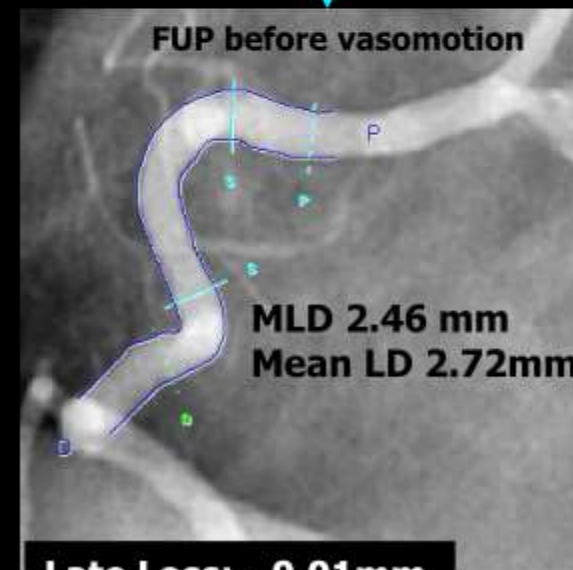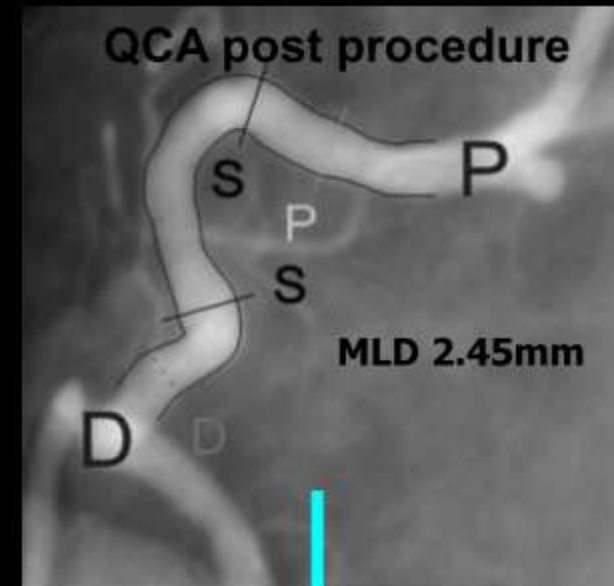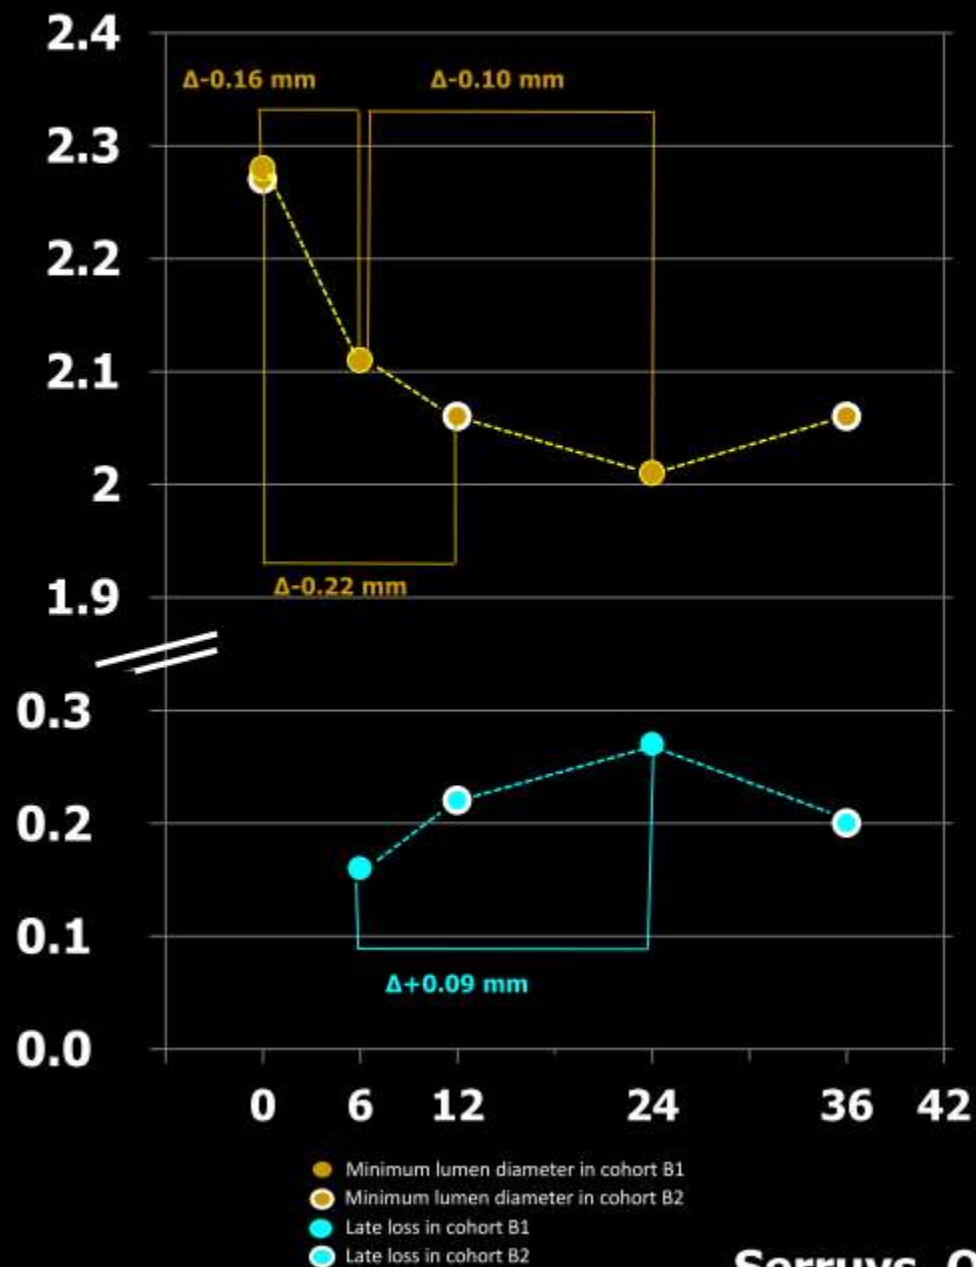

Late Loss: -0.01mm

Serruys, Onuma et al. Eurointervention 2014


# Serial IVUS

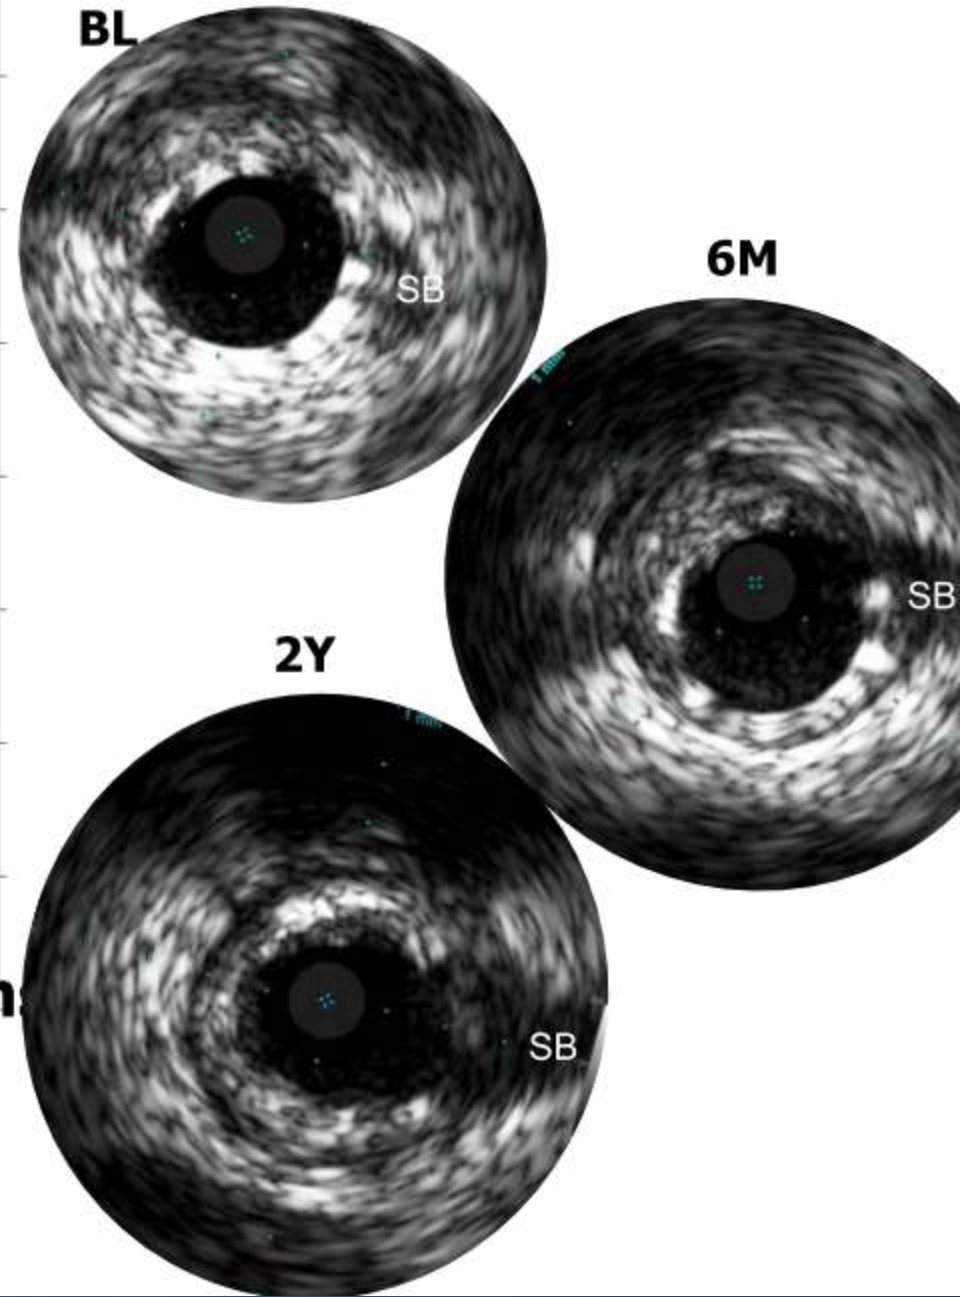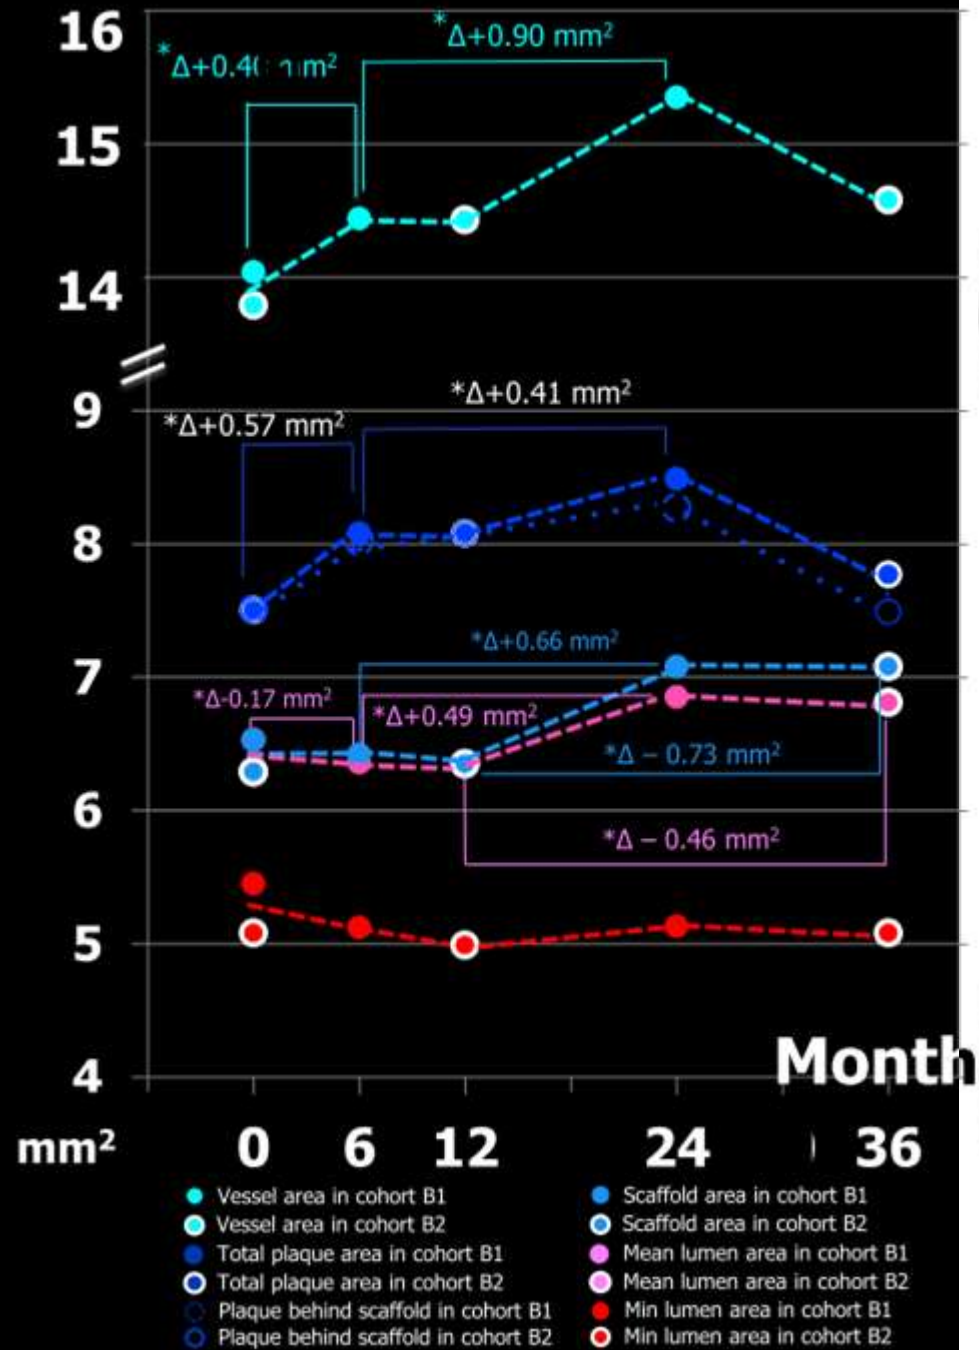



# ABSORB Cohort B

## IVUS

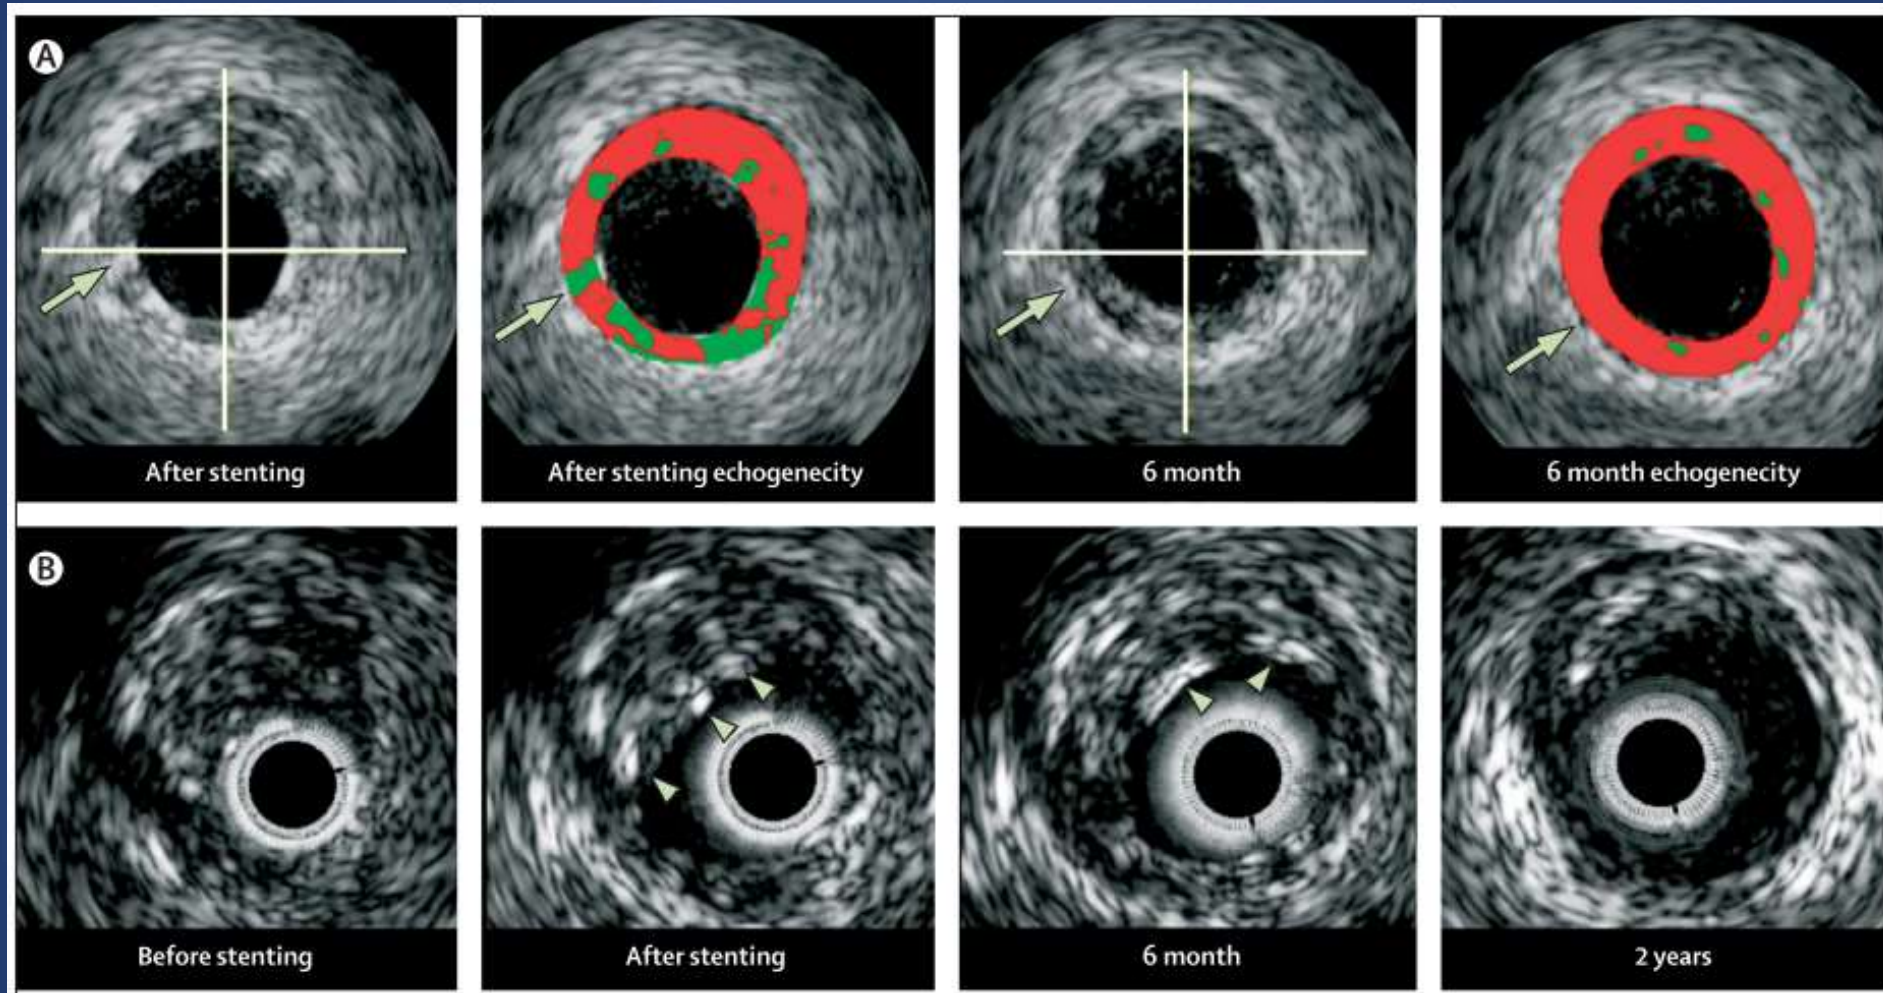


*Serruys PW et al. Lancet 2009;373:897*

*Serruys PW et al. EuroInt 2014 e-pub*

# ABSORB Cohort B

## VH-IVUS



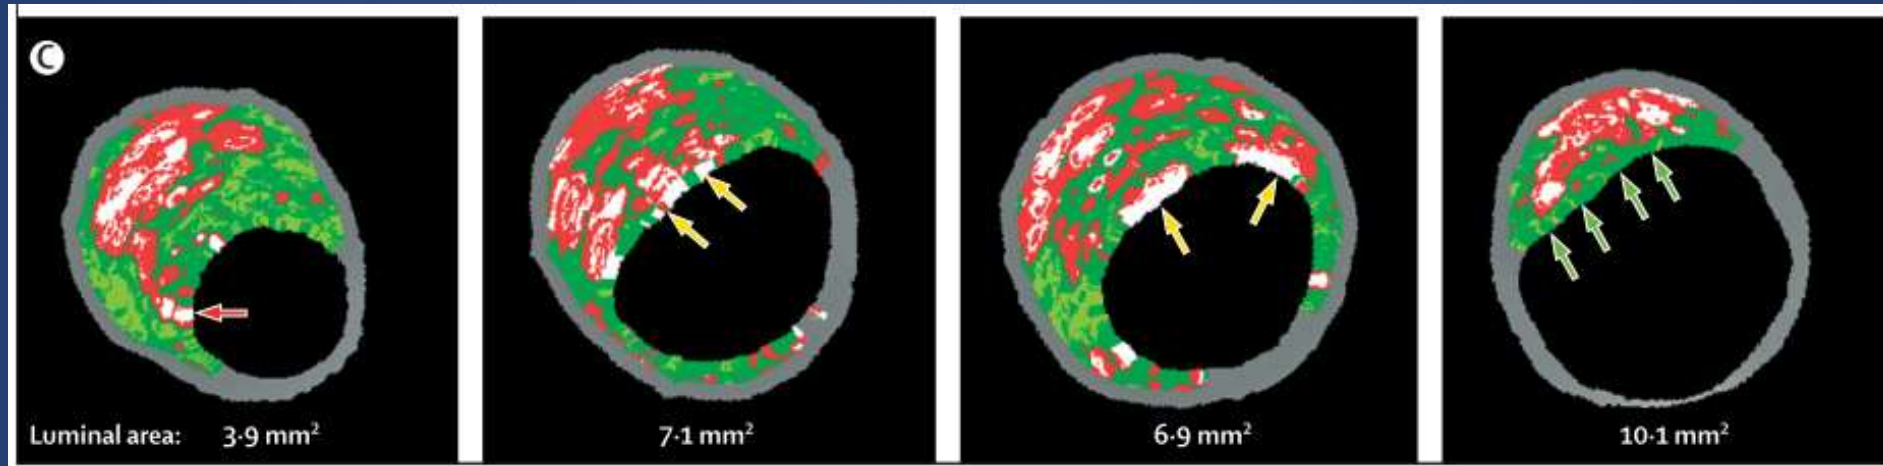


	Baseline (n=36)	1yr (n=36)	3yr (n=36)	p
<b>Dense calcium (%)</b>	30.74±10.11	24.95±8.28	21.84±8.41	<0.001
<b>Necrotic Core (%)</b>	32.10±6.62	30.01±6.29	26.11±5.99	<0.001
<b>Fibrofatty (%)</b>	2.94±2.43	4.23±2.29	6.87±3.66	<0.001
<b>Fibrous (%)</b>	34.22±10.05	40.80±9.60	45.18±9.38	<0.001

*Serruys PW et al. Lancet 2009;373:897*

*Serruys PW et al. EuroInt 2014 e-pub*

# Serial OCT

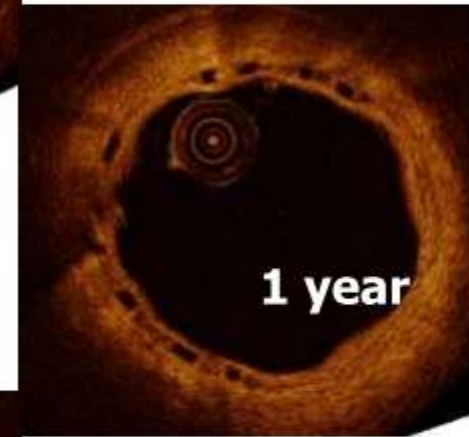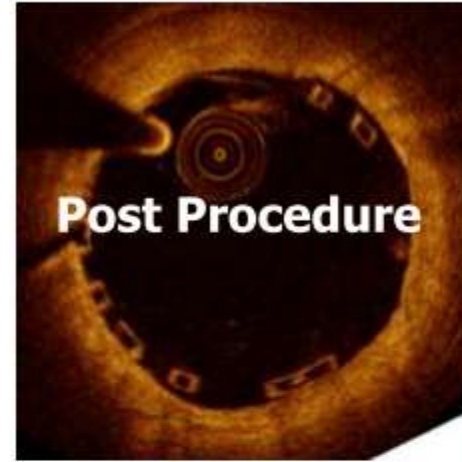
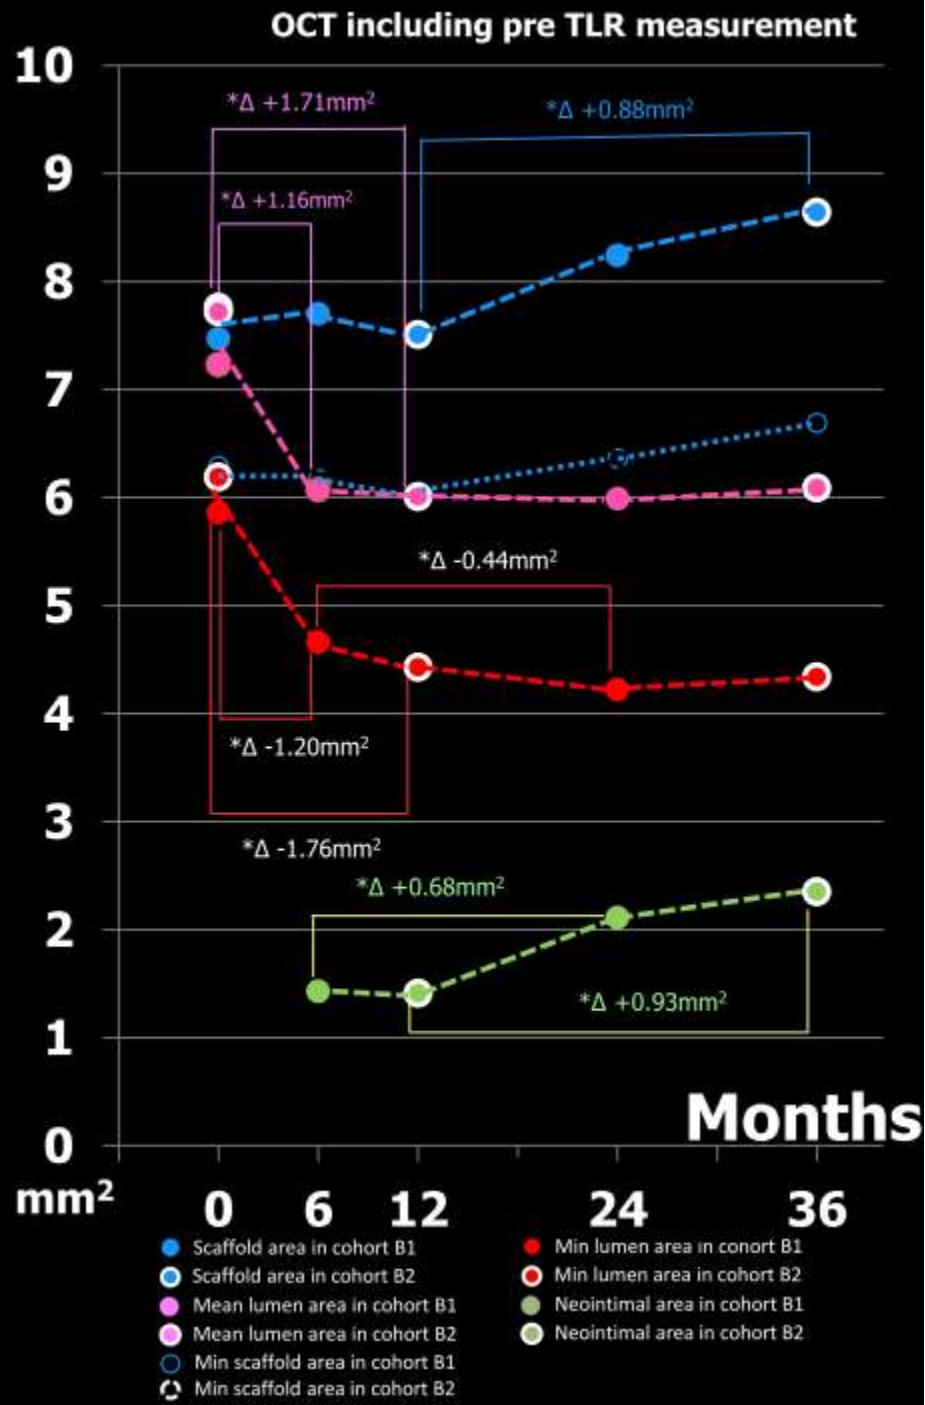




# Serial OCT

- The **mean and minimum scaffold area's** significantly increase between 1 and 3 years and compensate for the increase **in neointimal hyperplasia**
- As a consequence, **mean lumen area** and **minimal lumen area** remained unchanged between 1 year to 3 years.





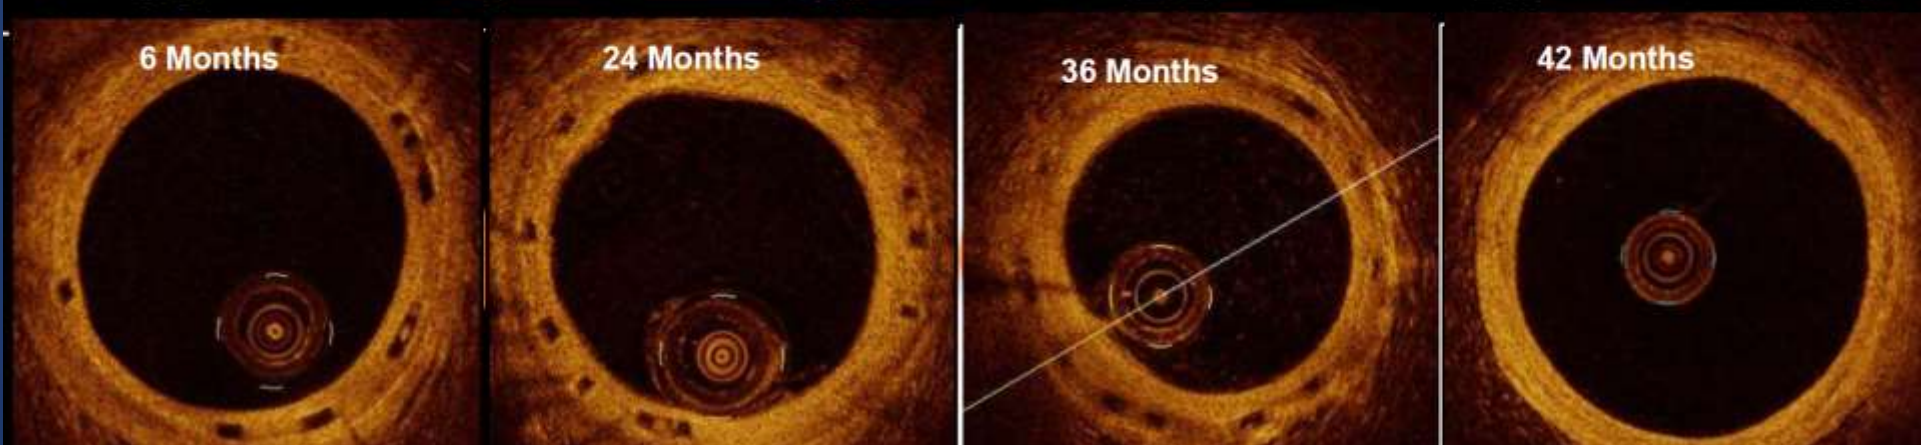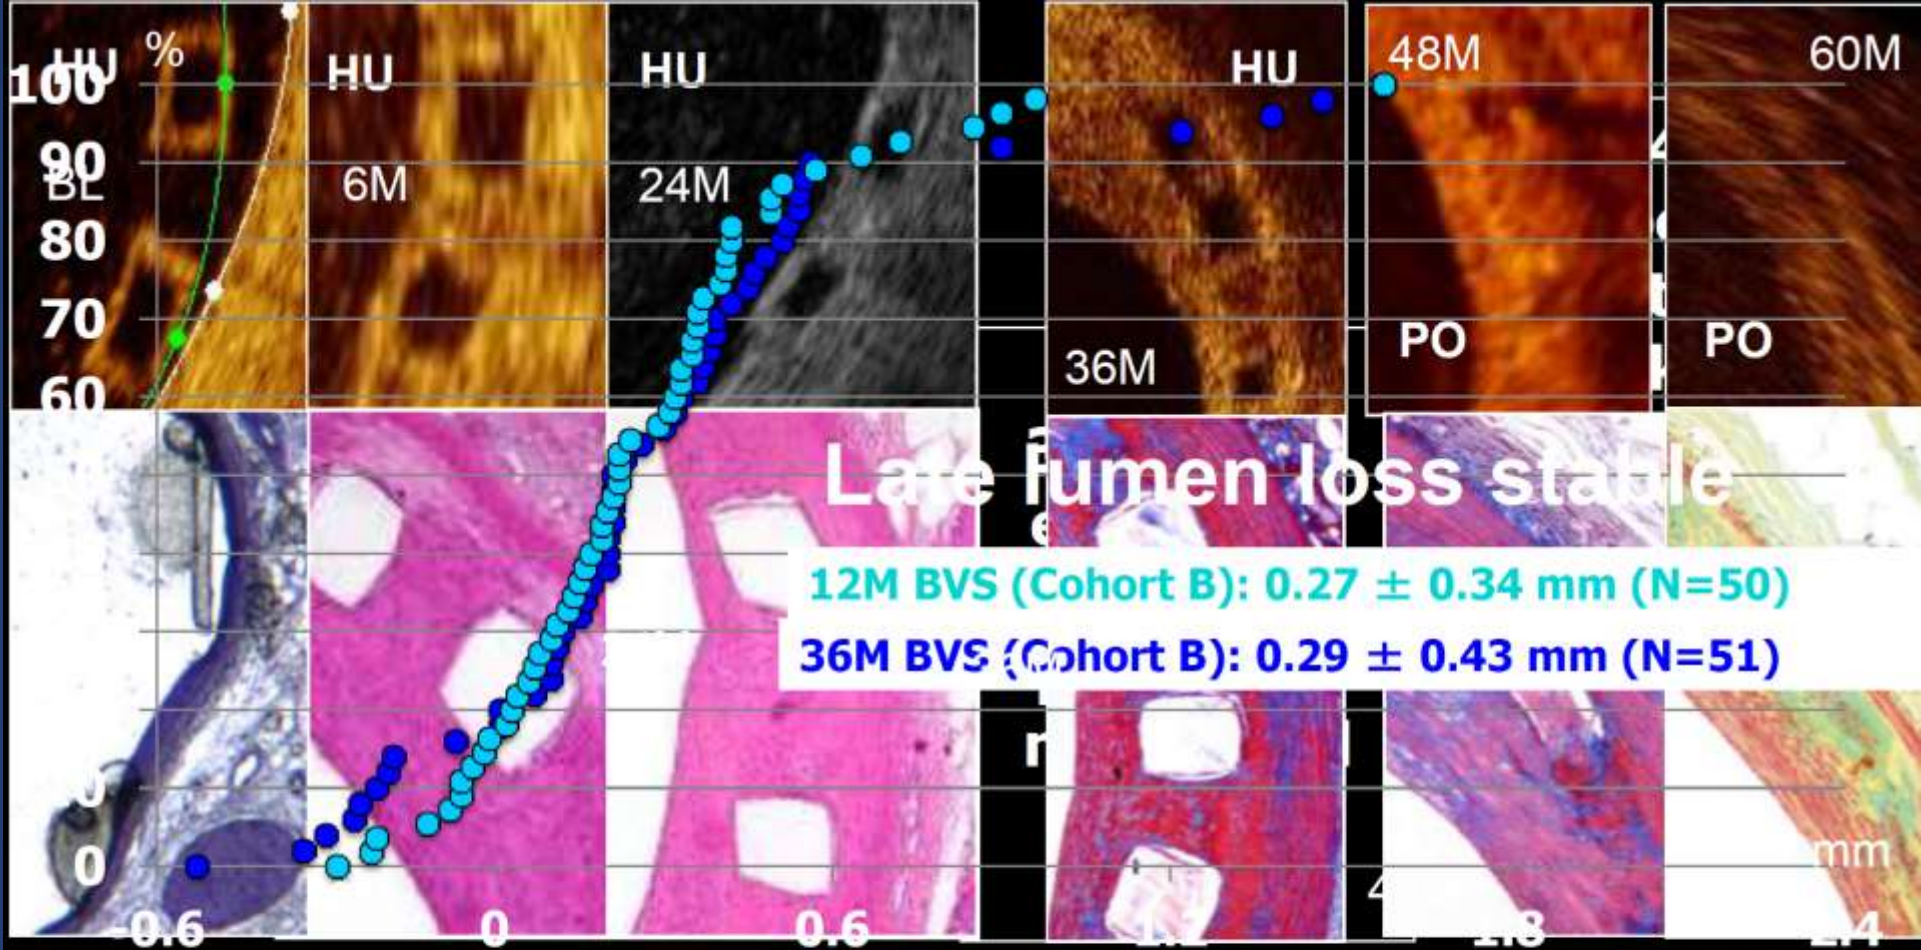




# ABSORB Cohort B

# ABSORB Cohort A & B

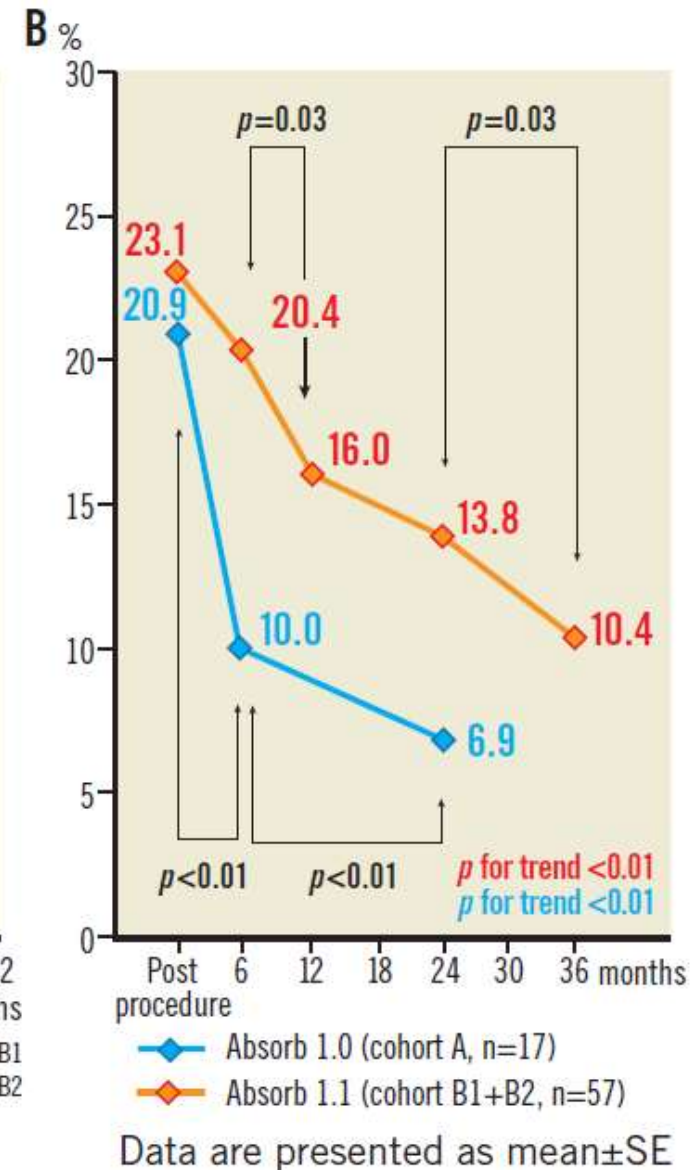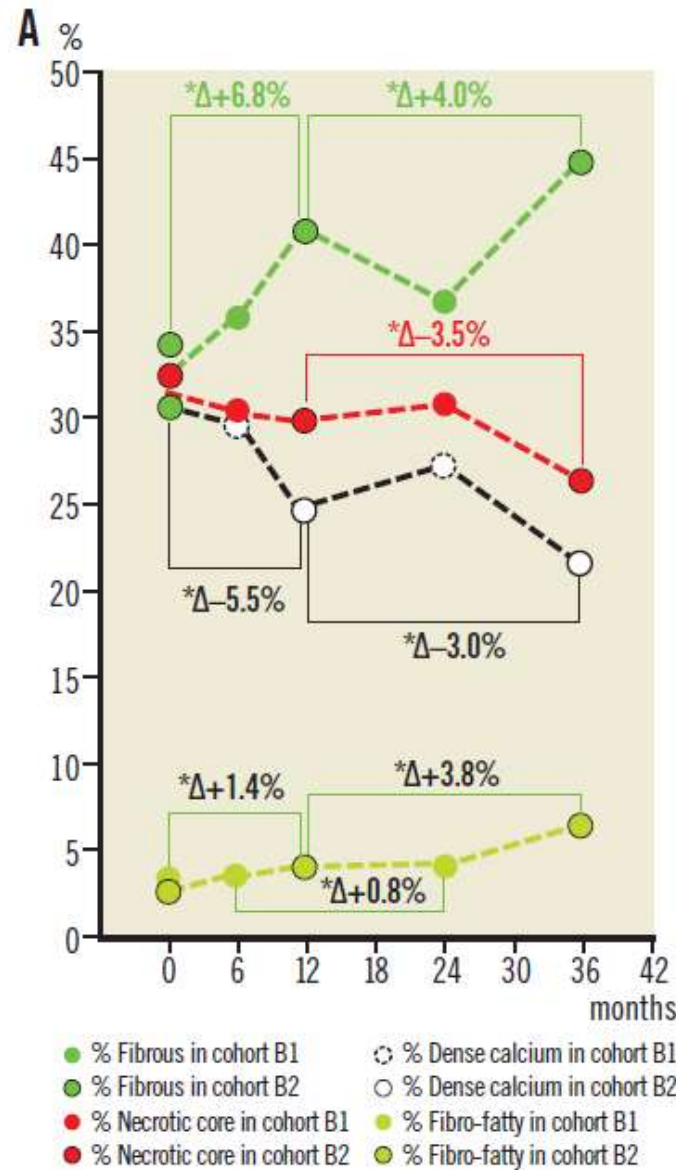


# Image for BRS implantation

# Vessel sizing by QCA

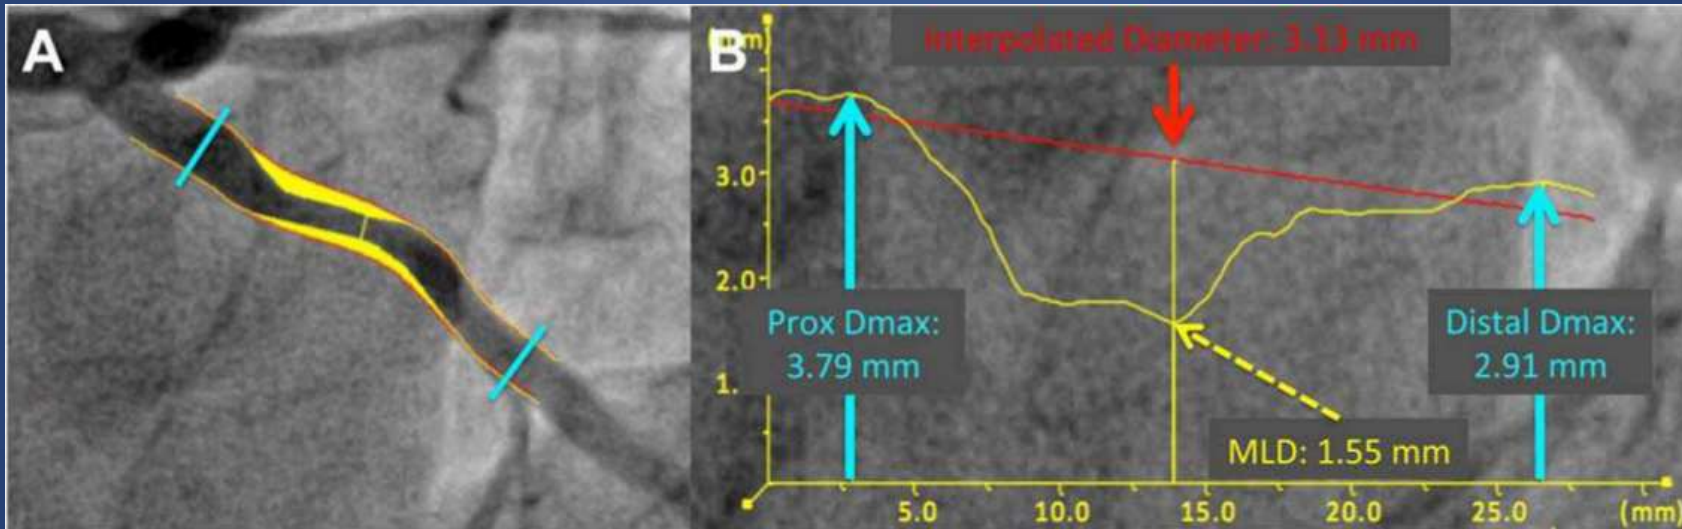


# Vessel sizing by IVUS

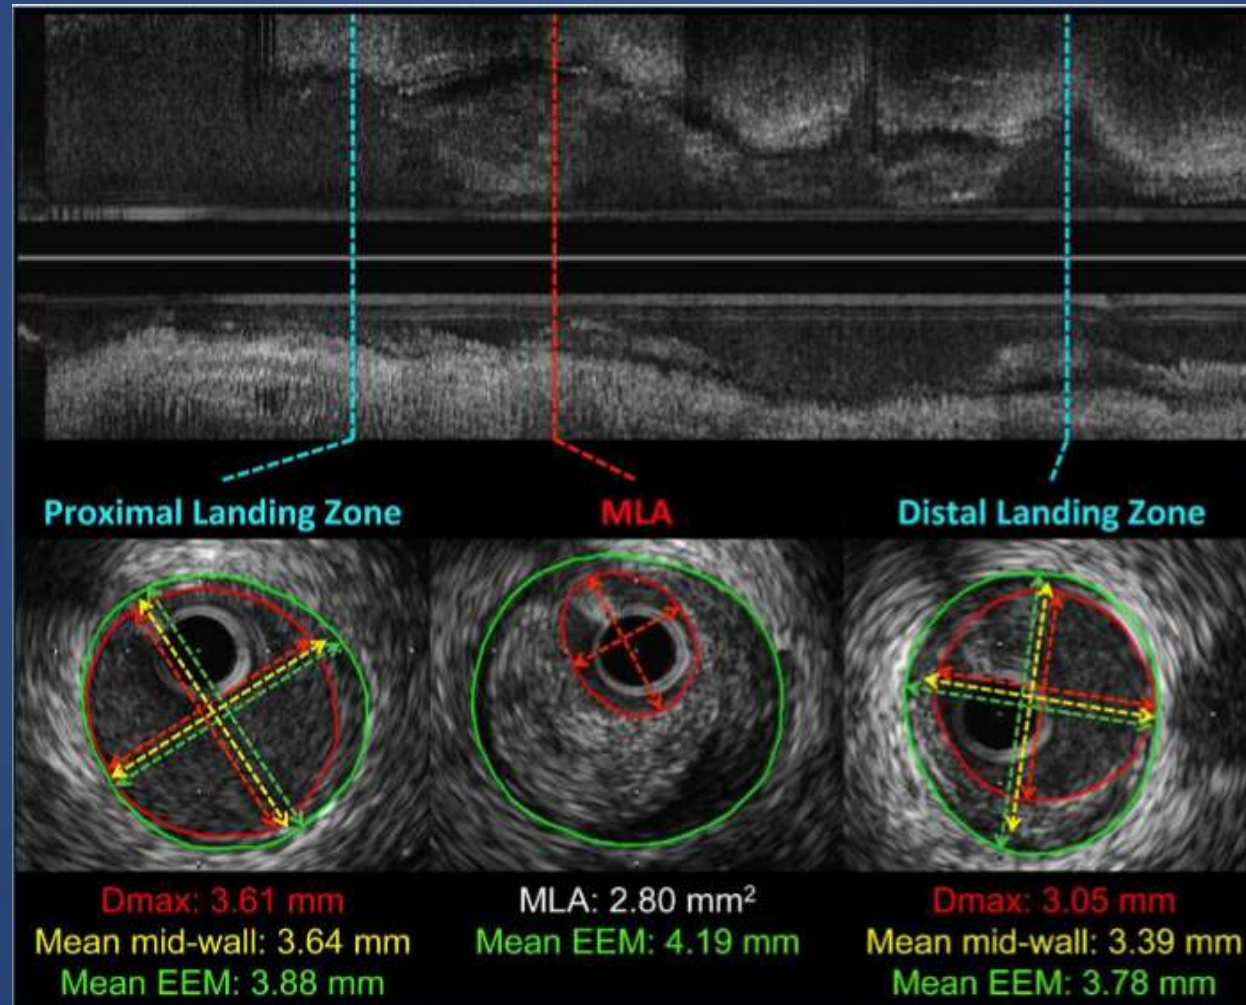




# Vessel sizing by OCT

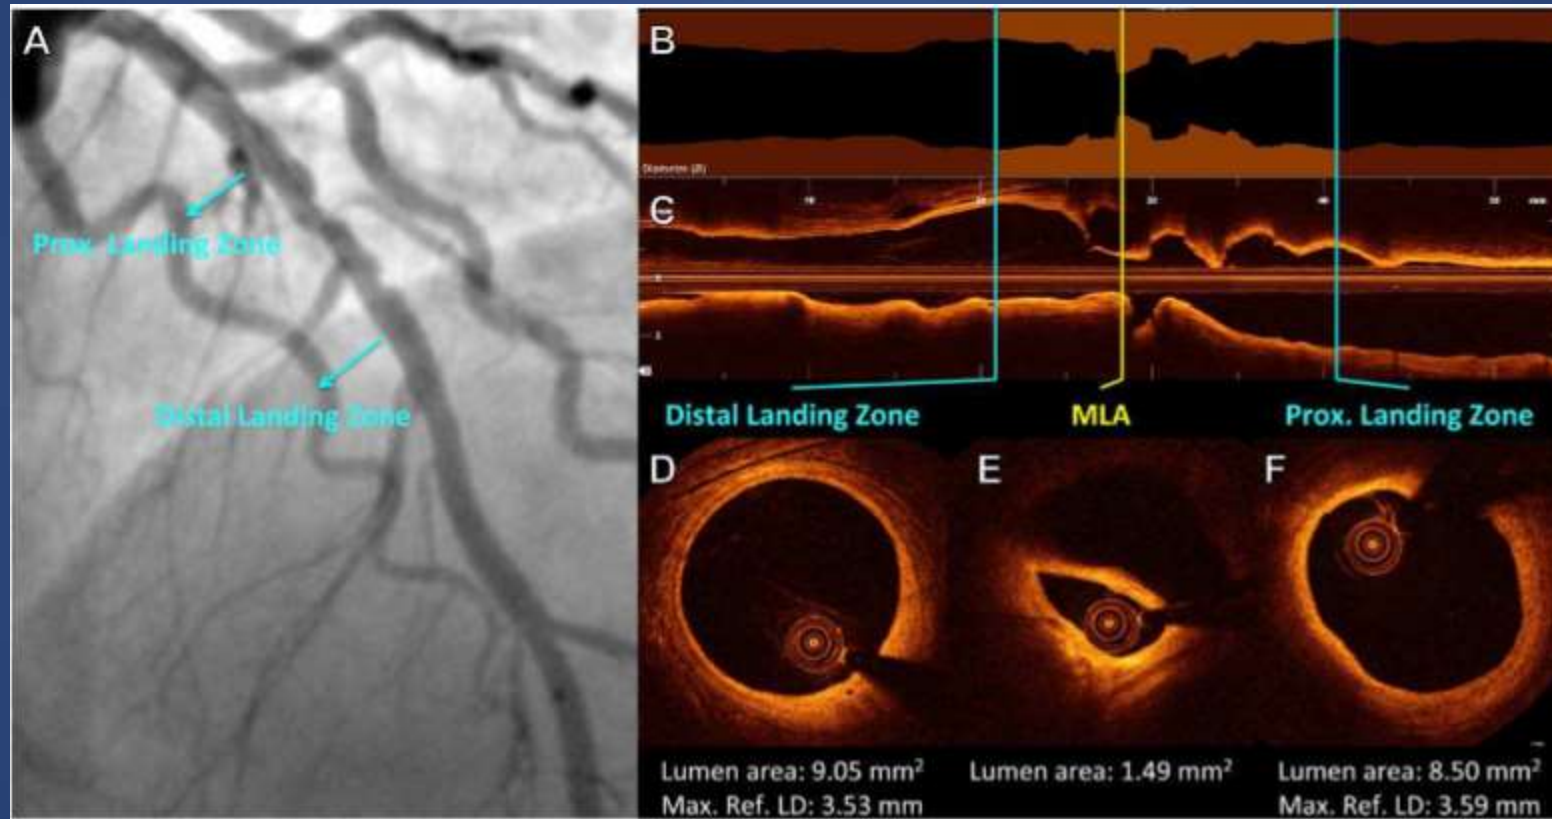


# Role of invasive image

## Proposed Algorithm

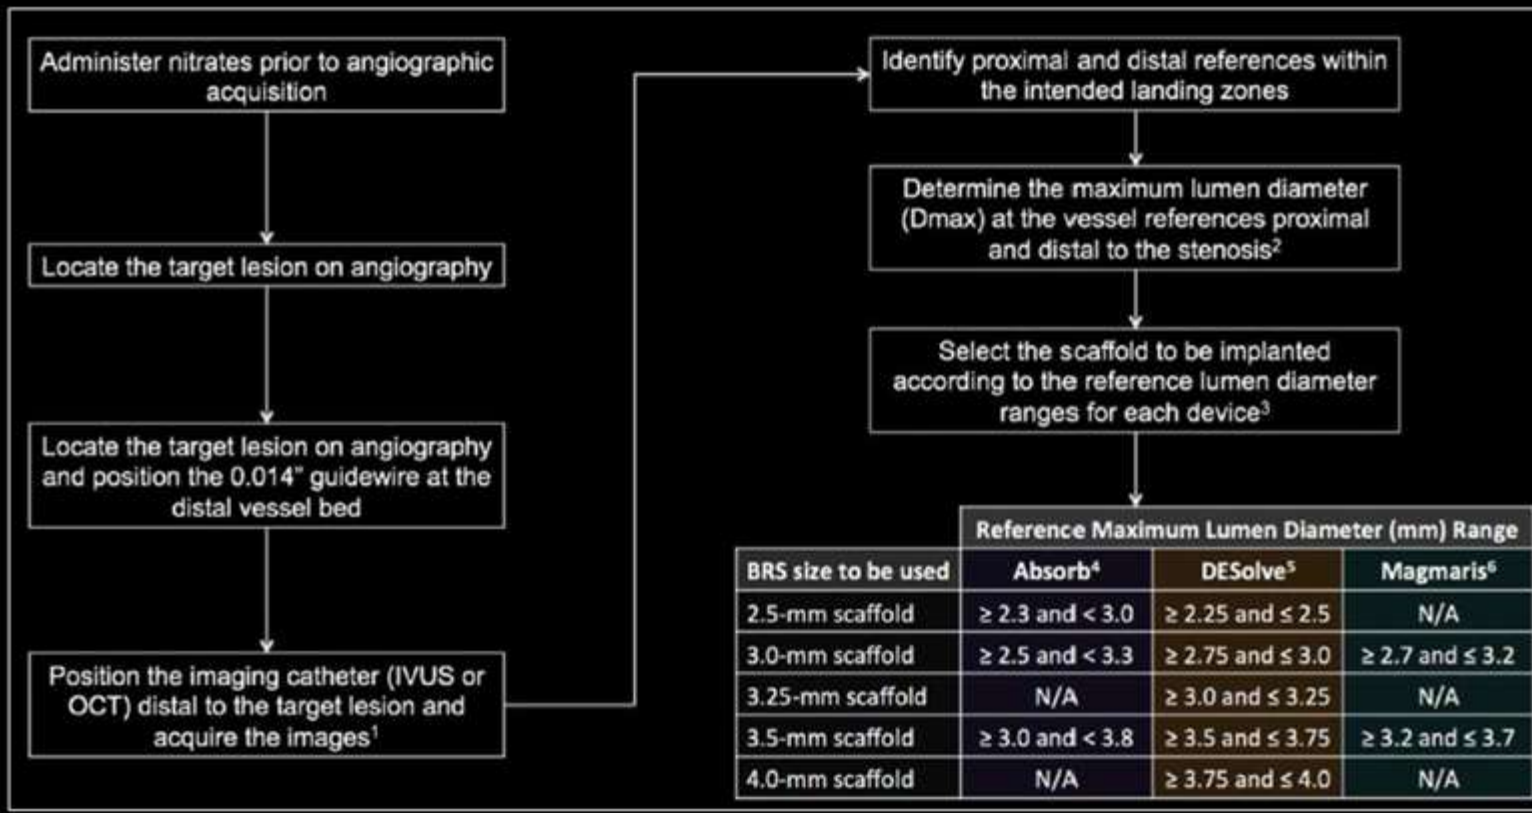


# Use of OCT

## When to use OCT in BRS implantation?

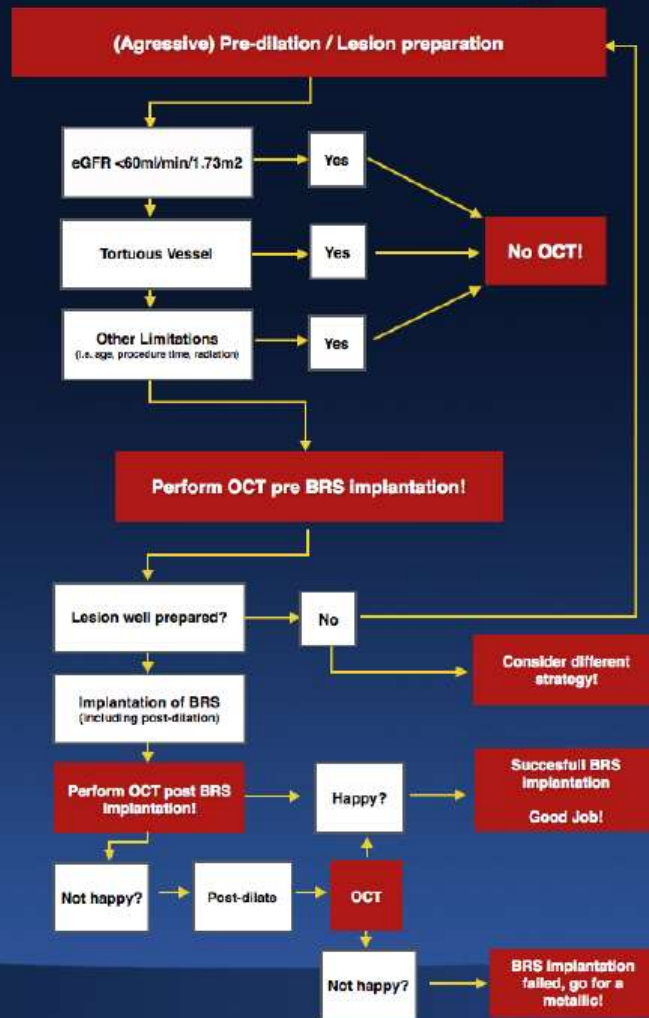


# ***BRS QCA vs. Imaging-guided***

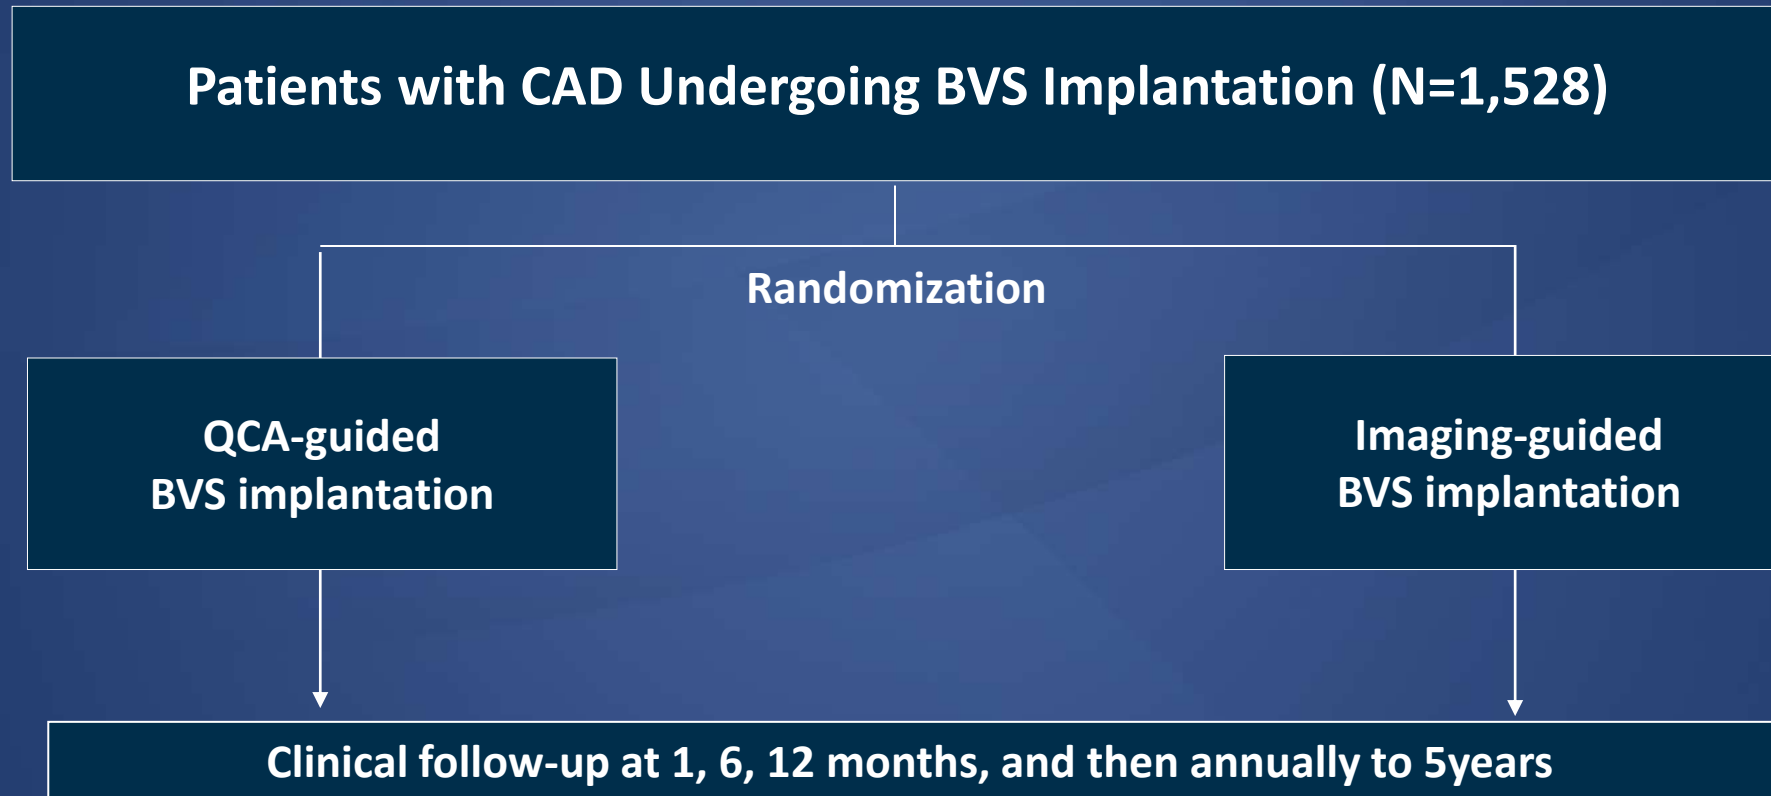


\*Primary endpoint: target-lesion failure (cardiac death, TV-MI, or ID-TLR) at 1 year

# BRS for ISR lesions: *RIBS VI*

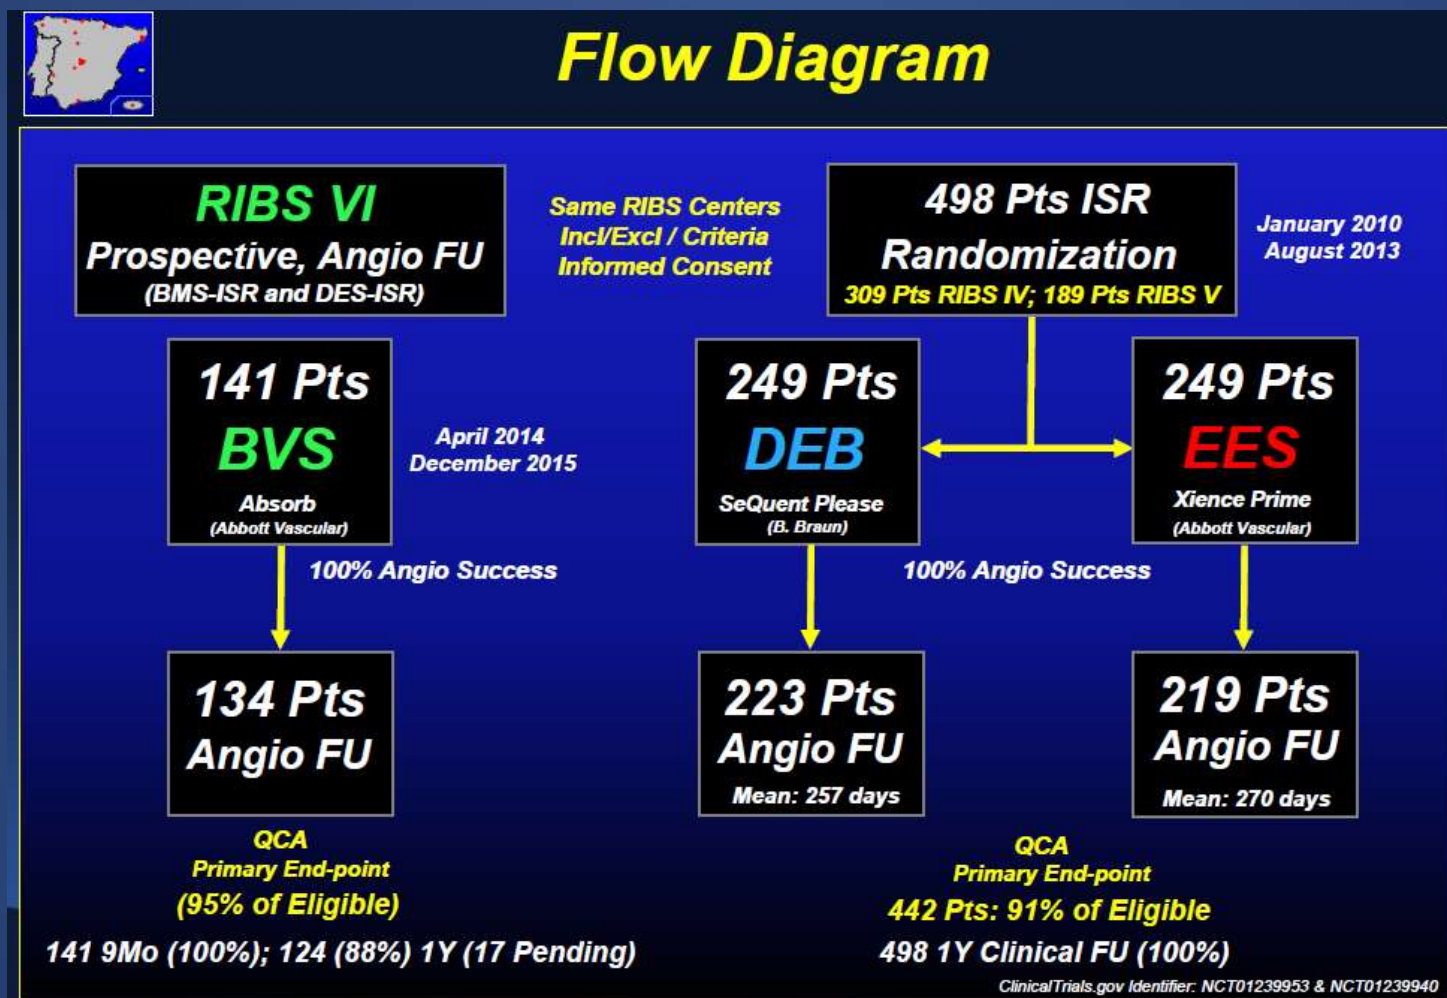



# RIBS VI


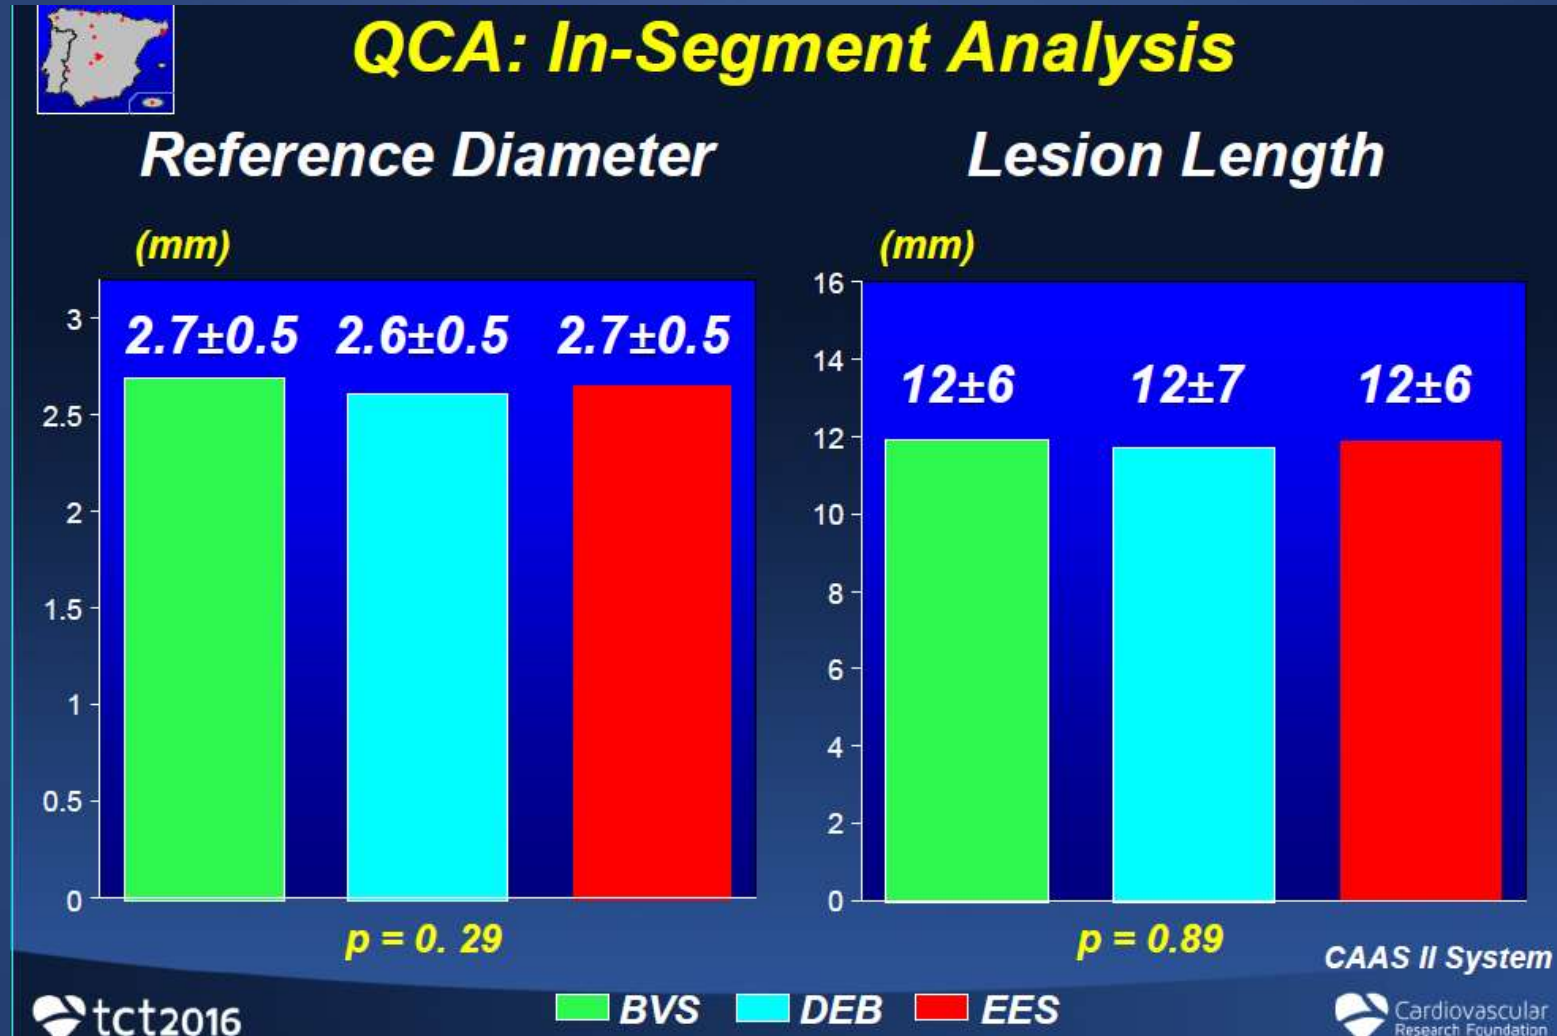





# RIBS VI




## QCA: MLD at FU

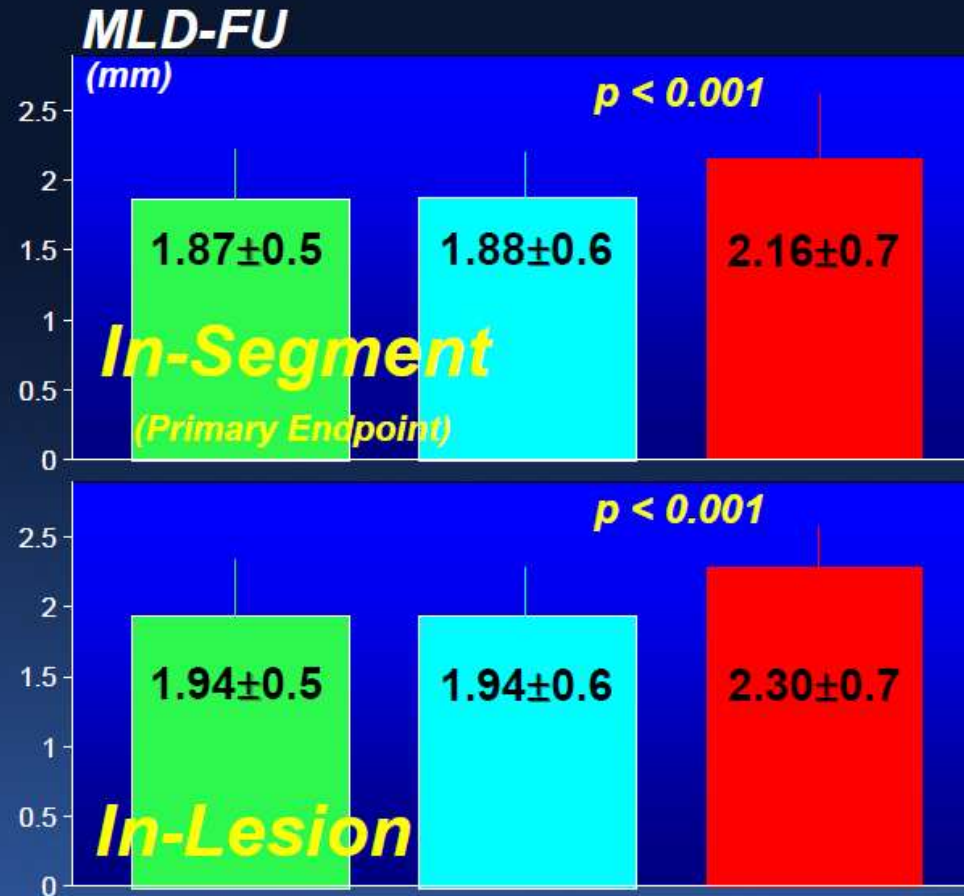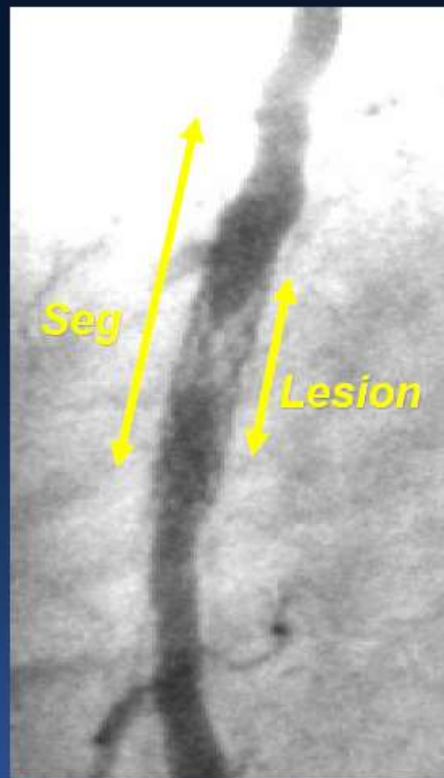


# RIBS VI

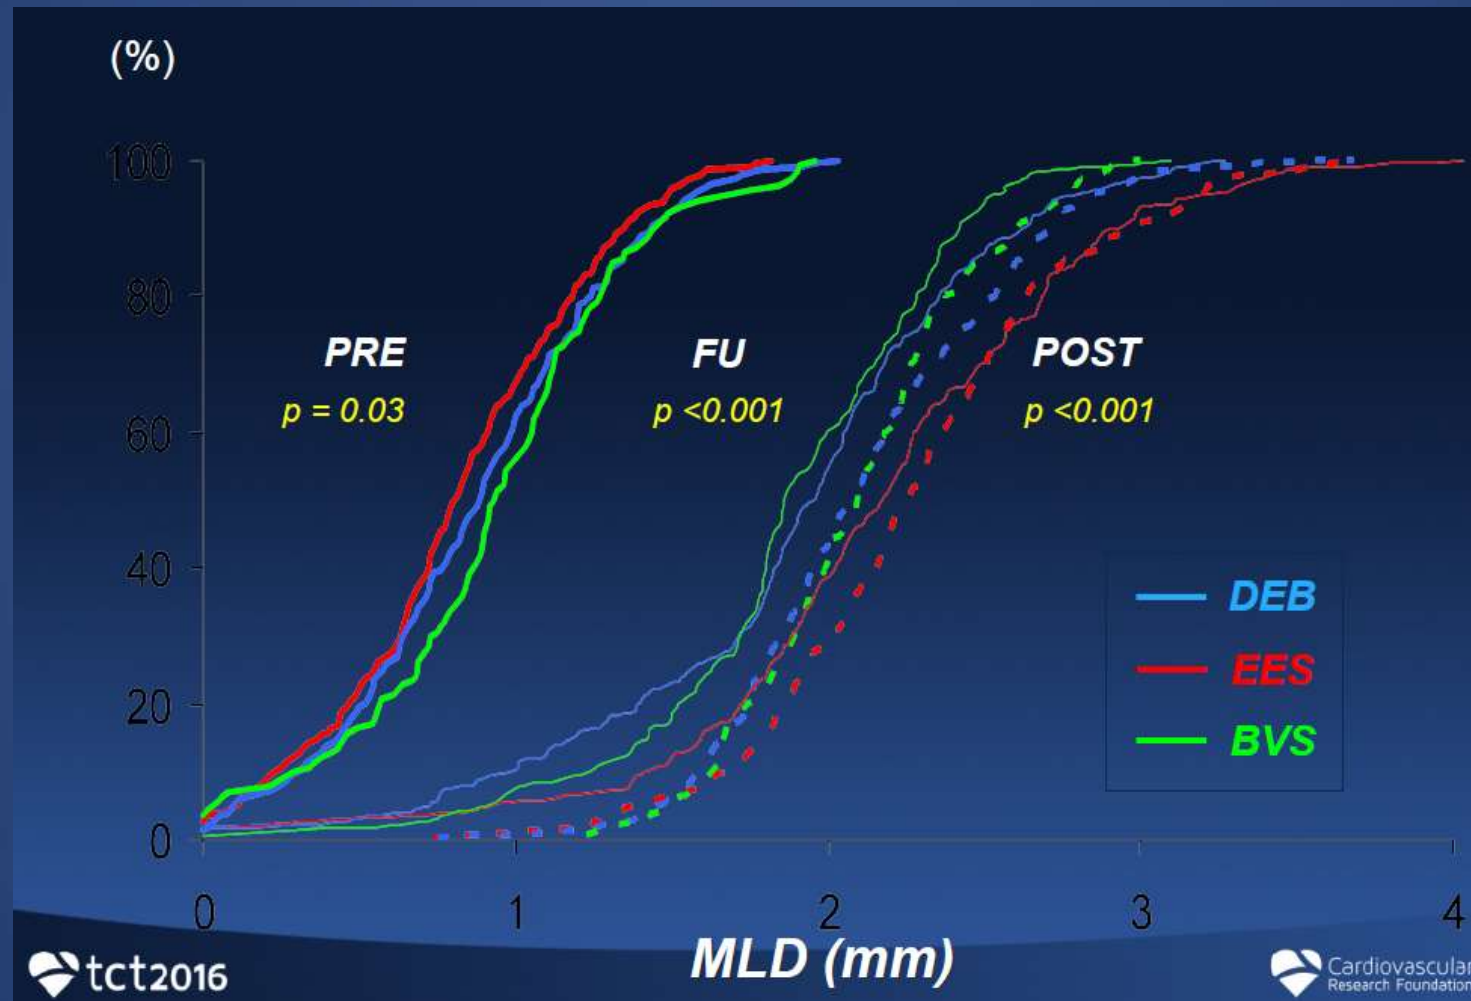

# RIBS VI

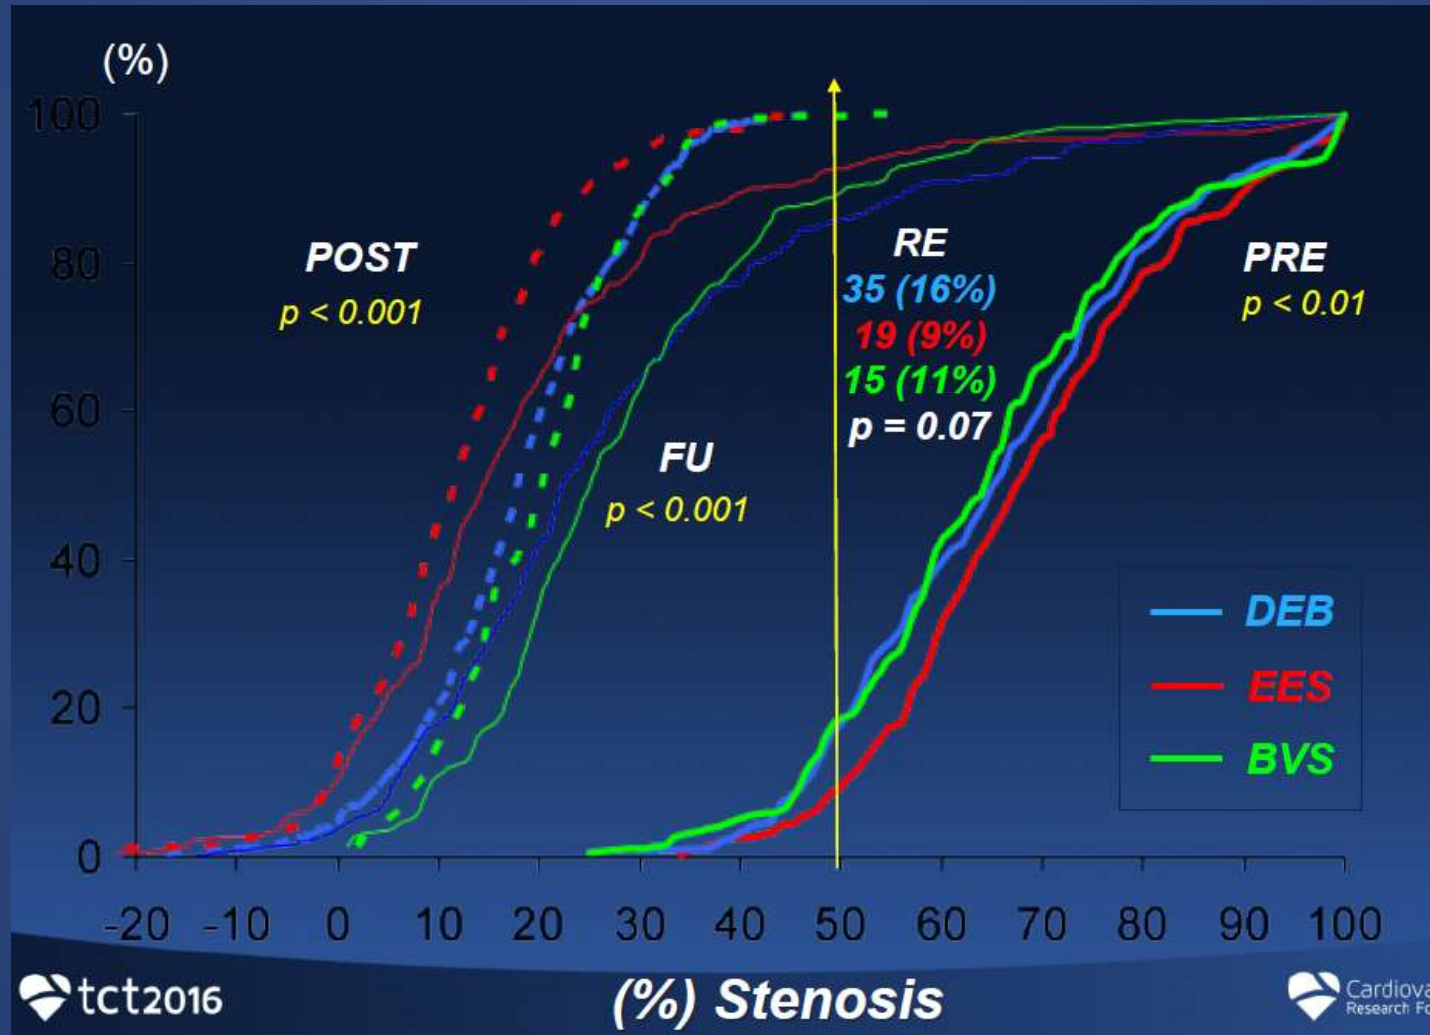

# RIBS VI

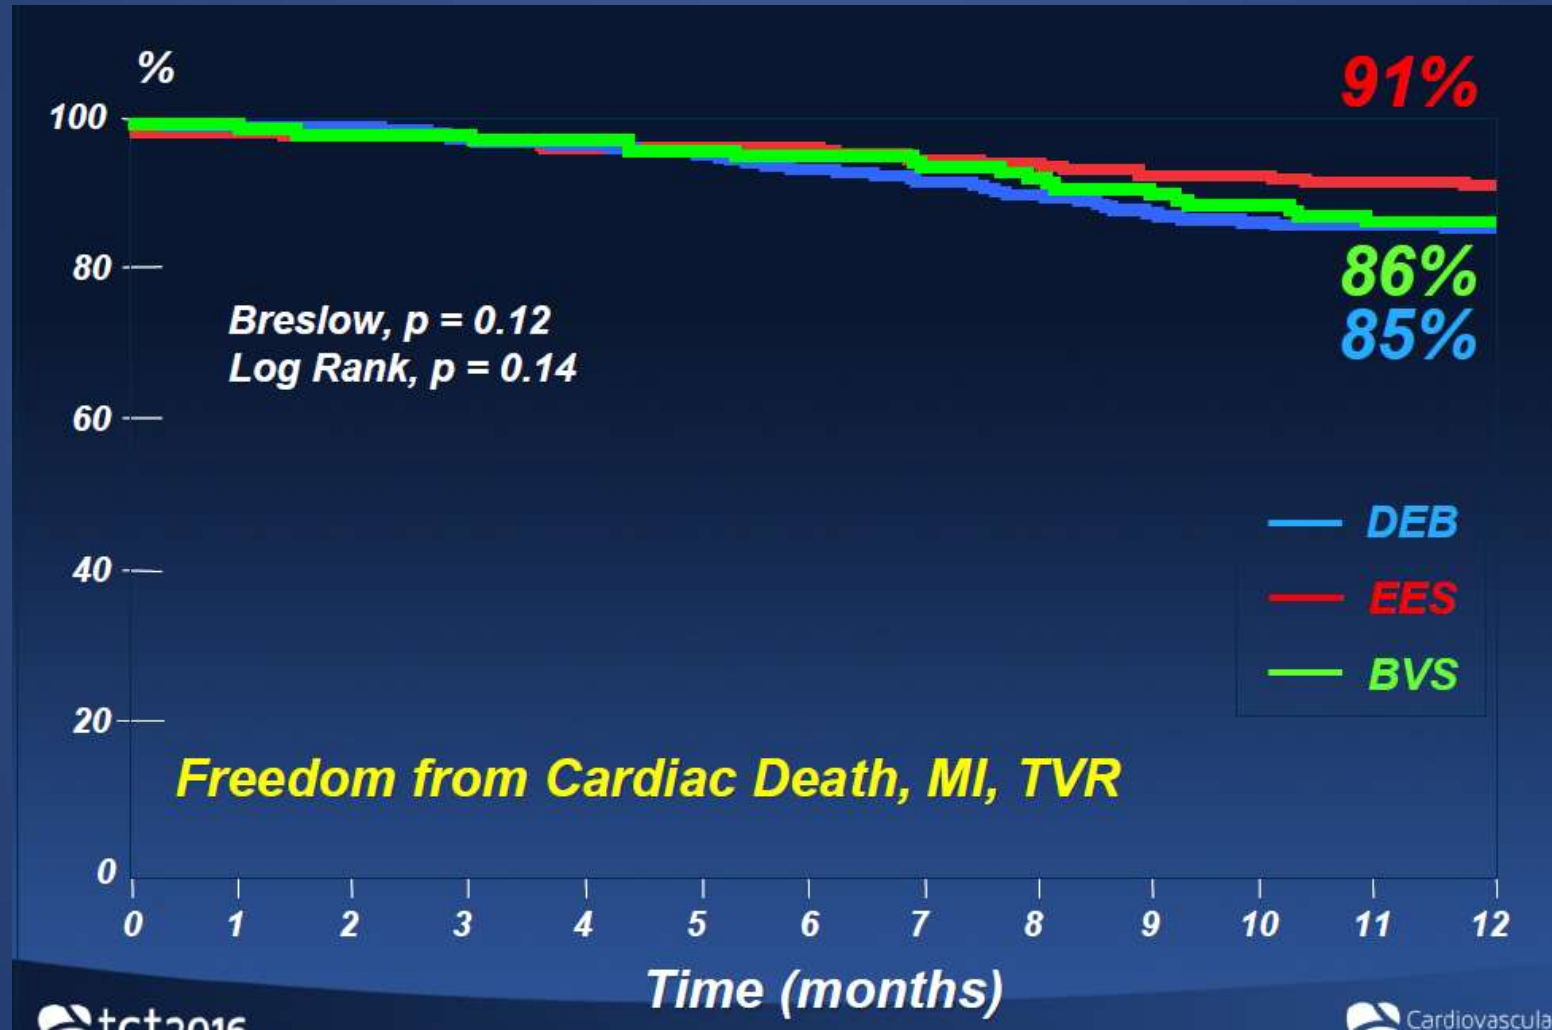


# RIBS VI






# BRS Hybrid technique

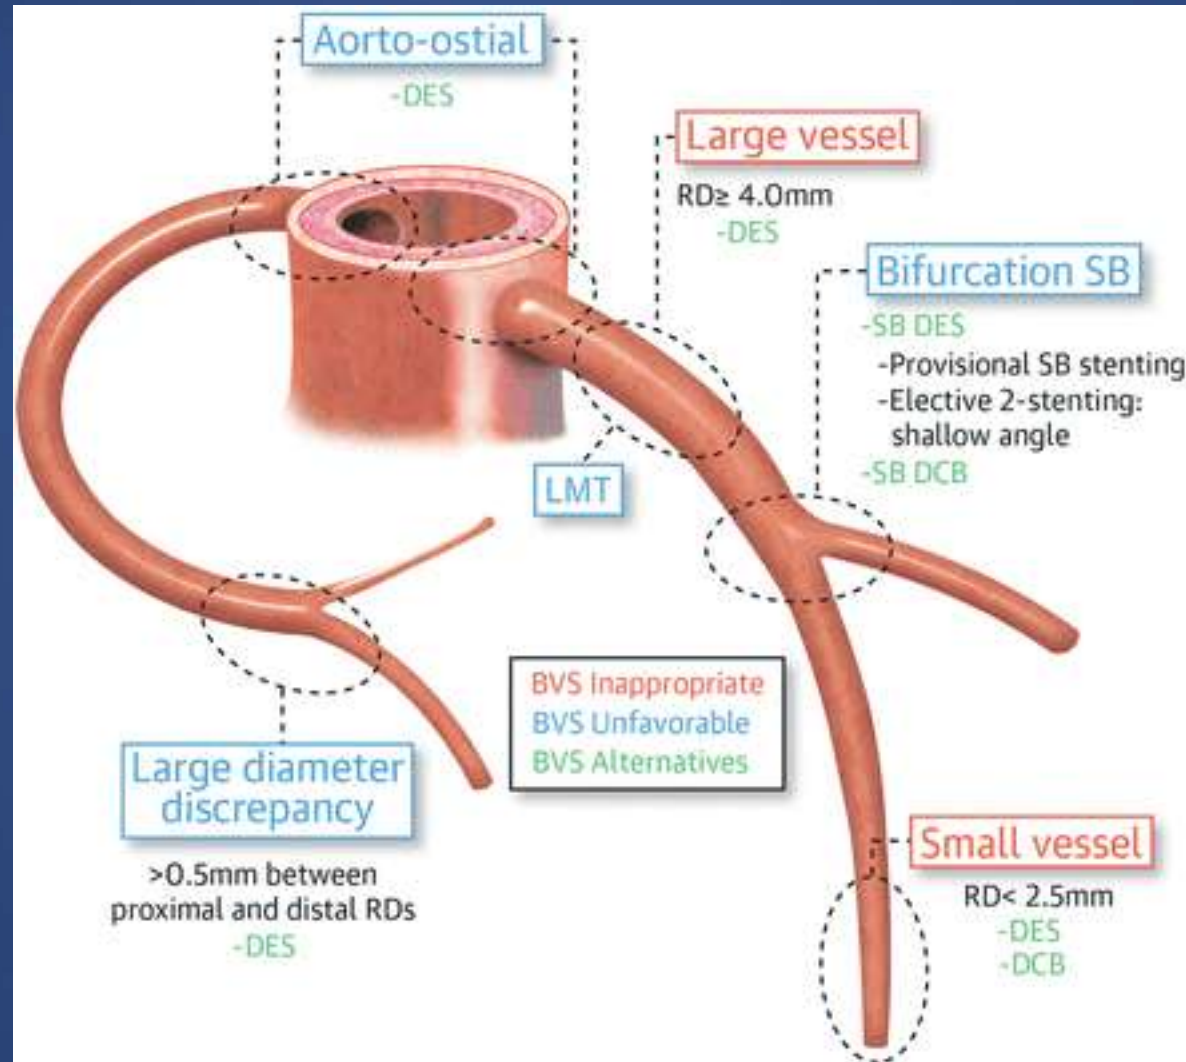


# BVS Hybrid technique

Involving long lesion

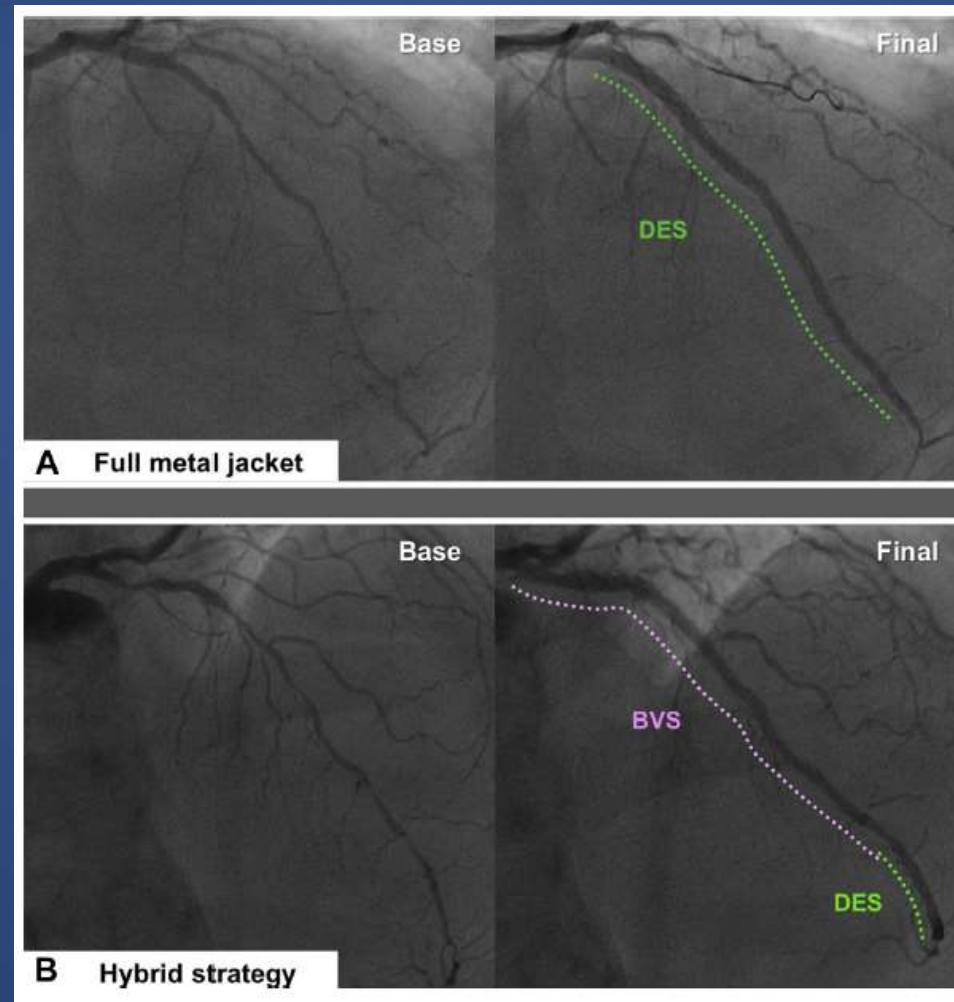


# BVS Hybrid technique


## Bifurcation Lesion

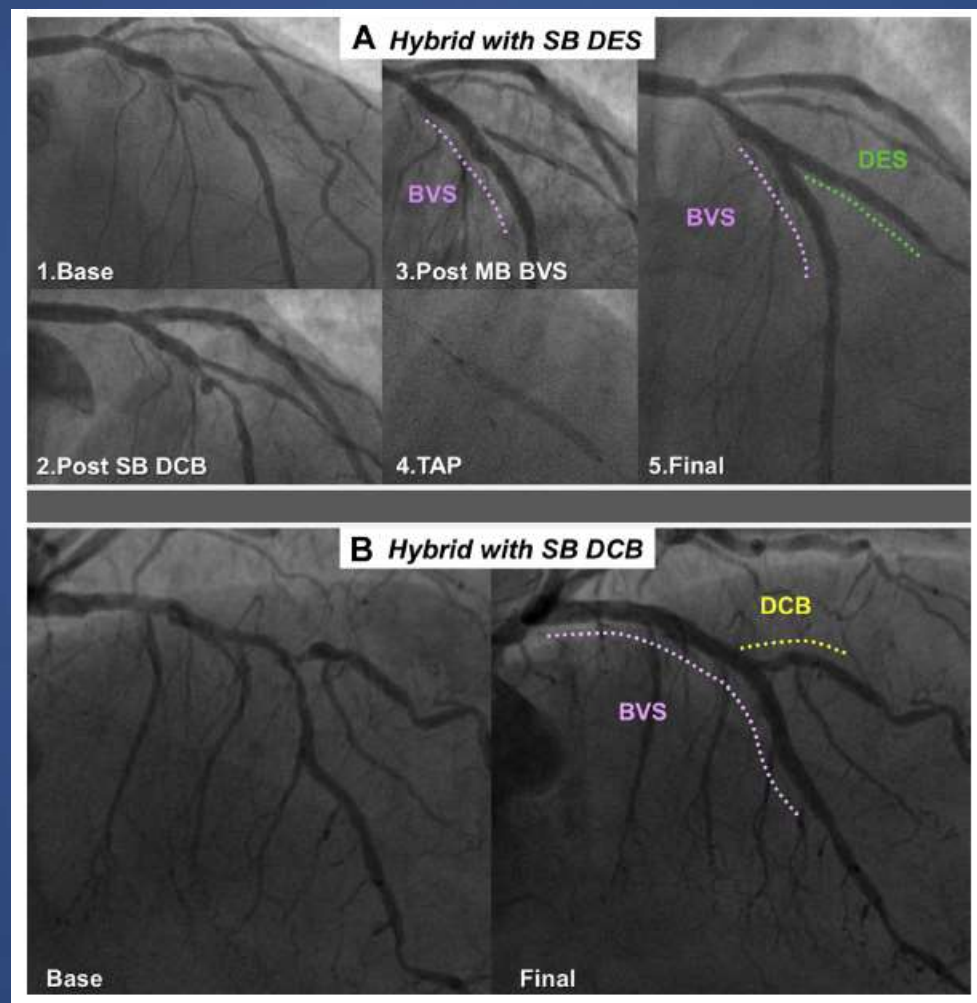

# Antiplatelet therapy for BVS

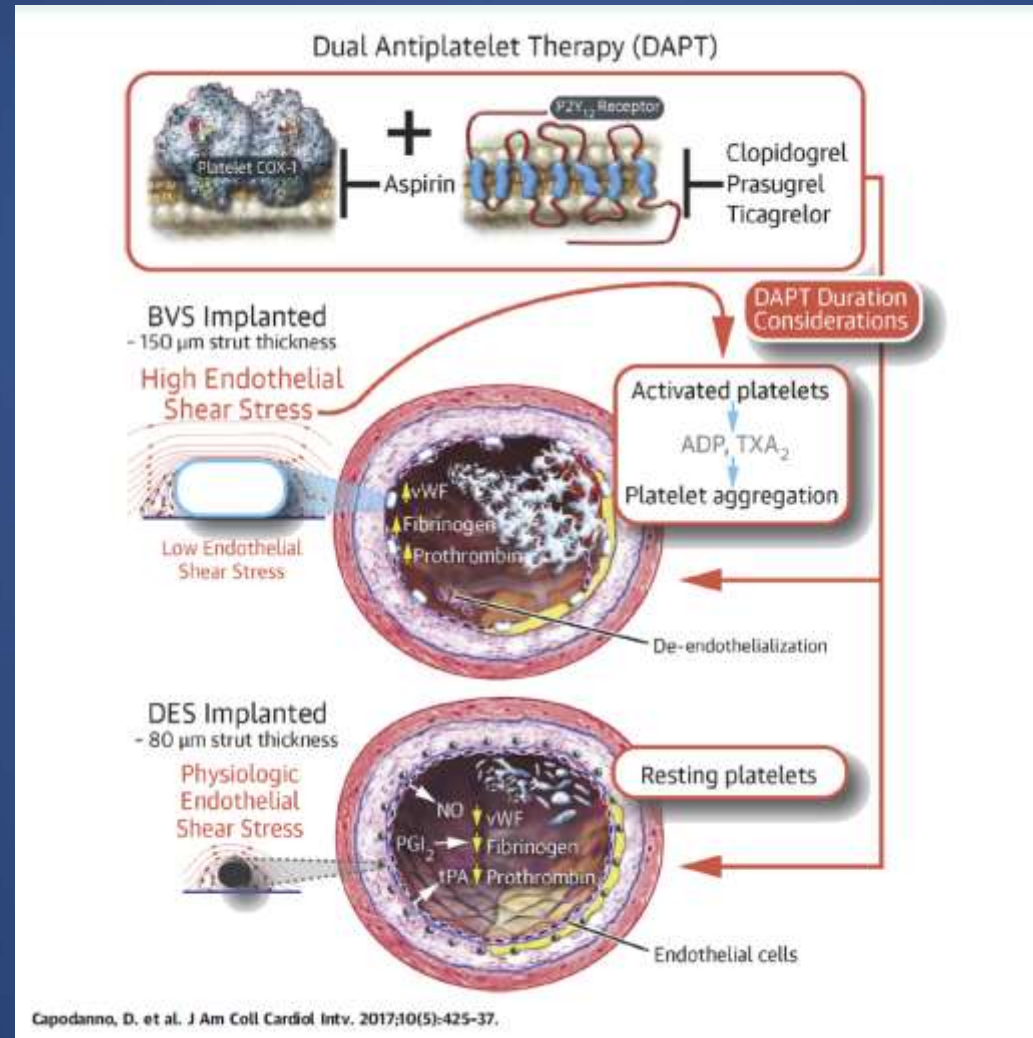


# Antiplatelet therapy for BVS

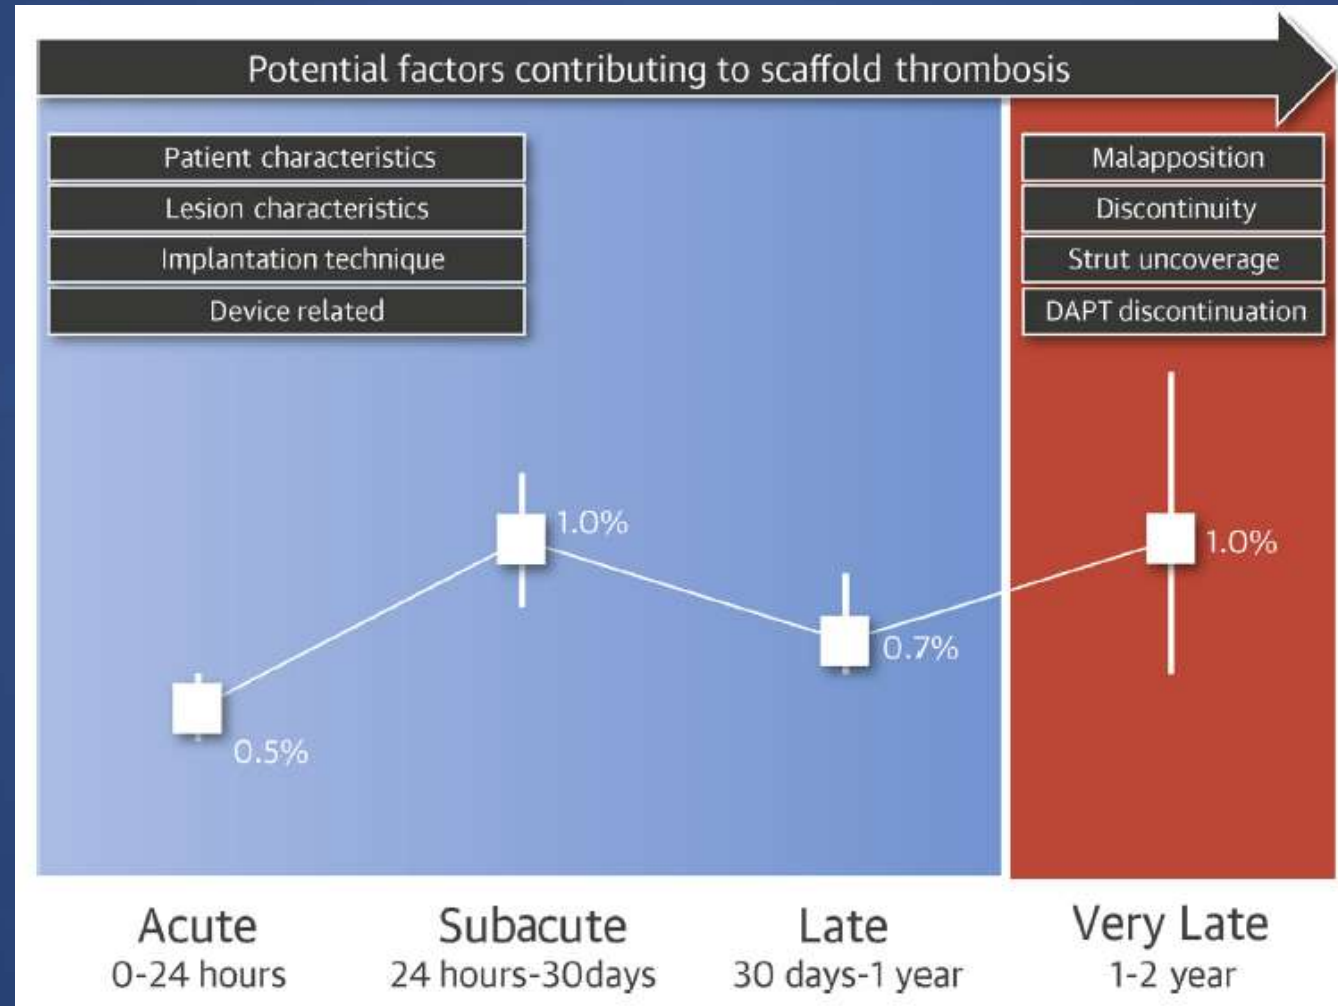



# Antiplatelet therapy for BVS

## Minimum Dual-Antiplatelet Therapy duration

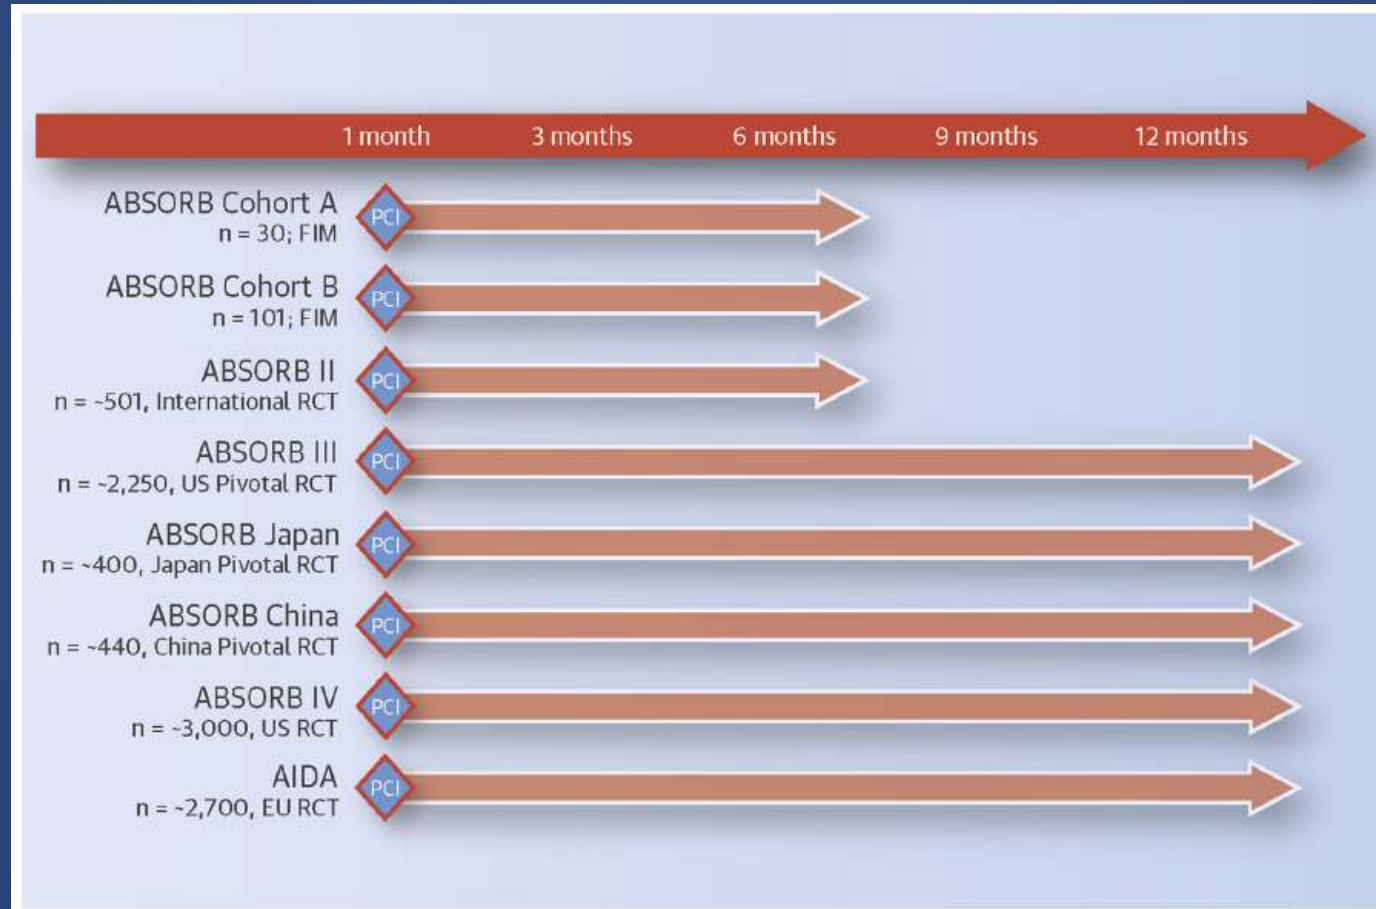

# Antiplatelet therapy for BVS

## Very late Scaffold thrombosis




# Antiplatelet therapy for BVS

## Event rates and Adherence to DAPT

	ABSORB II (23,25,43)		ABSORB CHINA (14)		ABSORB JAPAN (13,24)		ABSORB III (15)	
	BVS	EES	BVS	EES	BVS	EES	BVS	EES
Patients	335	166	241	239	266	134	1322	686
On P2Y <sub>12</sub> inhibitors								
1-yr follow-up	83.0%	83.0%	98.7%	99.2%	97.0%	97.3%	94.4%	95.0%
2-yr follow-up	36.2%	34.3%	NR	NR	52.3%	50.7%	—	—
3-yr follow-up	31.0%	30.0%	—	—	—	—	—	—
Definite or probable device thrombosis								
1-yr follow-up	0.9%	0.0%	0.4%	0.0%	1.5%	1.5%	1.5%	0.7%
2-yr follow-up	1.5%	0.0%	0.8%	0.0%	3.1%	1.5%	—	—
3-yr follow-up	2.8%	0.0%	—	—	—	—	—	—
ARR 1-2 yr follow-up	+0.6%	0.0%	+0.4%	0.0%	+1.6%	0.0%	—	—
ARR 2-3 yr follow-up	+1.3%	0.0%	—	—	—	—	—	—

# Antiplatelet therapy for BVS

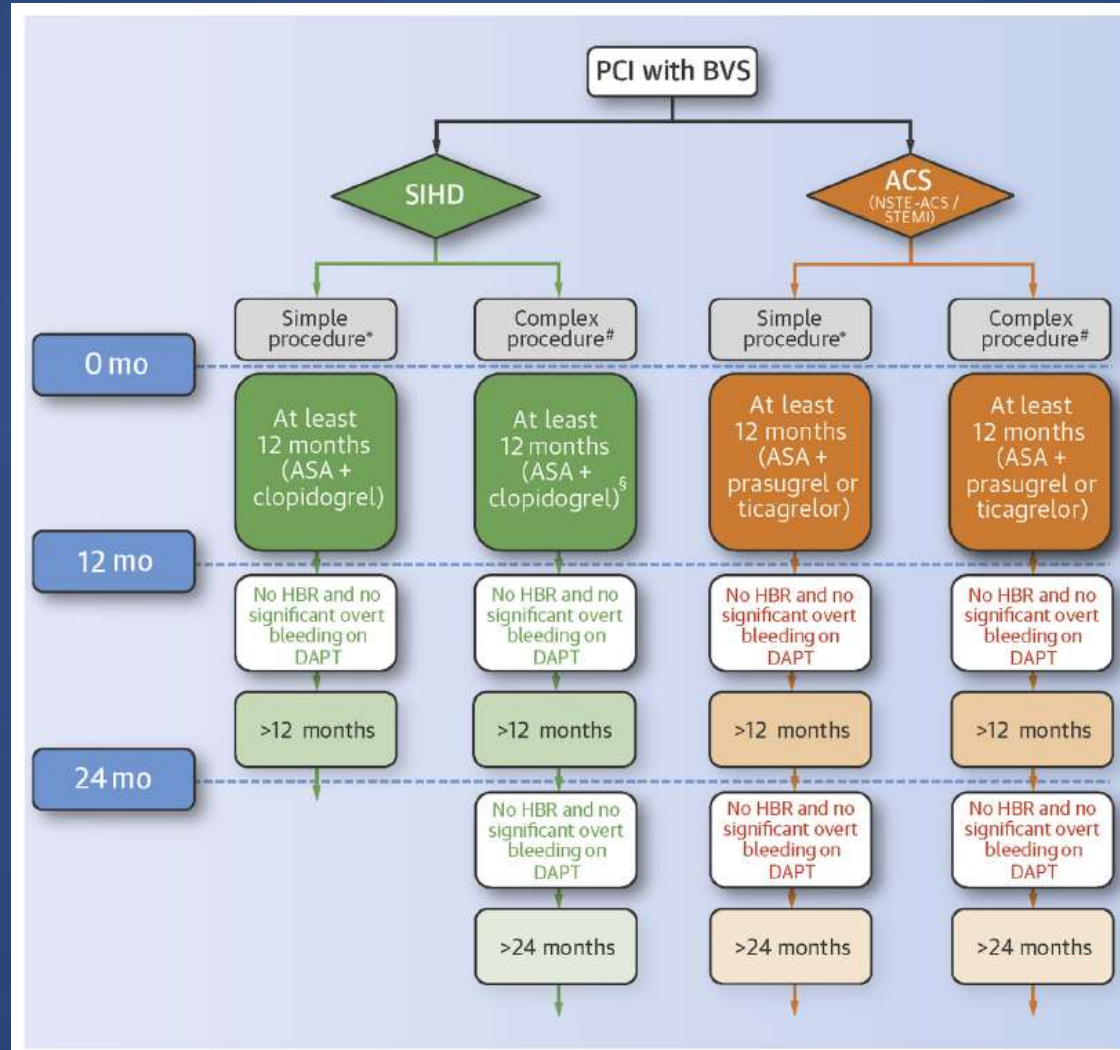


# ***BVS How Long DAPT?***

Optimal Duration of Antiplatelet Therapy after  
Bioresorbable Vascular Scaffold Implantation  
to Reduce Late Coronary Arterial Thrombotic Events

## **BVS-LATE Trial**

Patients on dual antiplatelet therapy without death, MI, or any revascularization  
During at least the first 12 months after Bioresorbable Vascular Scaffold implantation

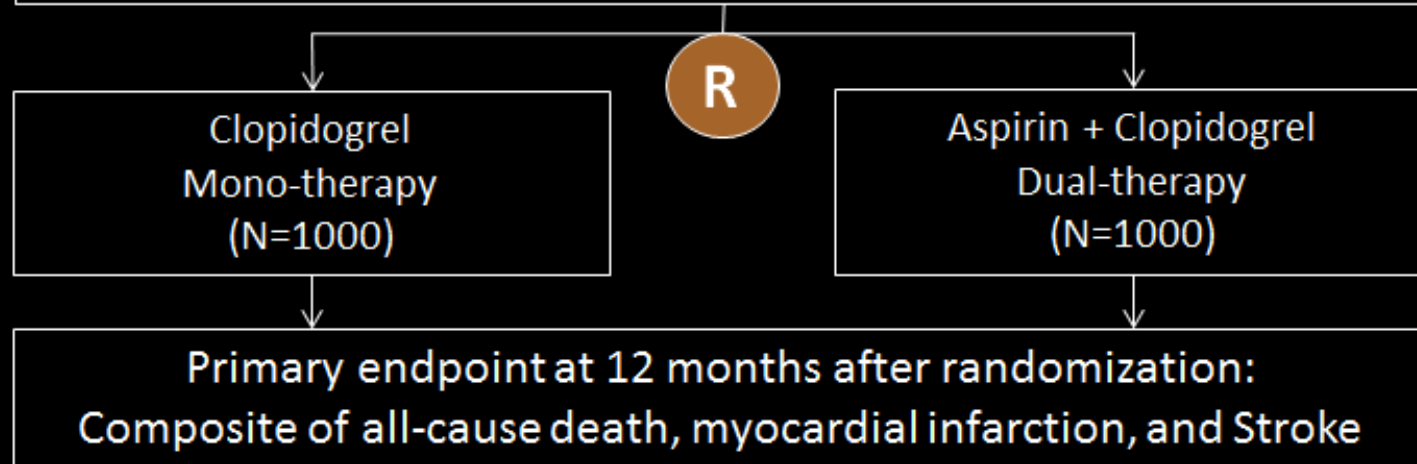



# Unresolved Mechanical Issues of BVS

- Complex lesions; calcified or tortuous, long lesion, bifurcation, left main
- Stretchability and fracture
- Overlapping
- Side branch
- Relatively high late loss

# ***Appropriate Use of Absorb in Current Practice***

## ***Appropriate***

Big Vessel >2.5 mm  
Young Age <70 years  
Diabetes  
STEMI  
Multi-vessel Disease  
Long Lesion  
Bifurcation (Provisional)  
CTO

## ***Not Yet***


Bifurcation (2 stents)  
Severe Calcification  
ISR

# What do I need to Know to Use the Absorb Scaffold Appropriately?

1. Is Imaging guided BRS implantation mandatory ?
2. What are the early results in complex lesions compared to those of 2<sup>nd</sup> Generation DES ?
3. Is one year DAPT enough ?
4. Are the long term results really better with Absorb ?

# How to Do *QCA guided Absorb* ?

QCA  
Proximal RD  
3.7 mm

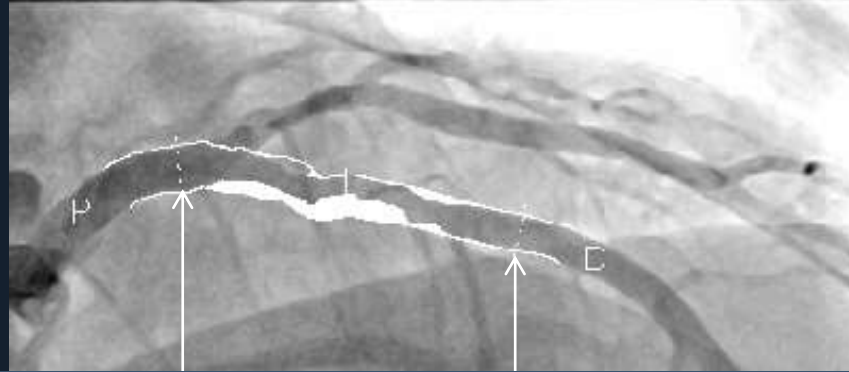

QCA  
Distal RD  
3.0 mm


- P** 3.0x 20 mm NC balloon pre-dilation
- S** 3.5x 28 mm Absorb deployed
- P** 3.5 mm NC balloon post-dilation for distal part and 4.0x 15 mm NC balloon post-dilation for proximal part

# How to Do *IVUS guided Absorb* ?

## *Exactly Same Procedure !*


QCA  
Proximal RD  
3.7 mm

IVUS RD  
4.2 mm

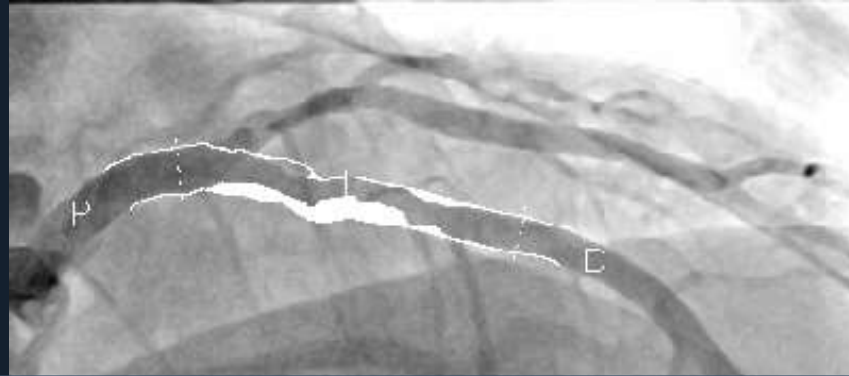


QCA  
Distal RD  
3.0 mm

IVUS RD  
3.5 mm

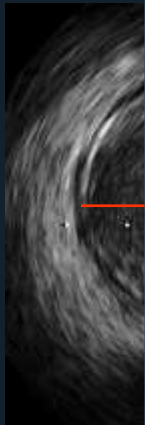


- P** 3.0x 20 mm NC balloon pre-dilation
- S** 3.5x 28 mm Absorb deployed
- P** 3.5 mm NC balloon post-dilation for distal part and 4.0x 15 mm NC balloon post-dilation for proximal part





# Increased Risk of ST


## Definite or Probable Scaffold Thrombosis

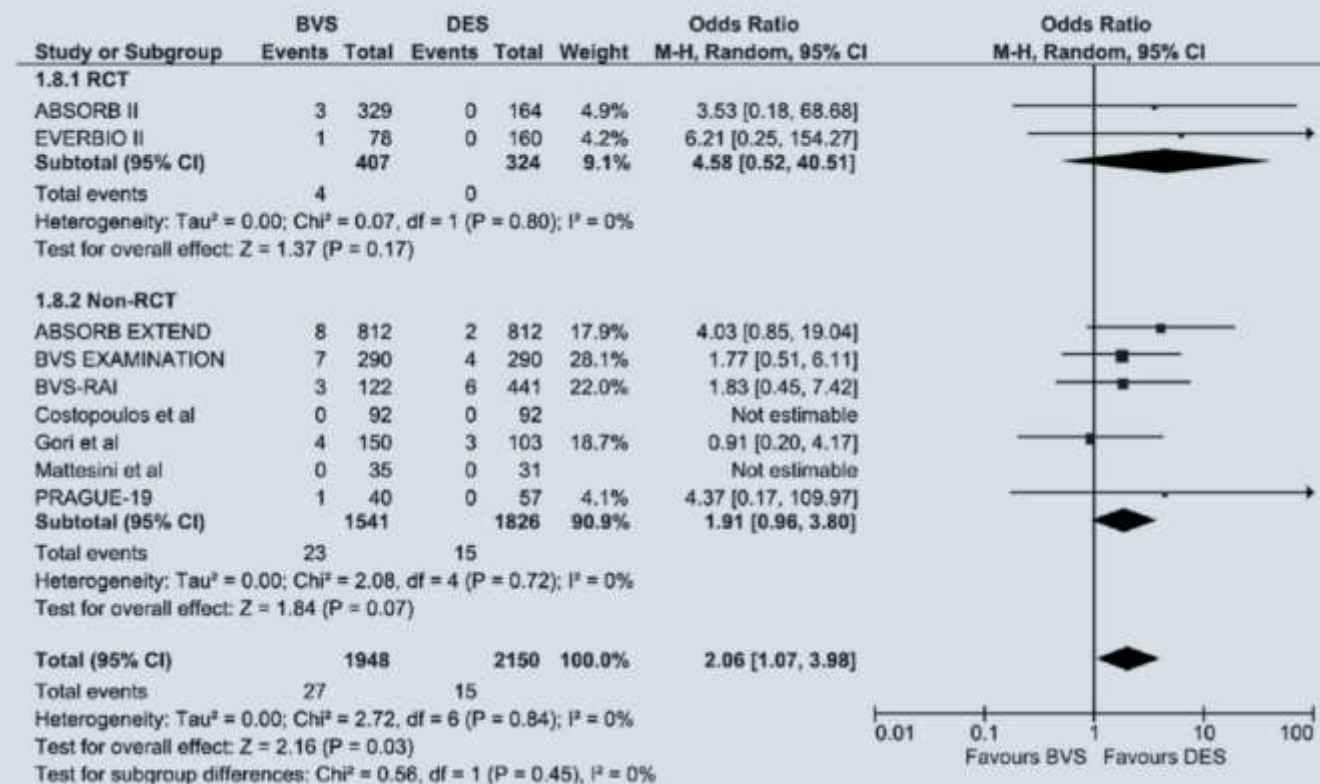

# *Concept of PSP*

# *BVS Thrombosis Reduced with Improved Technique !*

Scaffold  
Thrombosis (%)

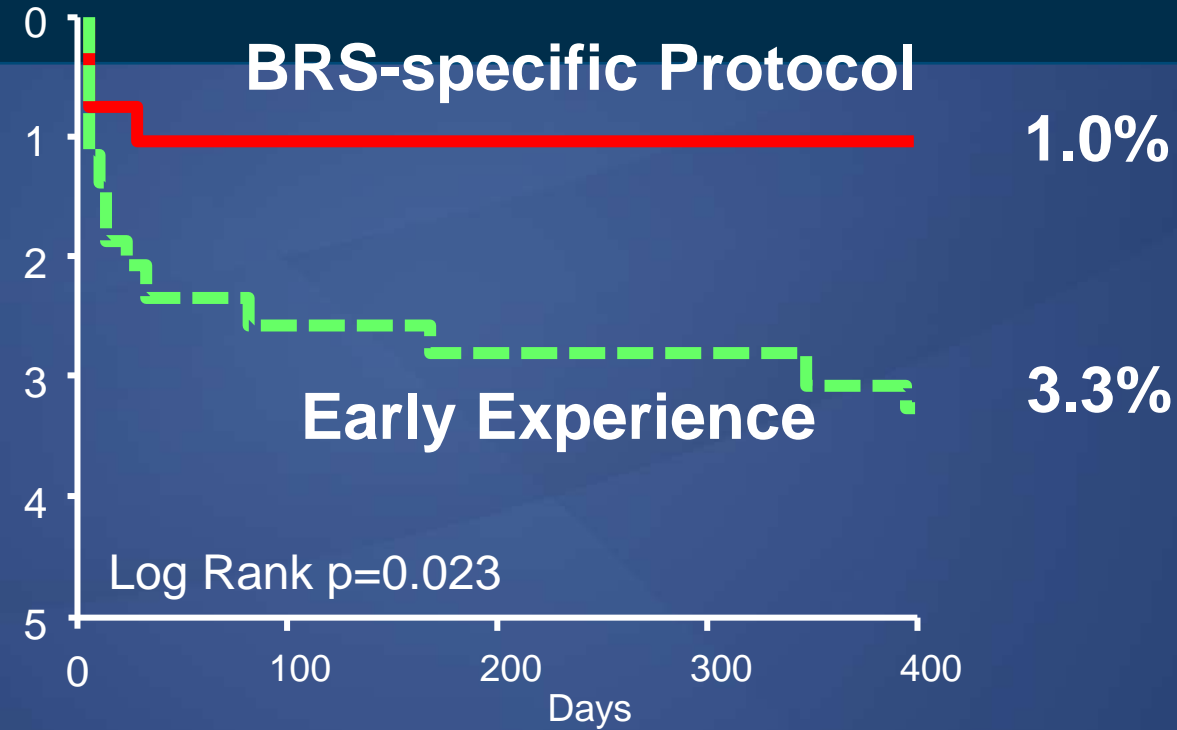

Patients					
Early Experience	369	369	369	369	369
Absorb-specific	292	292	281	217	155

# *Recommended Technique*

## *BVS Specific Protocol*

### **P** *Pre-Dilation*

Pre-dilation with noncompliant balloon, 1:1 with the RVD.

### **S** *Sizing* *Appropriately*

BVS of the same size as the RVD at 10 to 12 atm.


### **P** *Post-Dilation*

Post-dilation with noncompliant balloon with a maximum of 0.5mm larger at 14 to 16 atm.

# PSP Use by Trial (As-Treated Population)


EXTEND	108/772	(14.0%)
ABSORB-II	21/324	(6.5%)
ABSORB-Japan	35/258	(13.6%)
ABSORB-China	32/237	(13.5%)
ABSORB-III	96/1224	(7.8%)

# Significant Improvement of Outcomes In GHOST-EU At 1 Year *With Completed PSP*

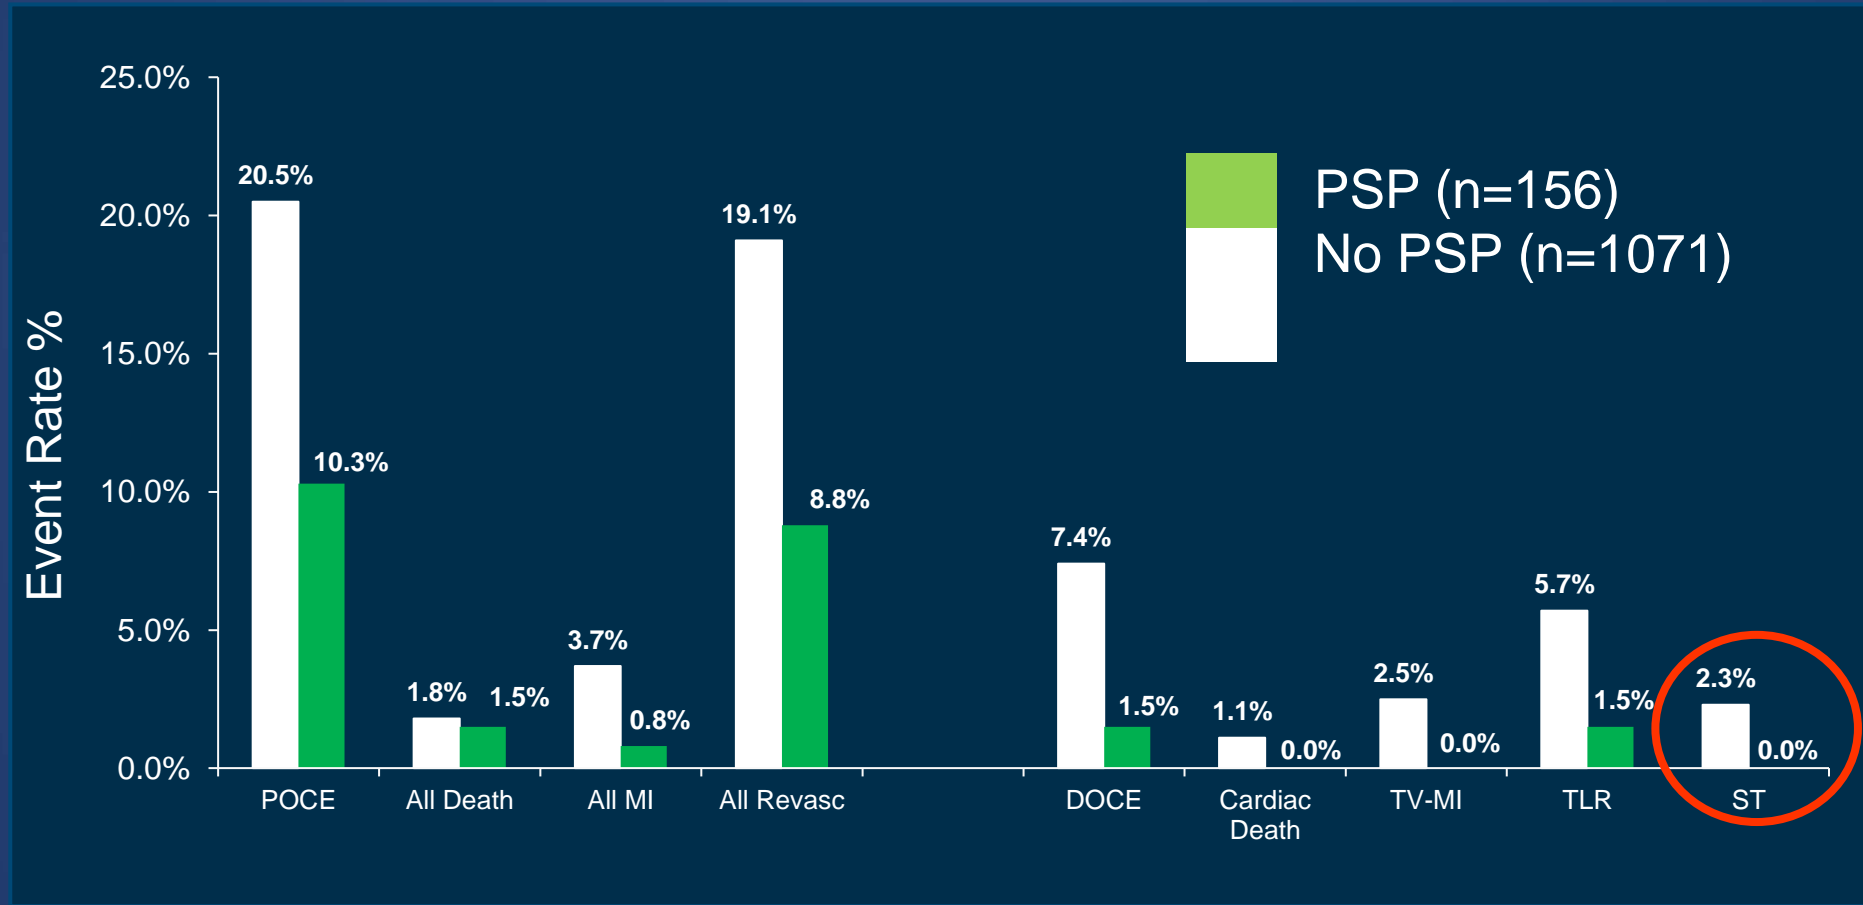




# PSP Analysis - TLF At 3-Years (Absorb Patients, As-Treated Population)

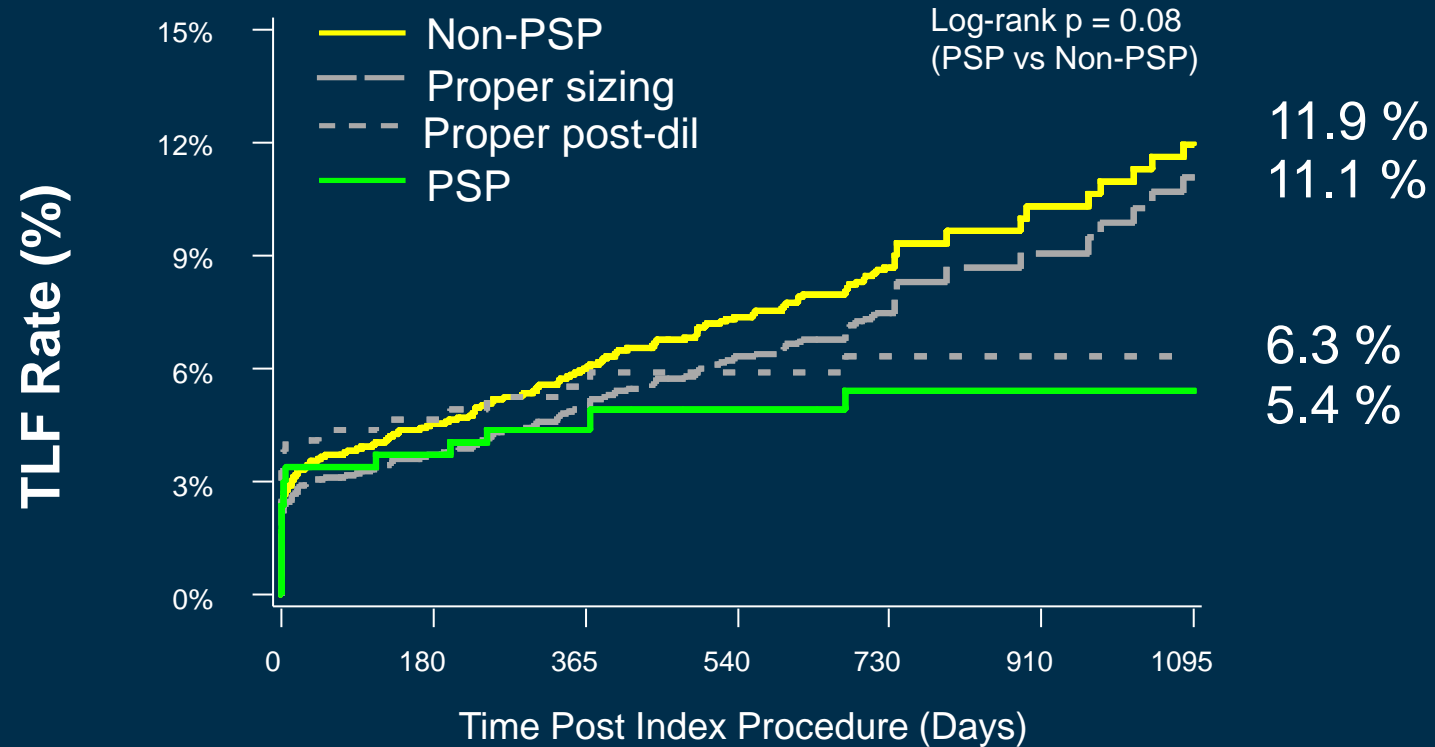

	0	365	730	1095
Non-PSP	2549	2375	1289	268
Proper Sizing	2261	2125	1195	223
Proper post-dil	365	341	219	24
PSP	297	280	186	20

0-365 days population: A-EXTEND, A-II, A-Japan, A-China, A-III  
 366-730 days population: A-EXTEND, A-II, A-Japan, A-China  
 731-1095 days population: A-II

# PSP Analysis – Def/Prob ST At 3-Years (Absorb Patients, As-Treated Population)

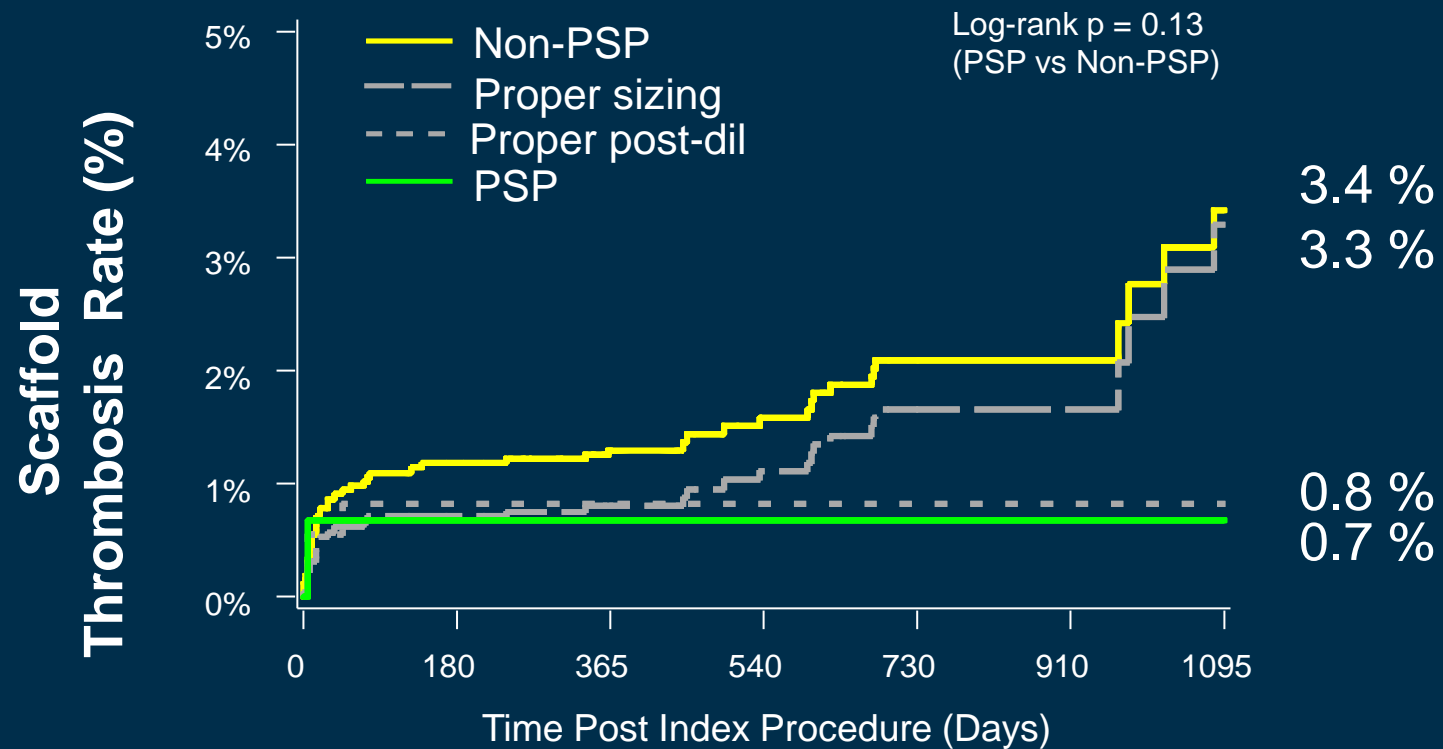

	0	365	730	1095
Non-PSP	2549	2483	1354	291
Proper Sizing	2261	2211	1247	238
Proper post-dil	365	357	227	26
PSP	297	290	192	21


0-365 days population: A-EXTEND, A-II, A-Japan, A-China, A-III

366-730 days population: A-EXTEND, A-II, A-Japan, A-China



731-1095 days population: A-II

# 1-Year ST in Very Small Vessels, ABSORB 3

## Impact of Post-Dilatation and Pressure

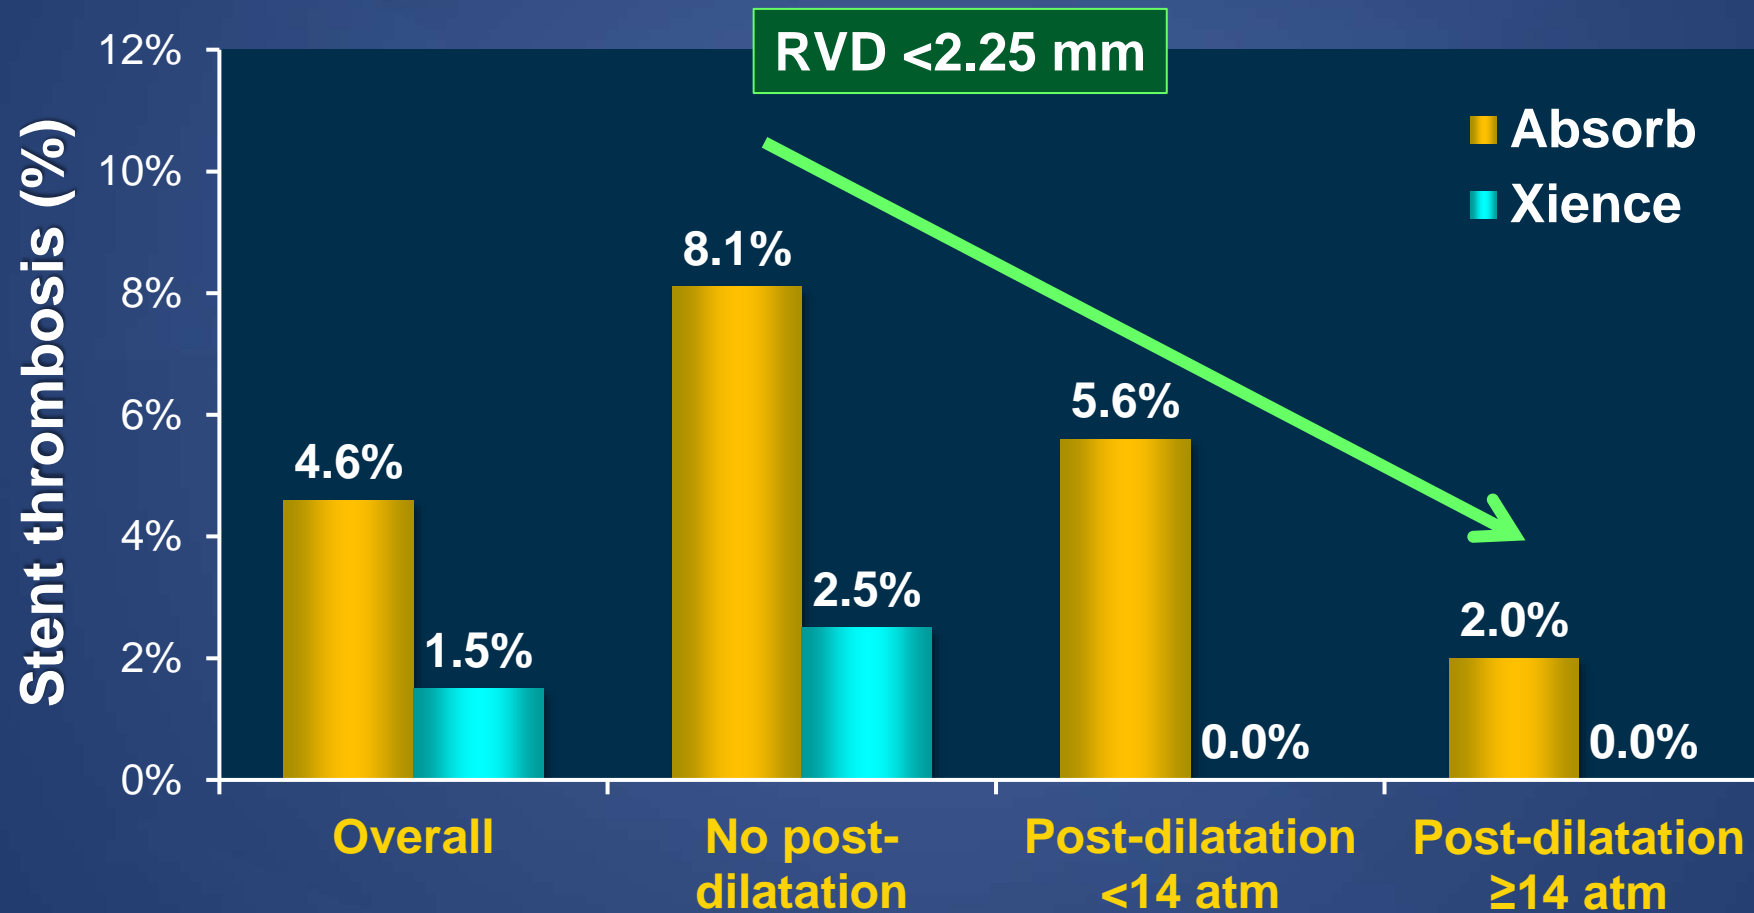


# Why is the high pressure post-dilatation so important? Embedding of struts?

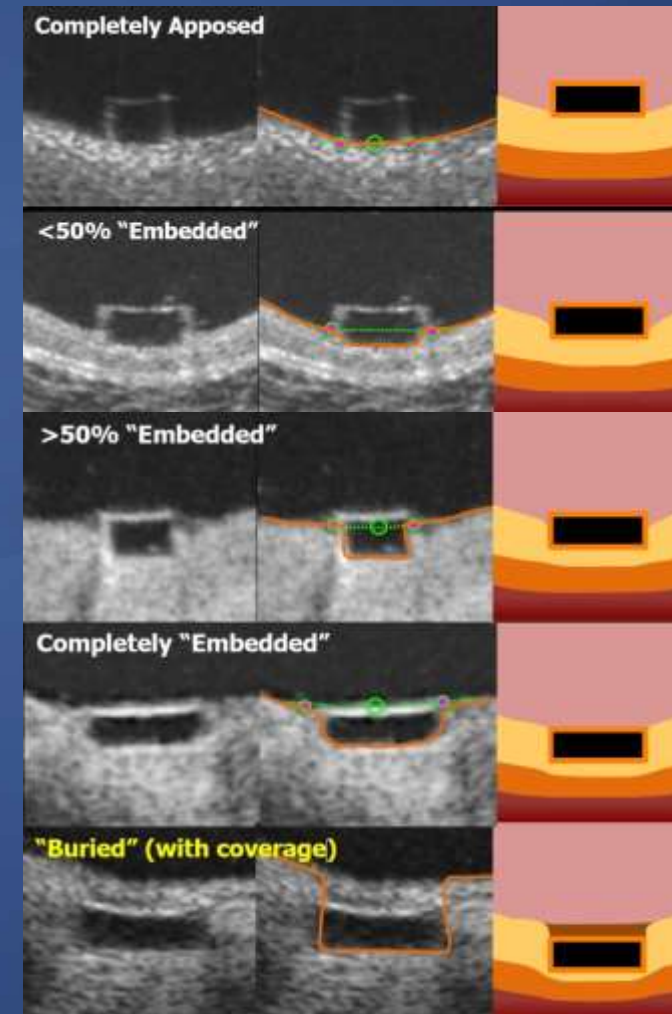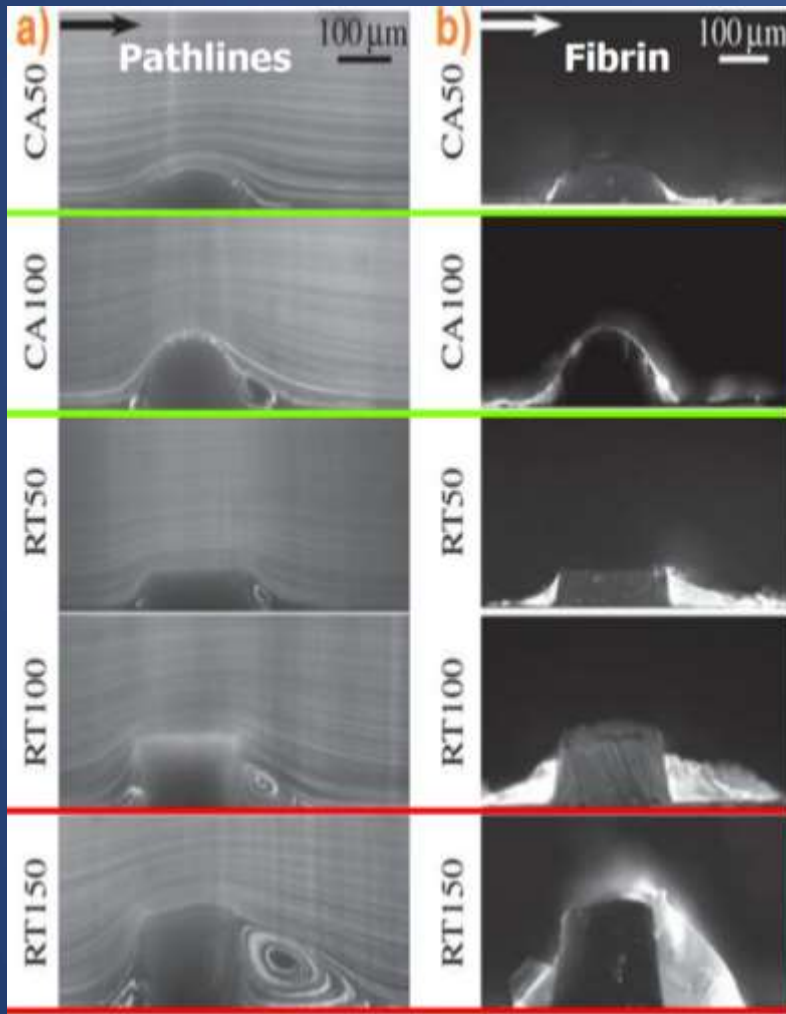

# Small vessel size issue

- A total of 1248 patients received Absorb scaffolds in the ABSORB Cohort B study (n=101), ABSORB EXTEND study (n=812), and ABSORB II trial (n=335)

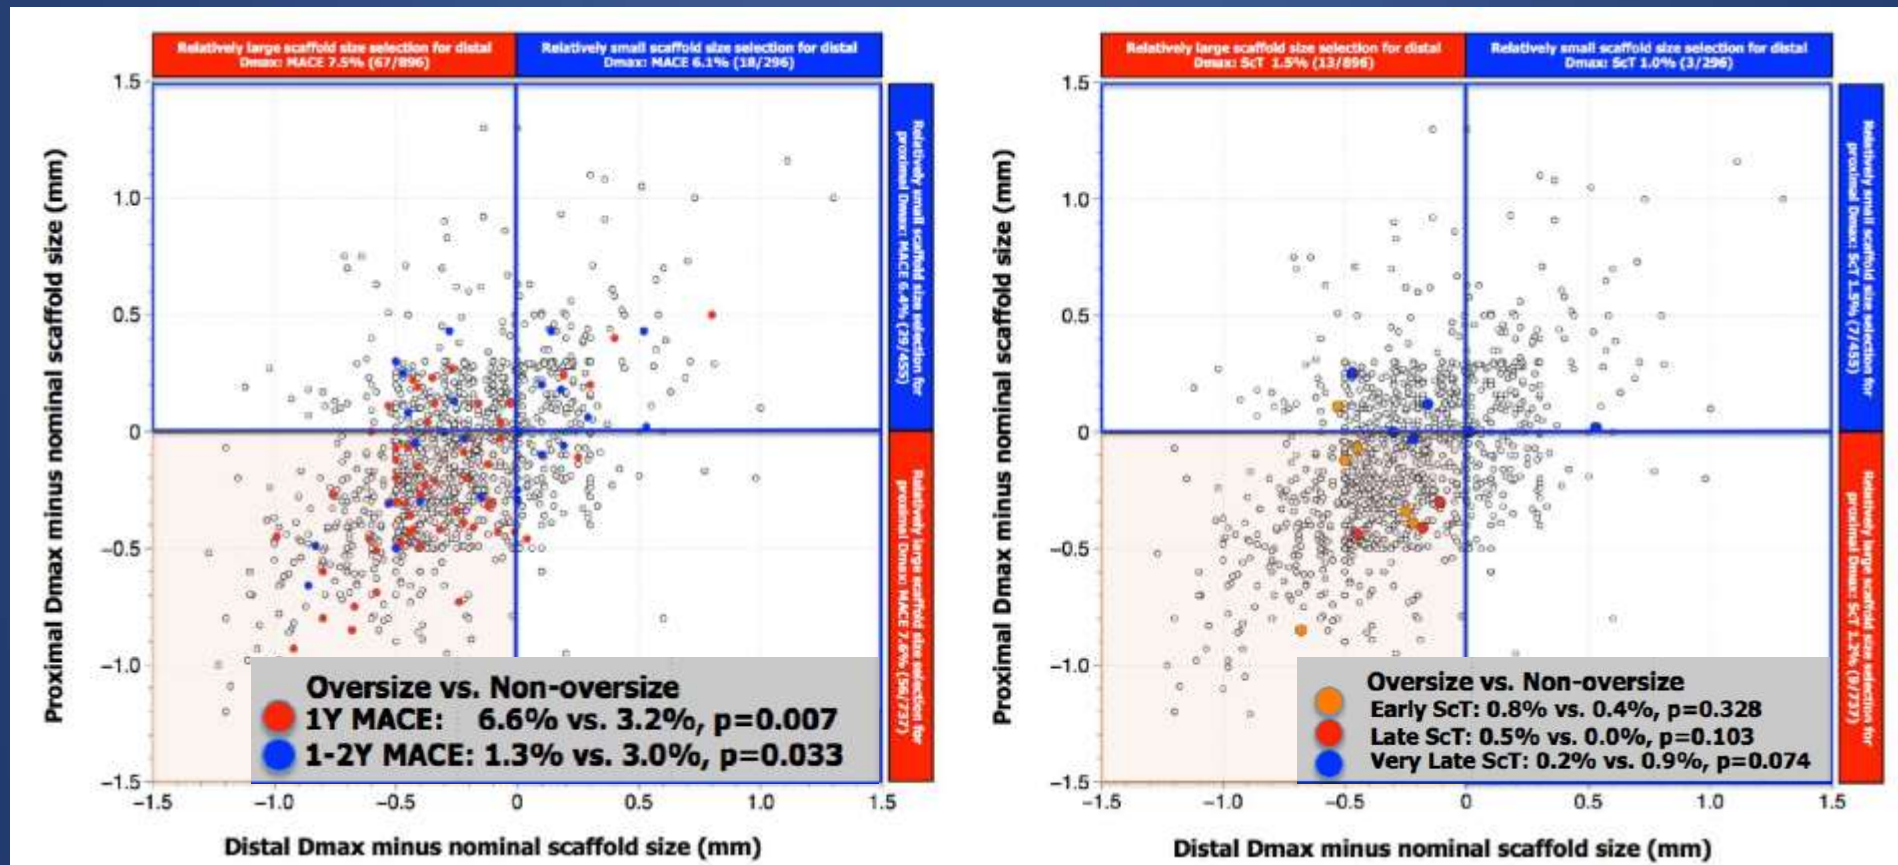

# AMC PSP

## QCA Guided

## IVUS Guided

**P**

**Pre-  
Dilation**

*Pre-dilation* with NC balloon,  
1:1 matched QCA RVD

*Pre-dilation* with NC balloon,  
1:1 matched distal RVD

**S**

**Sizing**

*Absorb*, 1:1 matched  
proximal QCA RVD

*Absorb*, 1:1 matched  
distal RVD

**P**


**Post-  
Dilatation**

*Post-dilation* with NC balloon,  
0.5 mm larger size  
(but  $\leq +0.5\text{mm}$ ,  $>14\text{atm}$ ).

*IVUS guided Post-dilation*  
with NC balloon



# ***BVS QCA vs. Imaging-guided***

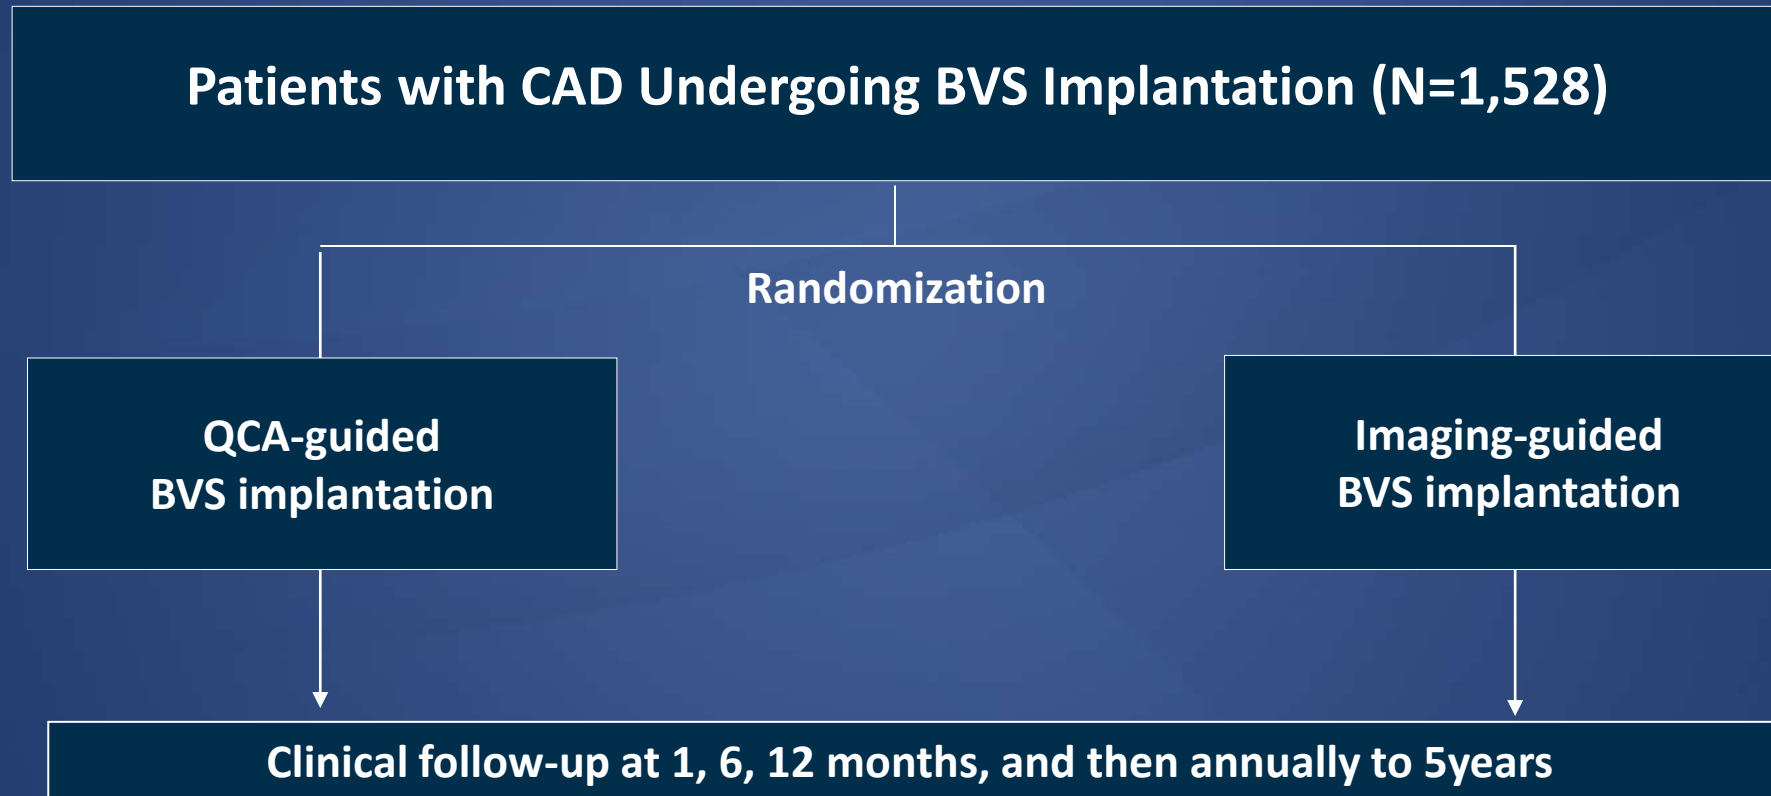

\*Primary endpoint: target-lesion failure (cardiac death, TV-MI, or ID-TLR) at 1 year

# BVS For Long Lesion ( $\geq 40\text{mm}$ )

Everolimus-Eluting Bioresorbable Scaffolds versus Everolimus-Eluting Metallic Stents for Diffuse Long Coronary Artery Disease

## ABSORB-LONG Trial

Patients requiring PCI for diffuse long coronary lesions:  
Lesion length  $\geq 40\text{ mm}$  (by visual estimation) receiving at least 2 overlapped stents  
(Total; 800 Patients)

Stratified randomization by (1) diabetes and (2) clinical site

ABSORB BVS  
(N=400)

XIENCE EES  
(N=400)

Clinical follow-up at 1, 2, 3, 4, and 5 years


\*Primary endpoint: target-lesion failure (composite of cardiac death, TV-MI, or ID-TLR) at 1 year

# ***BVS How Long DAPT?***

Optimal Duration of Antiplatelet Therapy after  
Bioresorbable Vascular Scaffold Implantation  
to Reduce Late Coronary Arterial Thrombotic Events

## **BVS-LATE Trial**

Patients on dual antiplatelet therapy without death, MI, or any revascularization  
During at least the first 12 months after Bioresorbable Vascular Scaffold implantation

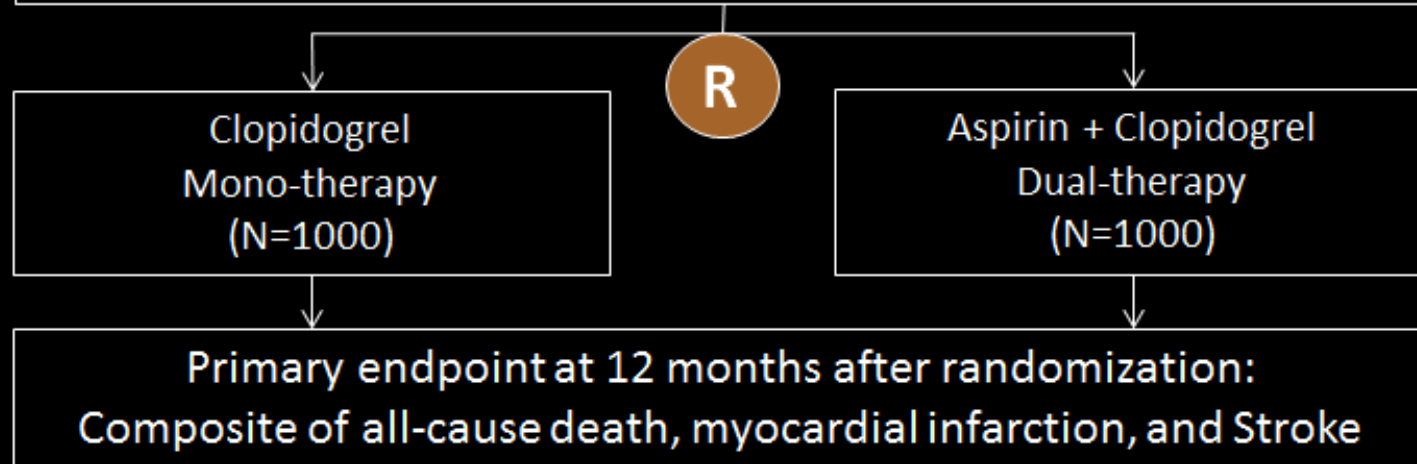

# BVS for AMI patients

Evaluation of effectiveness and safety of BVS  
in Routine Clinical Practice

## IRIS- BVS AMI Registry

Consecutive PCI patients receiving PCI with BVS in treatment of acute myocardial infarction

Patients receiving  
PCI with BVS(Absorb™)  
In acute myocardial infarction  
(N=500)

Patients receiving PCI with DES  
in acute myocardial infarction  
in IRIS-DES registry  
(N=500)

Clinical Follow-Up at 1-, 6-, and 12 months, 3 years, 5 years

Primary end-point: Composite of Death, MI, and TVR at 12 months

# BVS for Variant Angina

BVS Implantation in Patients with Variant Angina and MODerate coronary artery disease:  
Pilot study

## BIVA-MOD: Pilot study

Patients with Variant Angina with Moderate coronary artery disease

- 1) Vasospastic angina diagnosed by provocation test including ergonovine provocation coronary angiography or ergonovine echocardiogram
- 2) No-ischemia producing moderate coronary artery disease (stenosis > 50%, FFR > 0.8)
- 3) No history of previous coronary revascularization
- 4) No organic heart disease associated with myocardial ischemia or sudden cardiac death

Optimal medical treatment +  
BVS implantation  
(N=30)

Primary endpoint at 2 years : Composite of all-cause death,  
myocardial infarction, and angina-related hospitalization


# BVS for Vulnerable Plaque

## PREVENT Trial

*Any Epicardial Coronary Stenosis*

with FFR  $\geq 0.80$  and with Two of the following

1. IVUS MLA  $\leq 4.0\text{mm}^2$
2. IVUS Plaque Burden  $> 70\%$
3. Lipid-Rich Plaque on NIRS ( $_{\text{max}}\text{LCBI}_{4\text{mm}} > 315$ )
4. TCFA defined by OCT or VH-IVUS

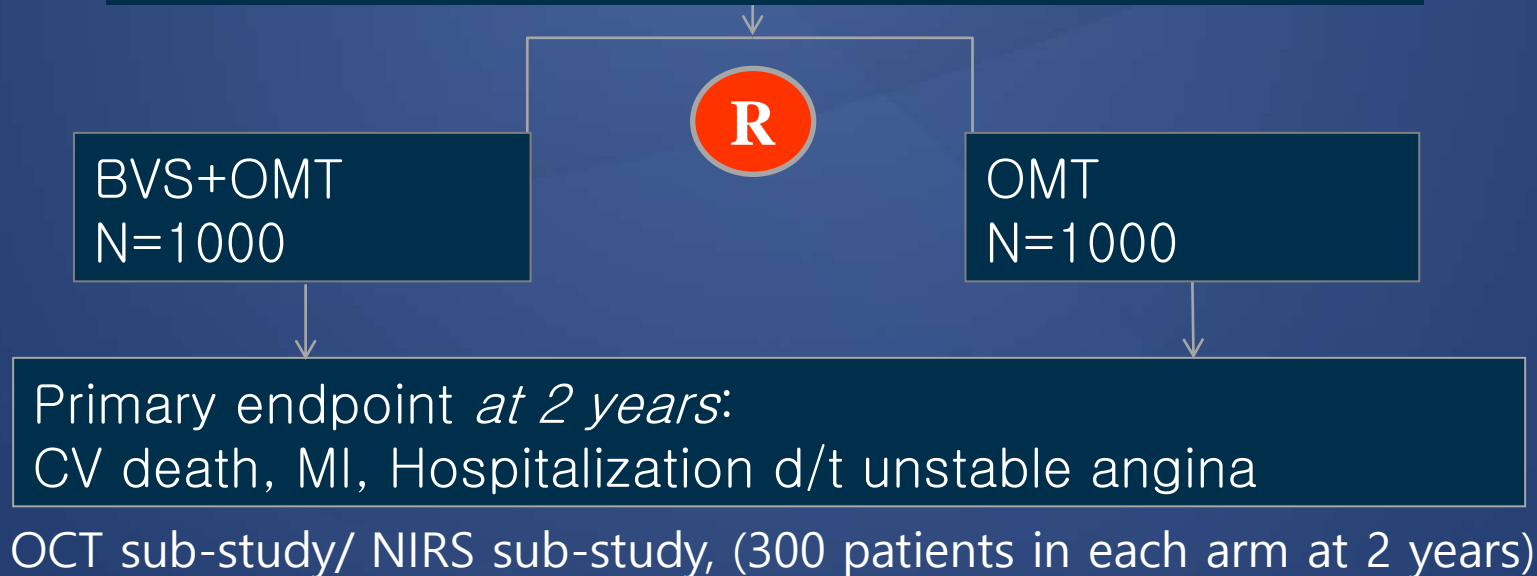




# Limitation of first generation BRS

- Larger catheter profile, reduced deliverability
- Thicker and wider struts than metallic DES
- Narrow expansion limits with risk of acute fracture
- Issues with scaffold visibility, overlap
- Greater recoil in some lesion
- Active bioresorption with risk of very late intraluminal scaffold dismantling

# Hype Cycle for Emerging Technologies

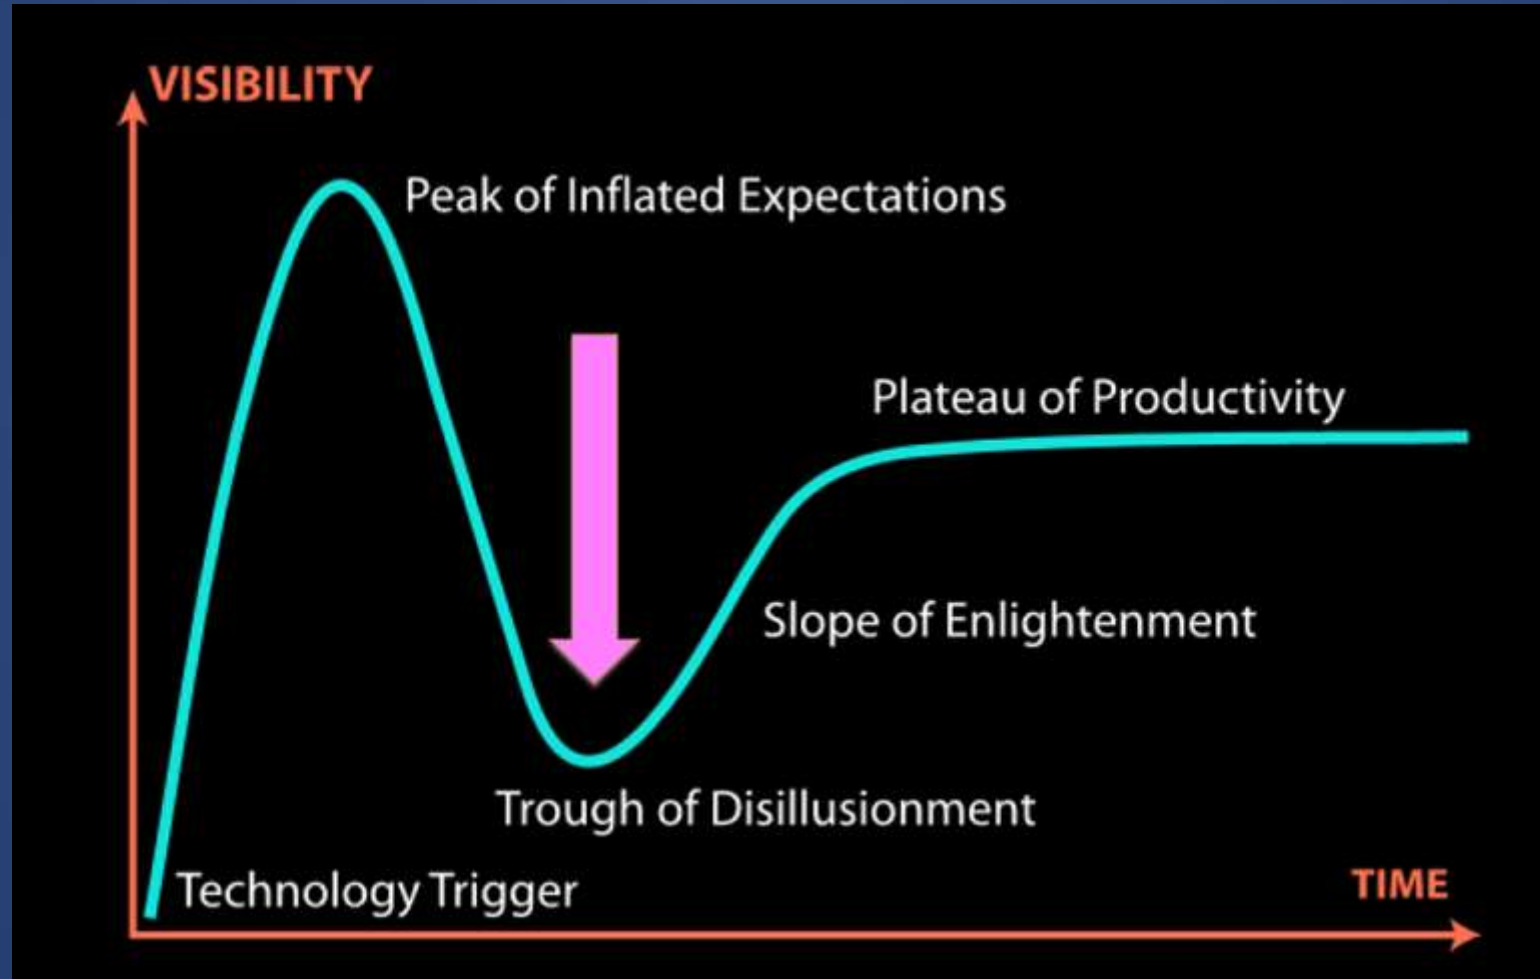


# Strut Thickness in Perspective

## In vivo Thrombogenicity

Joner M, Presented at EuroPCR 2014

### Absorb

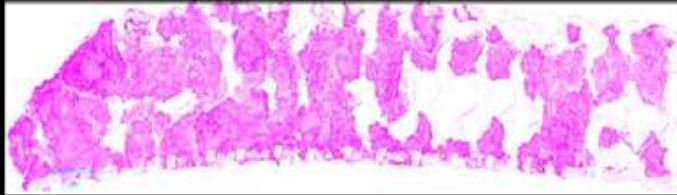


### Synergy



Thrombus formation assessed by immunofluorescence staining for platelet marker CD61 after 1 hour in ex-vivo pig AV shunt model

## Strut Thickness in Perspective

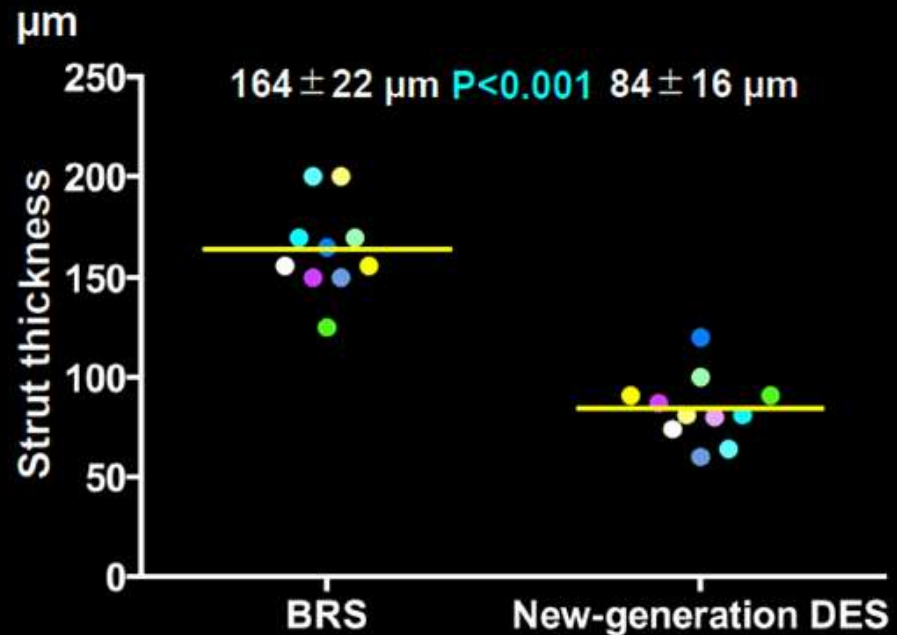

AMS-1 (165 µm), DREAMS-1 (125 µm), DREAMS-2 (150 µm), Igaki-Tamai (170 µm), BVS-1 (156 µm), BVS 1.1 (156 µm), DESolve (150 µm), REVA (200 µm), ART 18AY (170 µm), Ideal BTI (64 µm)

Biomatrix (120 µm), Endeavor (91 µm), Yukon PC (87 µm), Xience (81 µm), Resolute (91 µm), Synergy (74 µm), Orsiro (60 µm), DESyne (81 µm), Combo (100 µm), Mistent (64 µm), Ultimaster (80 µm)

# Structure Summary


*As of today, at least 32 devices have been developed !*





# New BRSs

Basic material	MAGNESIUM			OTHER		
Scaffold name	AMS	DREAMS 1.0	DREAMS 2.0	REVA BRS	REVA ReZolve	Ideal BioStent
Manufacturer	Biotronik, Berlin, Germany	Biotronik, Berlin, Germany	Biotronik, Berlin, Germany	Reva Medical Inc., San Diego, CA, USA	Reva Medical Inc., San Diego, CA, USA	Xenogenics Corp., Canton, MA, USA
Composition	Magnesium and rare earth metals	Magnesium and rare earth metals	Magnesium and rare earth metals	Desaminotyrosine polycarbonate	Desaminotyrosine polycarbonate	Poly-lactic anhydride containing 2 salicylic acid molecules linked to 1 sebacic acid molecule
Design of the latest generation	4-crown design	6-crown design	6-crown design	Slide-and-lock ("ratchet")	Slide-and-lock ("ratchet")	Tube with laser-cut voids
Thickness of strut, $\mu\text{m}$	165	120	150	204	122	200
Visualization	Latest generation with radiopaque markers			Fully radiopaque	Fully radiopaque	--
Special feature	Electronegative charge that emerges during degradation process has an antithrombotic function			--	--	Polymer causes less inflammation
Anti-proliferative drug elution	No	Paclitaxel	Sirolimus	Paclitaxel	Sirolimus	Sirolimus
Resorption time	2 mos	9–12 mos	--	2–3 yrs	2–3 yrs	15 mos
Status	Clinical evaluation	Clinical evaluation	Clinical evaluation	Clinical evaluation; CE trial ongoing	Clinical evaluation; CE trial ongoing	Clinical evaluation, pre-clinical evaluation of the thinner 2nd generation
Trials (no. in cohort and duration)	PROGRESS AMS 63 patients up to 28 mos	BIOSOLVE-I 46 patients up to 3 yrs	BIOSOLVE-II -- --	FIM -- 15 mos	RESTORE 26 patients 12 mos	FIM 11 patients 1.5 yrs

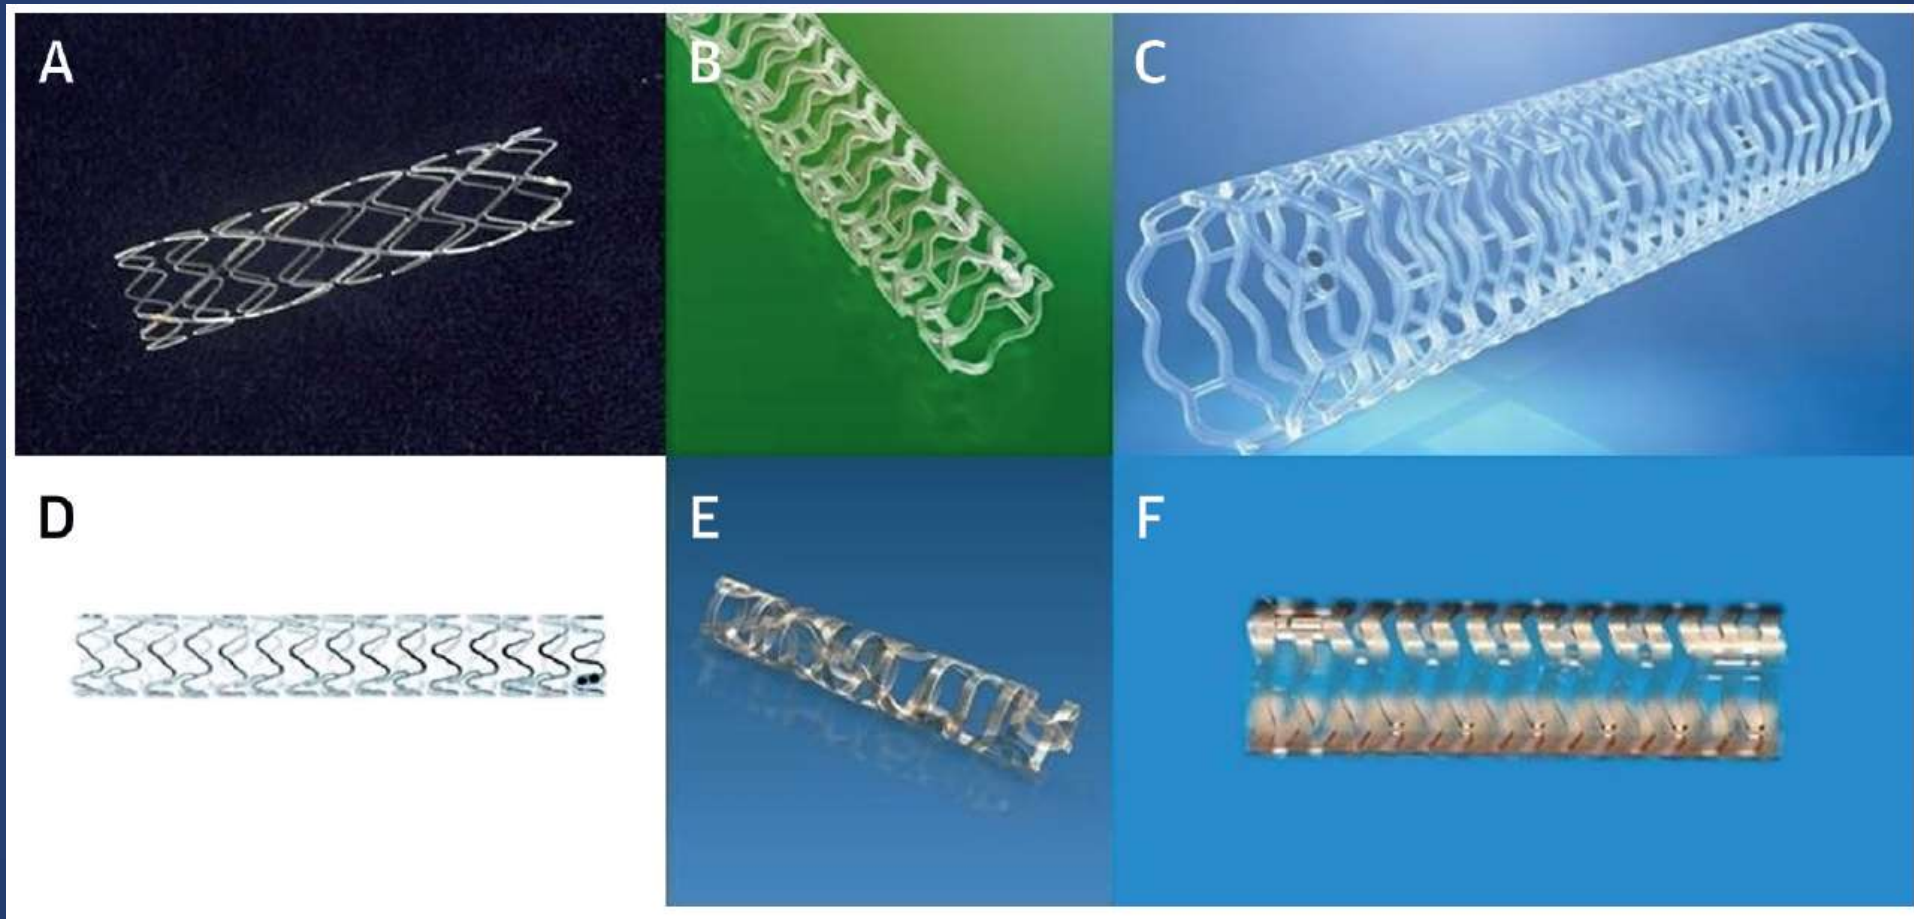

- (A) The Igaki-Tamai stent (Kyoto Medical Planning Co., Ltd., Kyoto, Japan)
- (B) The ABSORB Bioresorbable Vascular Scaffold (Abbott Vascular, Santa Clara, California)
- (C) The DESolve bioresorbable scaffold (Elixir Medical Corporation, Sunnyvale, California)
- (D) The DREAMS magnesium alloy (Biotronik, Berlin, Germany)
- (E) The ReZolve 2 BRS (Reva Medical Inc., San Diego, California)
- (F) The Ideal BioStent (Xenogenics Corp., Canton, Massachusetts)



# FANTOM II


## *Fantom Bioresorbable Scaffold*




***Fantom***<sup>®</sup> (REVA Medical)  
Sirolimus-Eluting Bioresorbable Scaffold  
Desaminotyrosine Polycarbonate

### Key Scaffold Features


- Complete scaffold visibility under x-ray
- Single-step continuous inflation
- Clinically significant expansion range
- Good radial strength at 125  $\mu$ m thickness
- Vasomotion restoration ~1 year (Preclinical)
- No special storage or handling

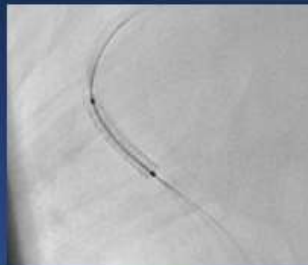

*Visibility*



*Deliverability*




*Vessel Patency*

# FANTOM II

## FANTOM II Study Design and Endpoints

- **Study Design**



- Safety and Performance Trial
- 2.5mm to 3.5mm vessels
- Lesion length  $\leq 20$ mm
- Primary Endpoint
  - MACE & Late Loss at 6 Months
- Secondary Endpoints
  - MACE all time points
  - Late Loss at 9 Months
  - Serial imaging sub-studies
    - Cohort A: 24 months
    - Cohort B: 48 months

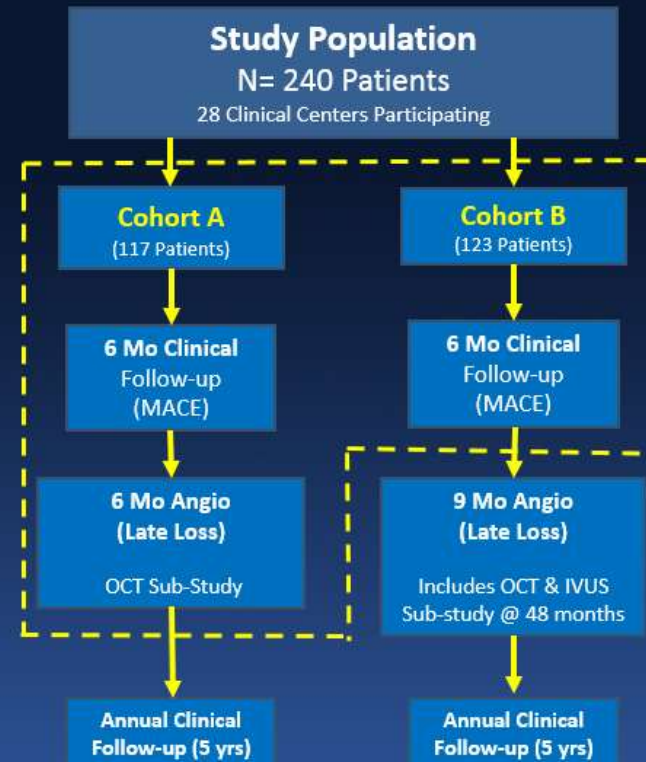

# FANTOM II

## Scaffold Lumen Area

PCI Research  
Aarhus University Hospital

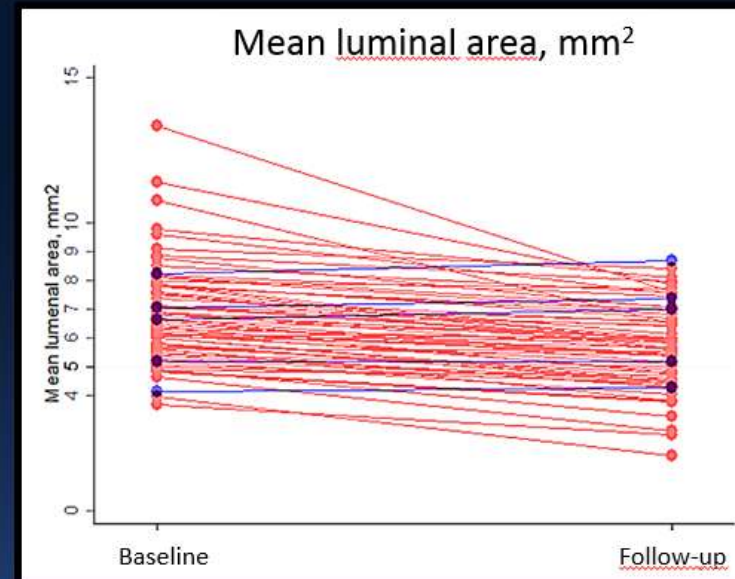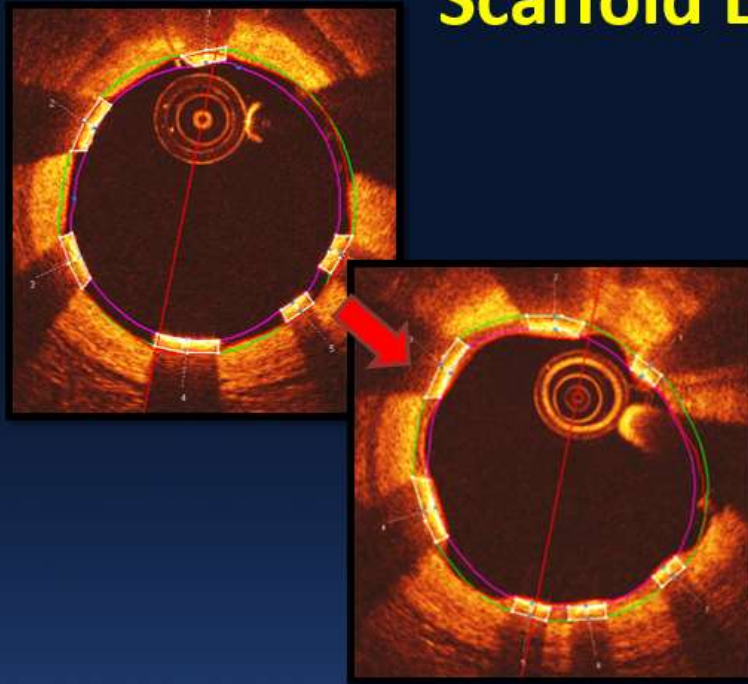

	Baseline	Follow-up	Difference	p-value
Mean lumen area (mm <sup>2</sup> )	6.8 (1.7)	5.7 (1.4)	-1.1 (-1.3;-0.9)	<0.0001
Minimal lumen area (mm <sup>2</sup> )	5.3 (1.4)	4.4 (1.4)	-1.0 (-1.3;-0.7)	<0.0001



Mean(SD)



# FANTOM II

## Scaffold Lumen Area

PCI Research  
Aarhus University Hospital

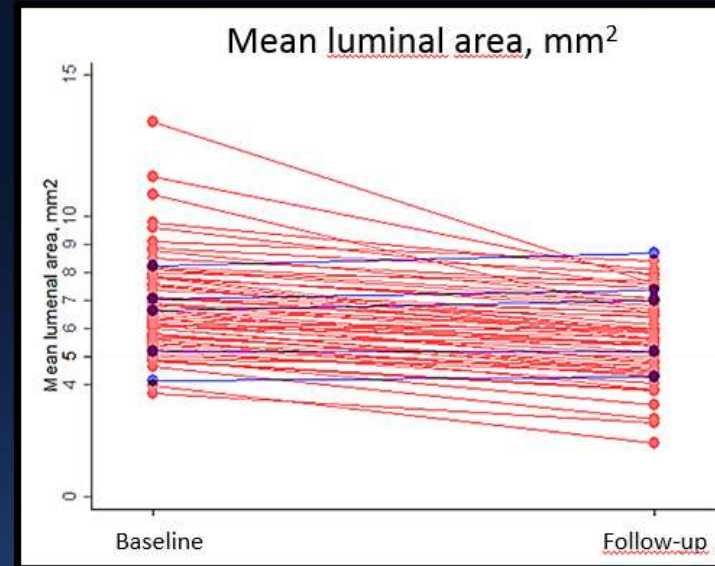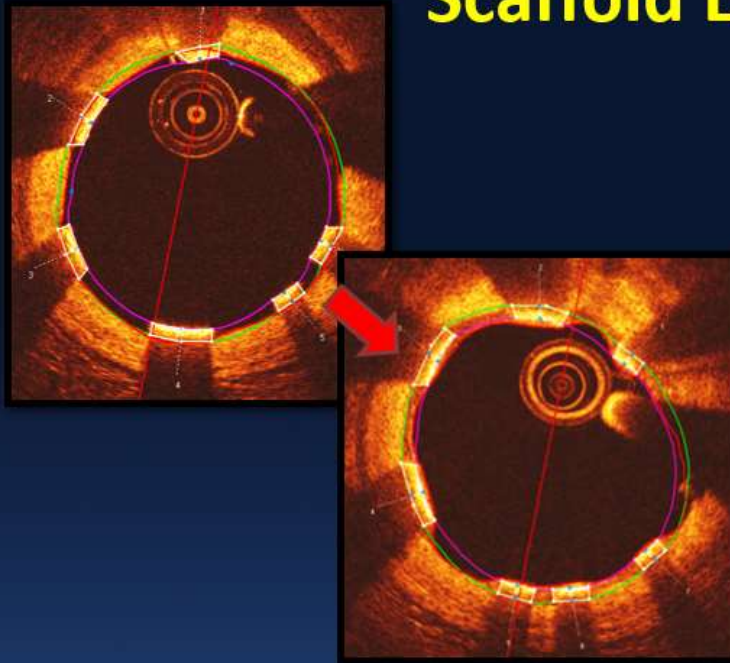



	Baseline	Follow-up	Difference	p-value
Mean lumen area (mm <sup>2</sup> )	6.8 (1.7)	5.7 (1.4)	-1.1 (-1.3;-0.9)	<0.0001
Minimal lumen area (mm <sup>2</sup> )	5.3 (1.4)	4.4 (1.4)	-1.0 (-1.3;-0.7)	<0.0001

Mean(SD)

# FANTOM II

PCI Research  
Aarhus University Hospital

## Strut Coverage

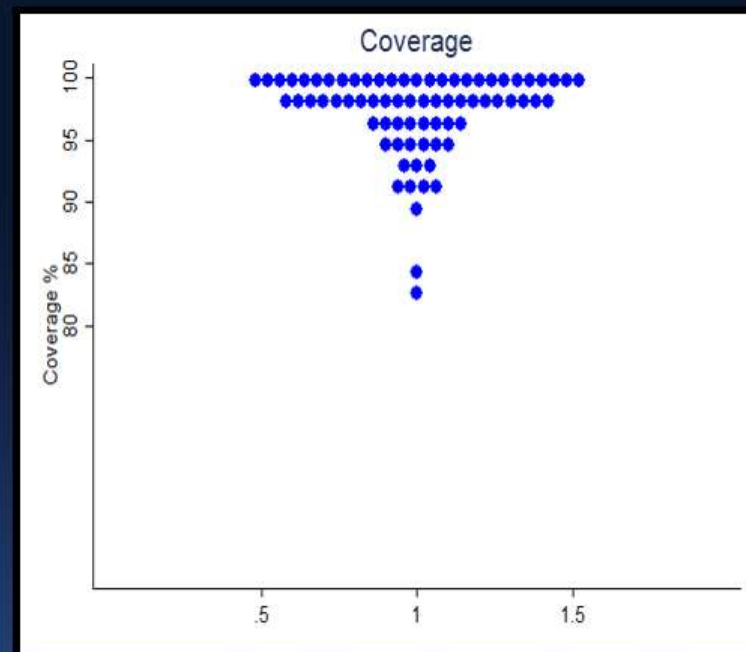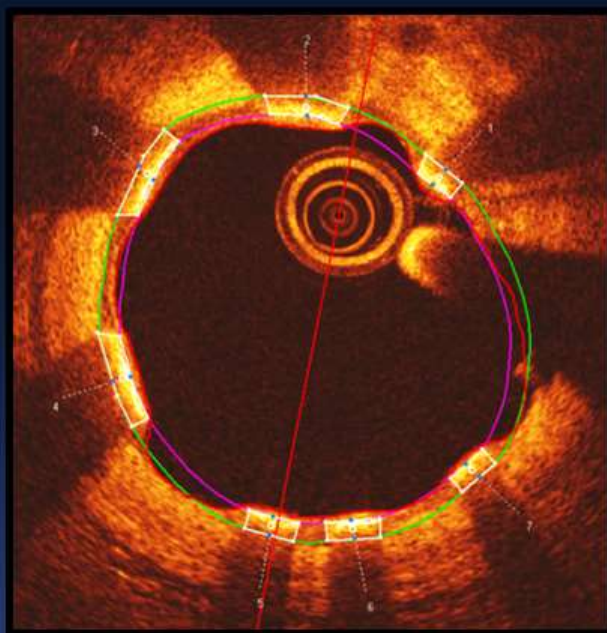

### Follow-up


Covered struts

98.1% (95.9;99.4)

Median(IQR)

# MeRes-1

## MeRes100 (developed in INDIA) Sirolimus Eluting Bioresorbable Vascular Scaffold

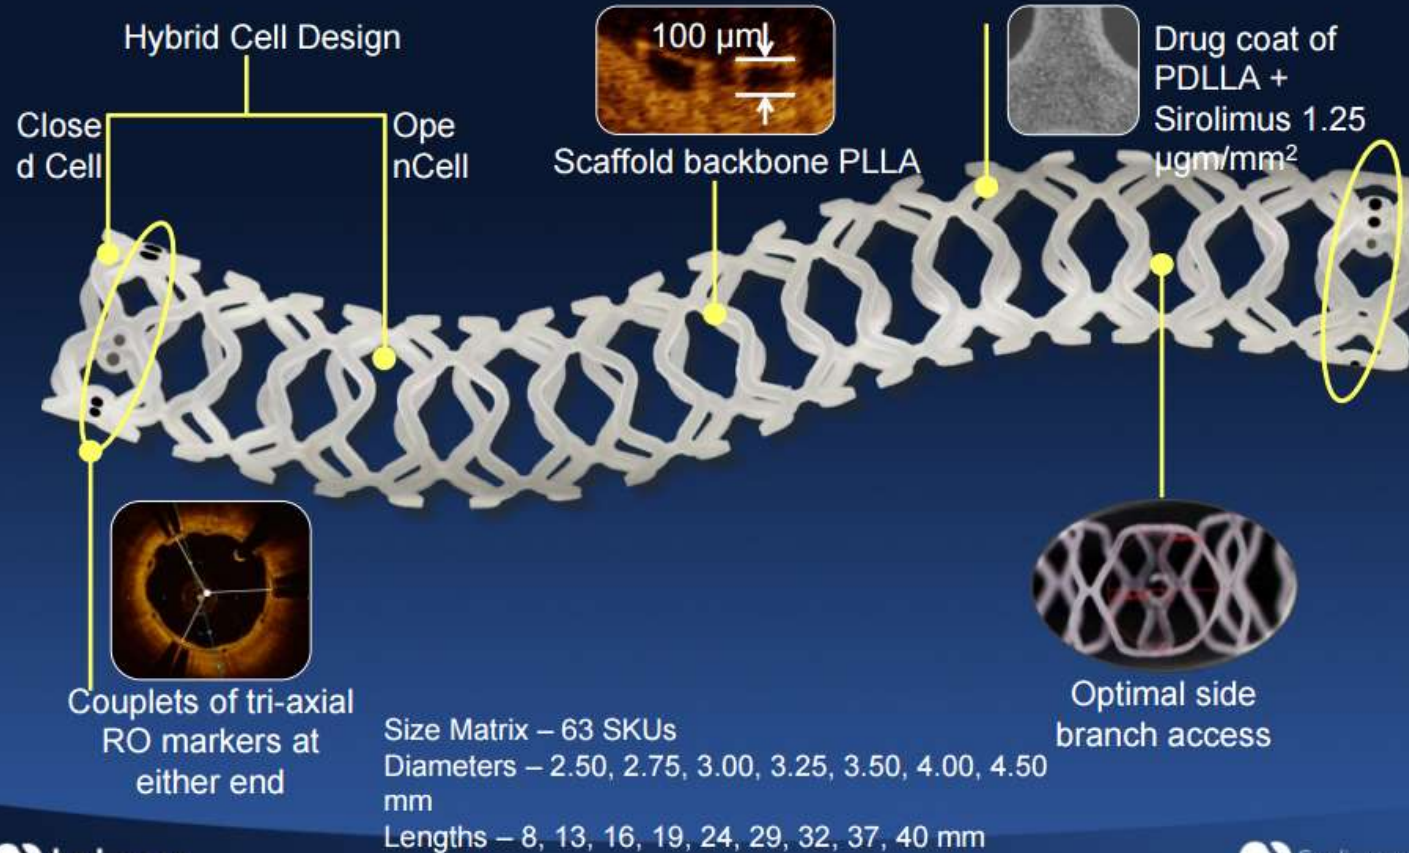



# MeRes-1

## MeRes-1 Study Design



**First-in-man Safety and Efficacy** in Patients with Single, De-novo Coronary Lesion (in up to 2 vessels) treated by a Single MeRes100 Scaffold up to 24mm length **in 108 pts**



\*QCA, IVUS, OCT & MSCT follow-up

CLINICAL FOLLOW-UP	108	108	108	108	108
ANGIOGRAPHIC FOLLOW-UP	-	36	-	36	-
OCT FOLLOW-UP	-	13	-	13	-
IVUS FOLLOW-UP	-	12	-	12	-
MSCT FOLLOW-UP	-	-	12	-	-

Diameters – 2.75, 3.00, and 3.50 mm

DAPT Rx 1 year

Length – 19 and 24 mm




\* Pre-designated sites & patients consent. Regulatory approval study in India.




# MeReS-1

## Late Lumen Loss at 6-Month FU

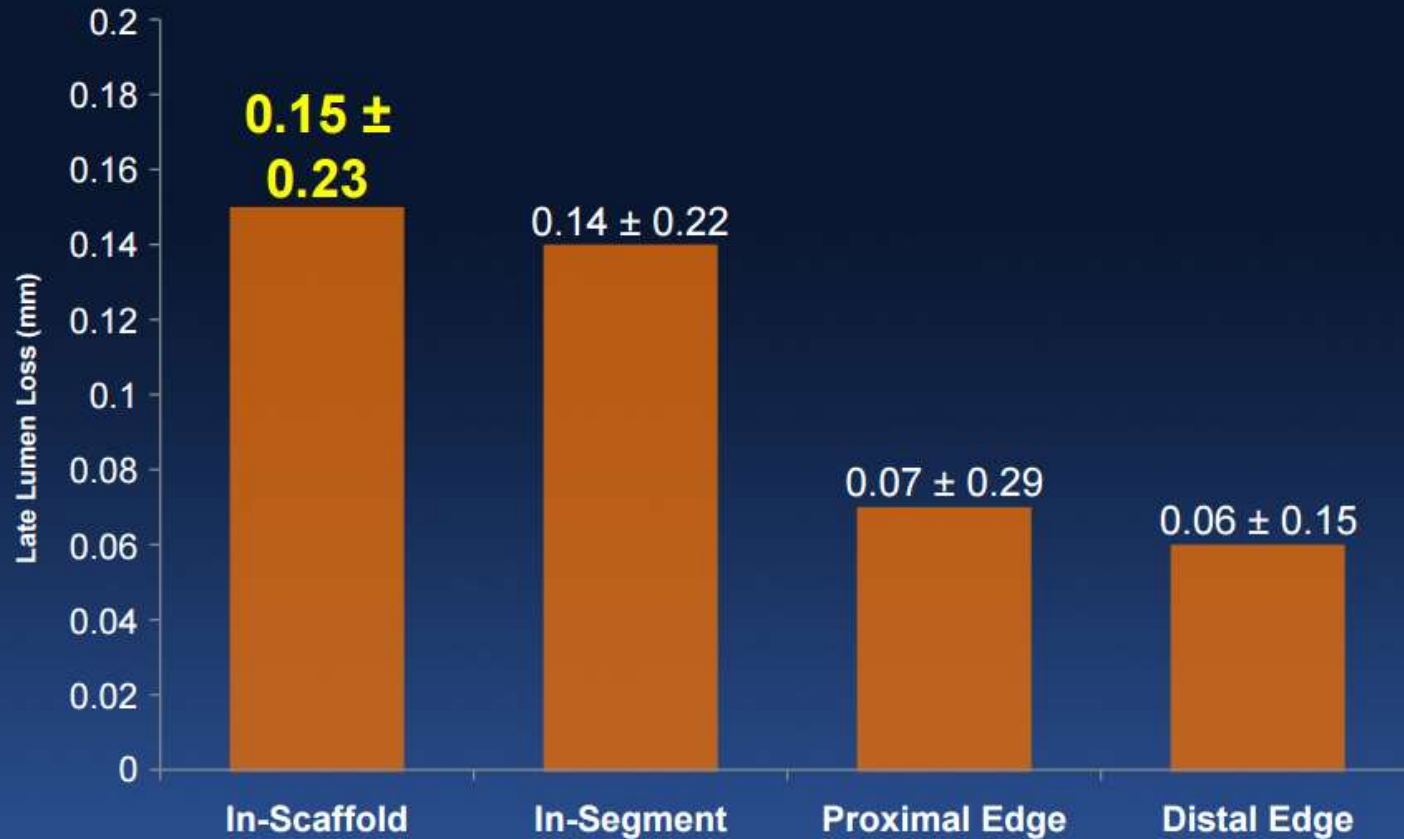

# MeReS-1


## CFD Curve for Late Lumen Loss at 6-Months FU

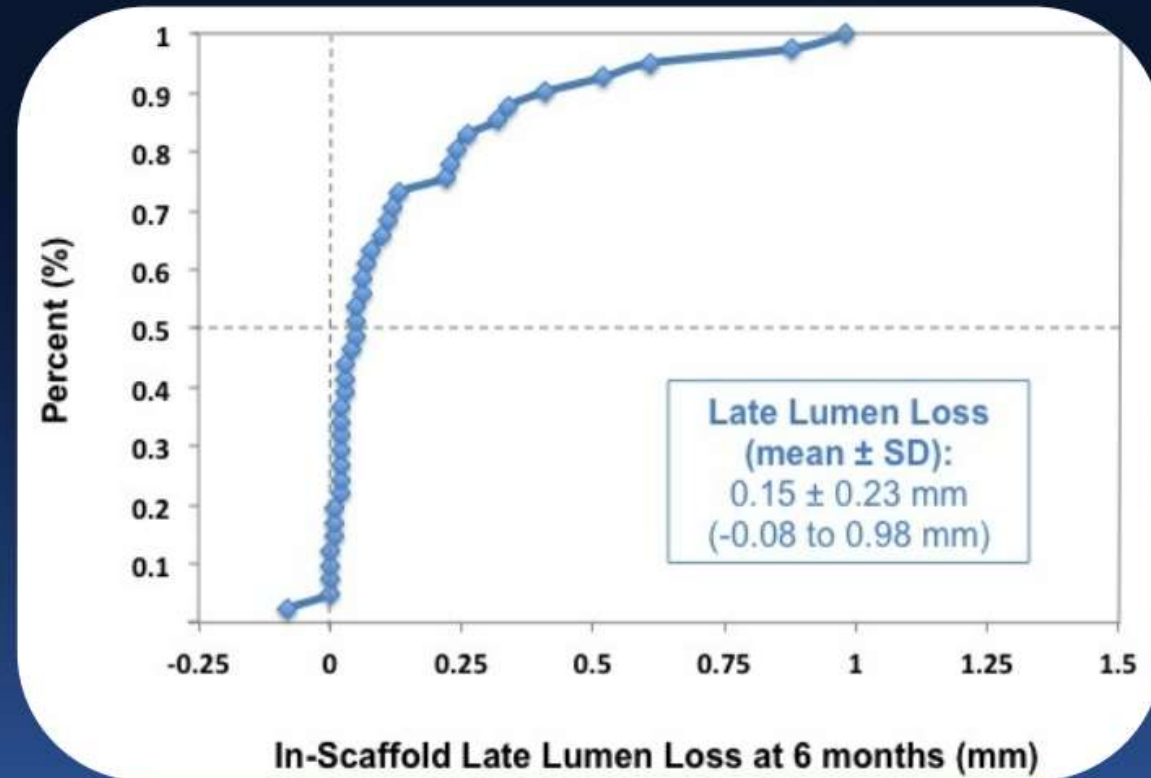

# FORTITUDE

## 1-Year Clinical and Imaging Outcomes of a Novel Ultra High Molecular Weight PLLA Sirolimus-Eluting Coronary BRS: A Prospective Multicenter International Investigation (The FORTITUDE® Study)


### FORTITUDE Study Design

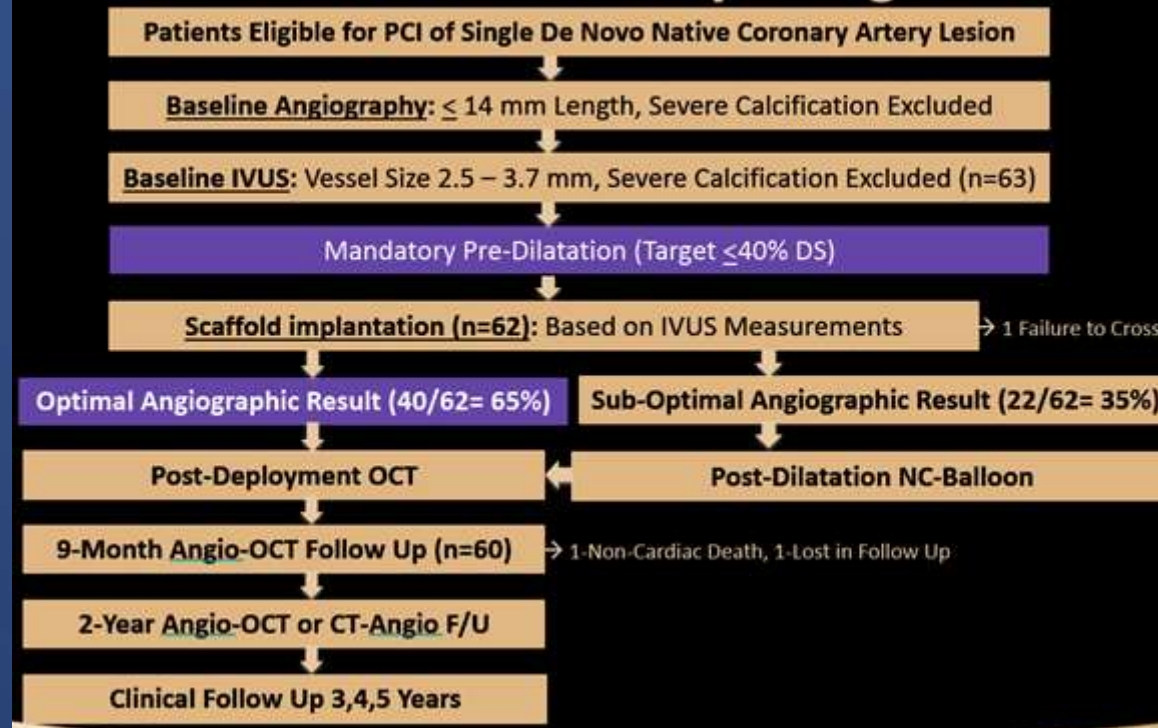



# FORTITUDE


## Primary Efficacy End Point: Cumulative Frequency Distribution 9-Month In-Scaffold Late Lumen Loss

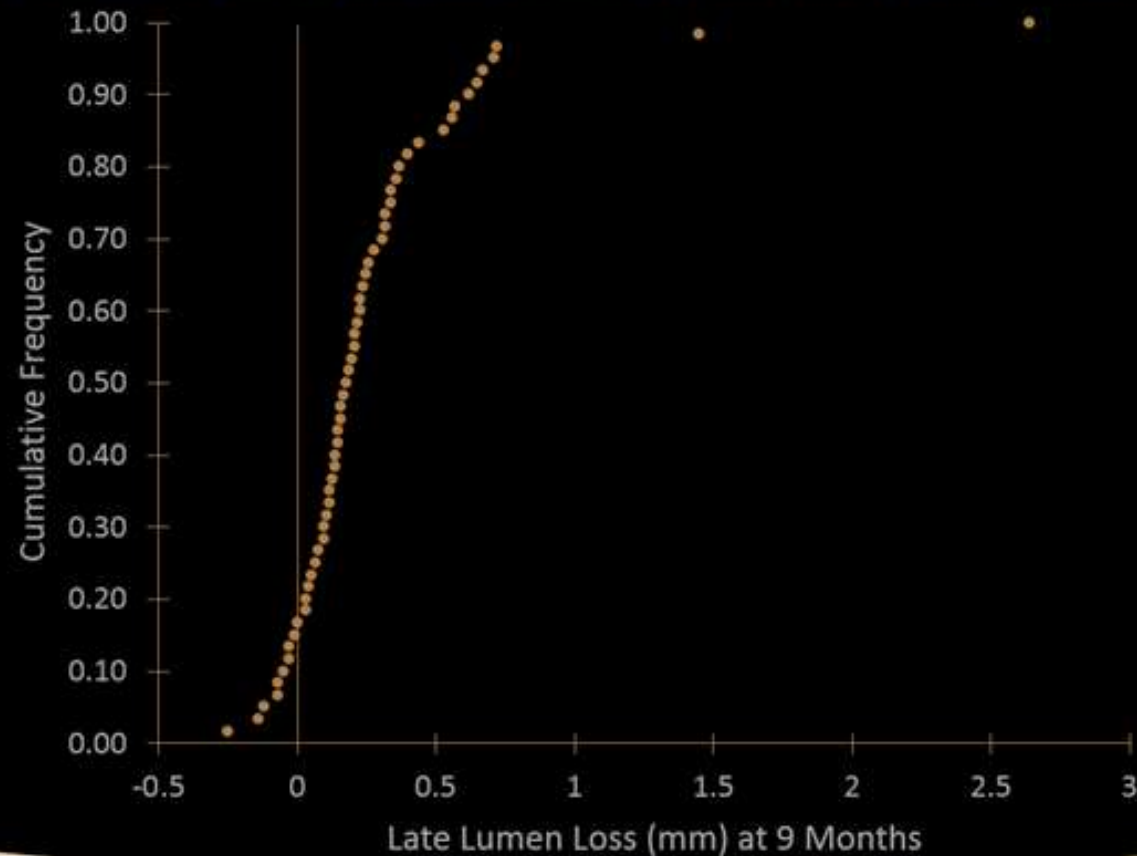

# FUTURE-I

## Features of the Firesorb BRS

### PLLA-based BRS

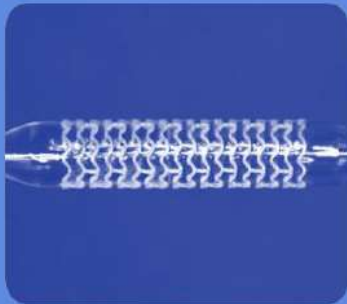

- PLLA backbone
- PDLLA coating
- Balloon Expandable

### Abluminal Eluting



- Abluminal coating
- Sirolimus
- Low drug dosage - 60% lower than BVS

### Thin Strut

Scaffold Size	Strut Thickness
2.5 ~ 2.75 mm	100 $\mu$ m
3.0 ~ 4.0 mm	125 $\mu$ m

- Lower crossing profile
- Shorter resorption time
- More deliverable



# FUTURE-I

## FUTURE-I (N=45)

Prospective, Single Center, First-in-Man Study

- Inclusion:**
- Age  $\geq 18$  years
  - Stable and unstable angina, silent ischemia, or OMI
  - Single, *de novo* lesion in native coronary artery with lesion length  $\leq 25$  mm (can be covered by 1 scaffold) and vessel size between 3.0~3.5 mm

- Exclusion:**
- AMI within 1 week
  - CTO (TIMI 0), left main disease, ostial lesion, multivessel disease, bifurcation (diameter of ostial SB  $\geq 2.0$  mm or %DS  $\geq 40\%$ ), and restenotic lesions

**Device Size:** Diameter: 3.0, 3.25, 3.5 mm; length: 13, 18, 23, 29 mm

### Imaging and Clinical Follow-up



# FUTURE-I

## Angiographic Results in Cohort 1

	Post-Procedure (N=30)	6M F/U (N=29)	Difference (95% CI)	P
Minimal Lumen Diameter, mm				
In-Scaffold	2.67 ± 0.22	2.53 ± 0.24	0.15 (0.11, 0.19)	<0.001
In-Segment	2.44 ± 0.27	2.36 ± 0.30	0.09 (0.03, 0.14)	0.003
Diameter Stenosis, %				
In-Scaffold	10.6 ± 4.7	14.1 ± 5.9	-3.5 (-5.4, -1.6)	0.001
In-Segment	15.4 ± 7.5	16.9 ± 8.7	-1.1 (-4.1, 1.9)	0.45
Acute Gain, mm				
In-Scaffold	1.67 ± 0.42	-	-	-
In-Segment	1.44 ± 0.48	-	-	-
Acute Recoil, mm	0.13 ± 0.10	-	-	-
Late Lumen Loss, mm				
In-Scaffold	-	0.15 ± 0.11	-	-
In-Segment	-	0.09 ± 0.15	-	-
Binary Restenosis, %	-	0%	-	-

# FUTURE-I

## Clinical Outcomes

	30 Days			6 Months		
	Overall (N=45)	Cohort 1 (N=30)	Cohort 2 (N=15)	Overall (N=45)	Cohort 1 (N=30)	Cohort 2 (N=15)
TLF	0% (0)	0% (0)	0% (0)	0% (0)	0% (0)	0% (0)
PoCE	2.2% (1)	3.3% (1)	0% (0)	2.2% (1)	3.3% (1)	0% (0)
All-Cause Death	0% (0)	0% (0)	0% (0)	0% (0)	0% (0)	0% (0)
Cardiac Death	0% (0)	0% (0)	0% (0)	0% (0)	0% (0)	0% (0)
Non-Cardiac Death	0% (0)	0% (0)	0% (0)	0% (0)	0% (0)	0% (0)
All MI	2.2% (1)	3.3% (1)	0% (0)	2.2% (1)	3.3% (1)	0% (0)
Target Vessel MI	0% (0)	0% (0)	0% (0)	0% (0)	0% (0)	0% (0)
Any Revascularization	2.2% (1)	3.3% (1)	0% (0)	2.2% (1)	3.3% (1)	0% (0)
ID-TVR	0% (0)	0% (0)	0% (0)	0% (0)	0% (0)	0% (0)
ID-TLR	0% (0)	0% (0)	0% (0)	0% (0)	0% (0)	0% (0)
Def/Prob ST	0% (0)	0% (0)	0% (0)	0% (0)	0% (0)	0% (0)



# FUTURE-I

## IVUS Results in Cohort 1

	Post-Procedure (N=30)	6M F/U (N=29)	Difference (95% CI)	P
<b>Cross-Section Level Analysis</b>	<b>1,365</b>	<b>1,227</b>	-	-
Mean Vessel Area, mm <sup>2</sup>	16.4 ± 3.49	16.2 ± 3.30	0.4 (-0.1, 1.0)	0.12
Minimal Vessel Area, mm <sup>2</sup>	13.6 ± 3.61	13.3 ± 3.21	0.5 (0.2, 0.8)	0.003
Mean Scaffold Area, mm <sup>2</sup>	7.87 ± 1.25	7.86 ± 1.25	0.1 (-0.1, 0.2)	0.37
Minimal Scaffold Area, mm <sup>2</sup>	6.74 ± 1.17	6.70 ± 1.21	0.1 (-0.1, 0.3)	0.41
Mean Lumen Area, mm <sup>2</sup>	7.68 ± 1.21	7.47 ± 1.27	0.3 (0.1, 0.5)	0.01
Minimal Lumen Area, mm <sup>2</sup>	6.60 ± 1.15	6.30 ± 1.22	0.4 (0.1, 0.6)	0.005
<b>Lesion Level Analysis</b>	<b>30</b>	<b>29</b>	-	-
Mean Neointimal Hyperplasia, mm <sup>2</sup>	-	0.18 ± 0.22	-	-
In-Scaffold Volumetric Obstruction, %	-	6.46 ± 2.57	-	-
Absolute Late Recoil, mm <sup>2</sup>	-	0.07 ± 0.39	-	-
Late Recoil, %	-	0.76 ± 4.86	-	-

# FUTURE-I

## OCT Results in Cohort 1

	Post- Procedure (N=30)	6M F/U (N=29)	Difference (95% CI)	P
<b>Strut Level Analysis</b>	<b>13,843</b>	<b>14,945</b>	-	-
Proportion of Covered Struts, %	-	98.4%	-	-
Incomplete Strut Apposition, %	0.85%	0.07%	0.82 (0.37, 1.27)	<0.001
Persistent Malapposition, %	-	0.07%	-	-
Late-Acquired Malapposition, %	-	0%	-	-
Mean Thickness of Strut Coverage, mm	-	0.05 ± 0.04	-	-
<b>Cross-Section Level Analysis</b>	<b>1,402</b>	<b>1,372</b>	-	-
Mean Black Core Area, mm <sup>2</sup>	0.13 ± 0.02	0.14 ± 0.03	-0.01 (-0.02, 0.0)	0.01
<b>Lesion Level Analysis</b>	<b>30</b>	<b>29</b>	-	-
Absolute Late Recoil, mm <sup>2</sup>	-	0.18 ± 0.44	-	-
Late Recoil, %	-	2.01 ± 5.20	-	-
Healing Score	-	3.14 ± 3.43	-	-



# XINSORB




*Balloon  
expanding*

- *Excellent deliverability*




*Bioresorbabl  
e Scaffold*

- *Polylactide (PLLA)*
- *Naturally resorbed, fully metabolized*
- *160  $\mu\text{m}$  of thickness*

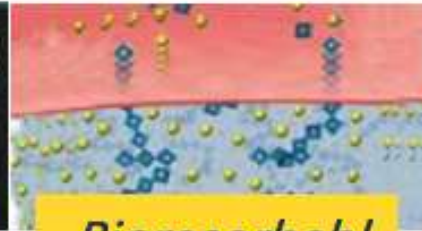

*Bioresorbabl  
e Coating*

- *Polylactide (PDLLA) coating*
- *Fully biodegradabl  
e*

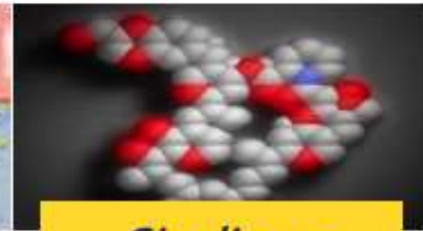

*Sirolimus*

- *12  $\mu\text{g}/\text{mm}$*
- *80% of drugs eluted in 28 days ex vivo*

# XINSORB

## 1-year QCA Results (per lesion)

	XINSORB (N=169)	TIVOLI® (N=167)	P-Value
RVD (mm) prox-	3.02 ± 0.47	3.02 ± 0.56	0.99
in-device	2.88 ± 0.46	2.88 ± 0.53	0.91
distal-	2.71 ± 0.50	2.64 ± 0.52	0.22
MLD (mm) prox-	2.82 ± 0.49	2.70 ± 0.62	0.06
in-device	2.42 ± 0.46	2.35 ± 0.51	0.16
distal-	2.56 ± 0.51	2.46 ± 0.55	0.07
DS (%) prox-	6.45 ± 8.35	11.69 ± 14.4	<0.01
in-device	15.88 ± 9.8	19.05 ± 14.8	0.02
distal-	5.13 ± 8.6	8.1 ± 13.2	0.02
In-device late luminal loss (mm)	0.23 ± 0.29	0.37 ± 0.38	<0.01
Peri-device late luminal loss (mm)	0.19 ± 0.32	0.31 ± 0.41	<0.01

# XINSORB

## 1-year Clinical Outcomes (per patient)

	XINSORB (N=191)	TIVOLI® (N=187)	P-Value
PoCE	4.7% (9)	7.0% (13)	0.35
DoCE (TLF)	1.6% (3)	4.8% (9)	0.07
All-cause death	1.0% (2)	0	0.50
- Cardiac death	0.5% (1)	0	NA
All MI*	0.5% (1)	1.1% (2)	0.62
- TV-MI*	0.5% (1)	0.5% (1)	1.0
All revascularization	3.7% (7)	6.4% (12)	0.22
- ID-TLR	1.0% (2)	4.9% (9)	0.25